

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040621\
 Data File : PP034705.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2021 16:28
 Operator : DD\AJ
 Sample : M1936-01 4X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEE066K-END-1

Manual Integrations
 APPROVED

Ankita
 4/7/2021 4:47:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:45:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.844	4.255	412482	253861	5.407	5.651
2)	SA Decachlor...	10.768	9.560	472237	169802	6.135m	6.014
Target Compounds							
26)	L6 AR-1254-1	7.062	6.375	131143	91144	47.696	49.403
27)	L6 AR-1254-2	7.291	6.532	377459	82011	88.769	51.261 #
28)	L6 AR-1254-3	7.672	6.952	272123	147592	59.621	59.137
29)	L6 AR-1254-4	7.969	7.188	265365	84299	85.827	64.128 #
30)	L6 AR-1254-5	8.394	7.616	284434	158620	80.036	78.044

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040621\
Data File : PP034705.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2021 16:28
Operator : DD\AJ
Sample : M1936-01 4X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:45:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

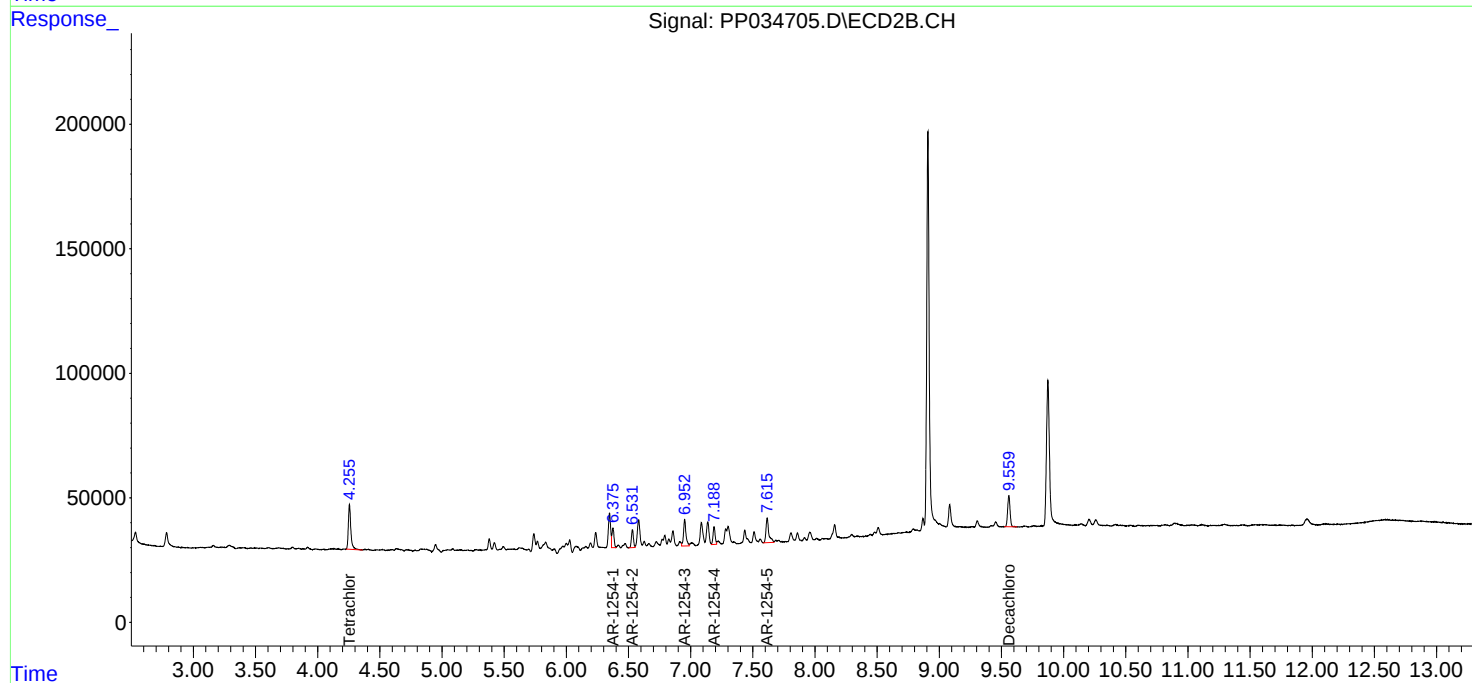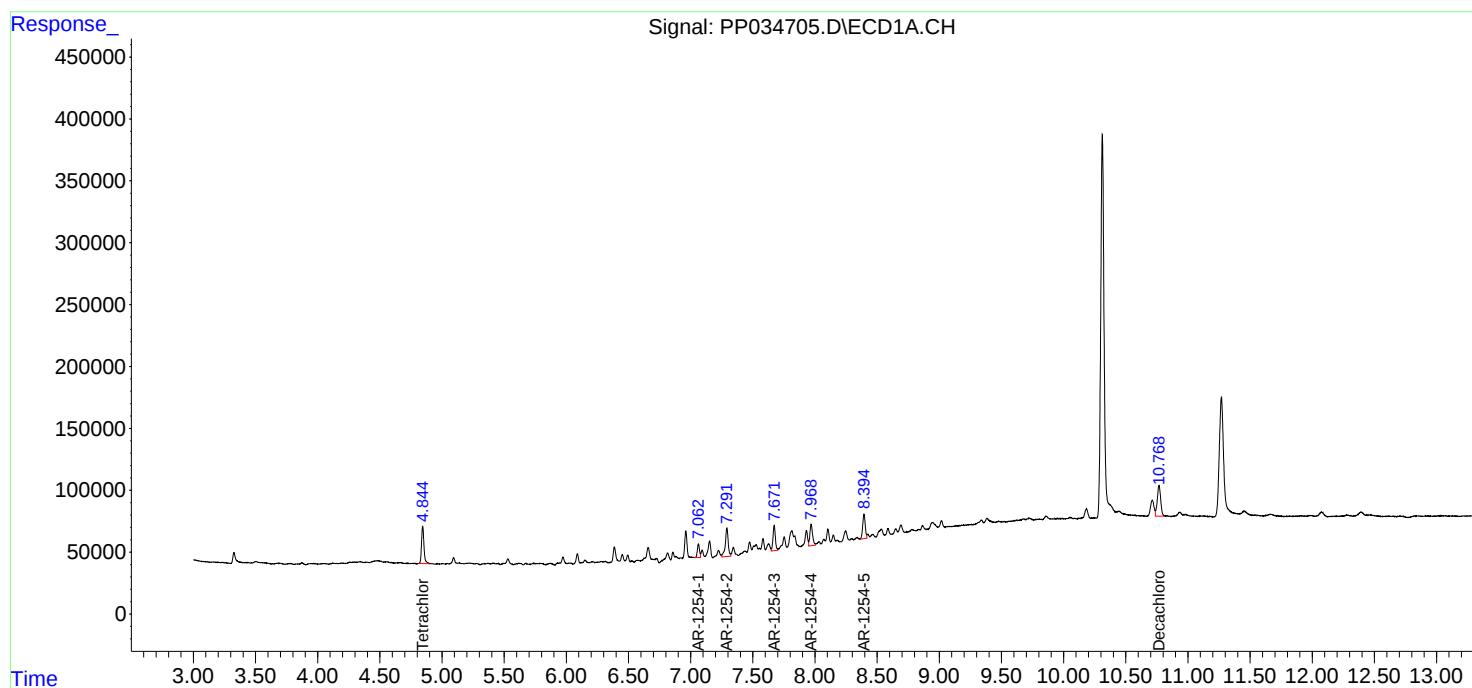

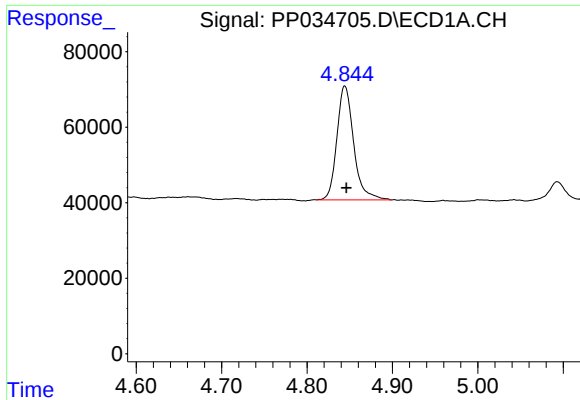


#1 Tetrachloro-m-xylene

R.T.: 4.844 min
Delta R.T.: -0.002 min
Response: 412482
Conc: 5.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:36 PM

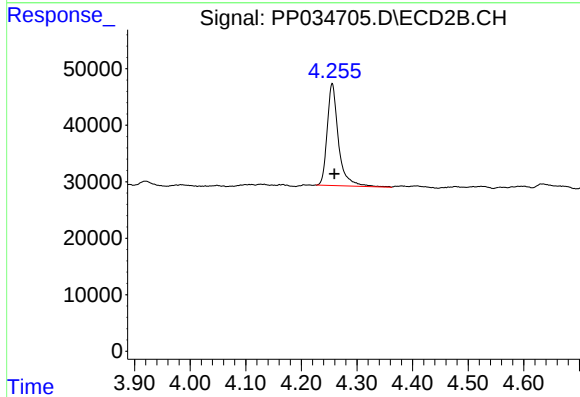


#1 Tetrachloro-m-xylene

R.T.: 4.255 min
Delta R.T.: -0.004 min
Response: 253861
Conc: 5.65 ng/ml

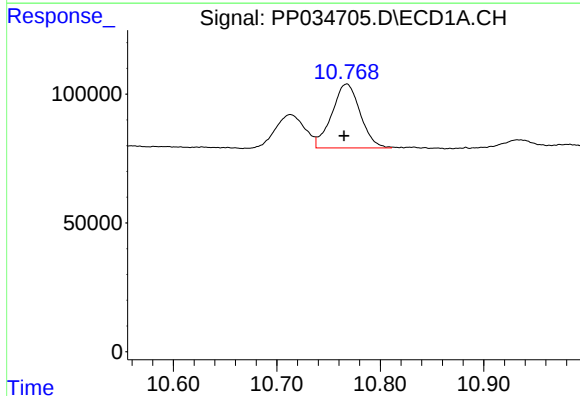


#2 Decachlorobiphenyl

R.T.: 10.768 min
Delta R.T.: 0.002 min
Response: 472237
Conc: 6.13 ng/ml m

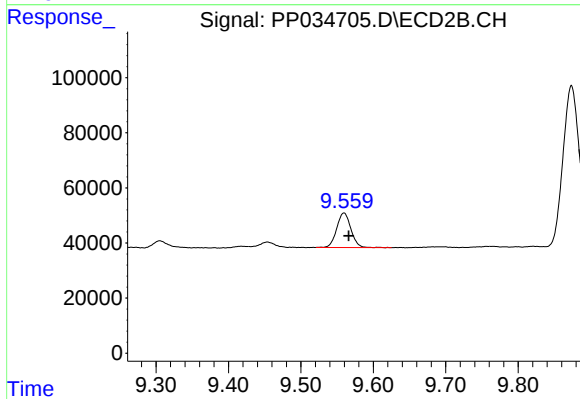

#2 Decachlorobiphenyl

R.T.: 9.560 min
Delta R.T.: -0.007 min
Response: 169802
Conc: 6.01 ng/ml

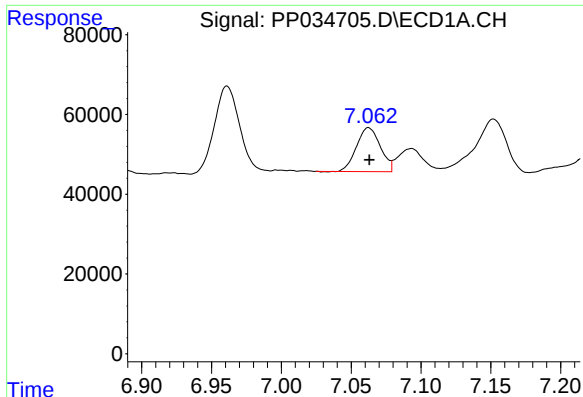


#26 AR-1254-1

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 131143
Conc: 47.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:36 PM

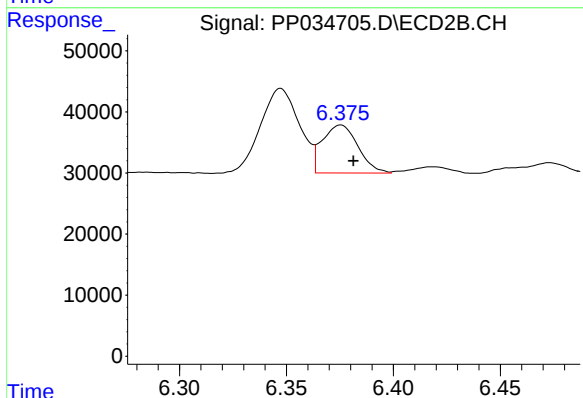


#26 AR-1254-1

R.T.: 6.375 min
Delta R.T.: -0.006 min
Response: 91144
Conc: 49.40 ng/ml

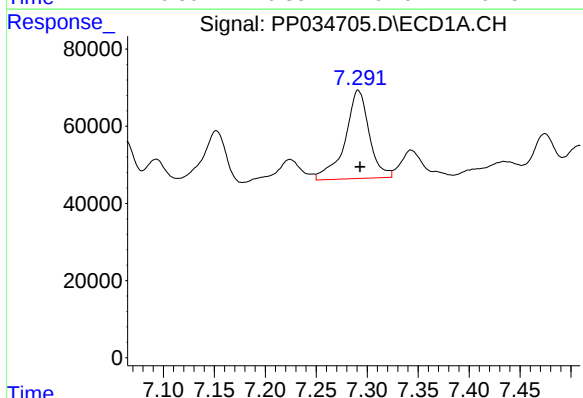


#27 AR-1254-2

R.T.: 7.291 min
Delta R.T.: -0.002 min
Response: 377459
Conc: 88.77 ng/ml

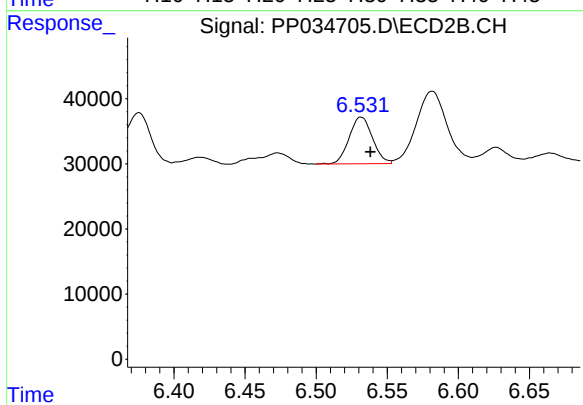

#27 AR-1254-2

R.T.: 6.532 min
Delta R.T.: -0.006 min
Response: 82011
Conc: 51.26 ng/ml

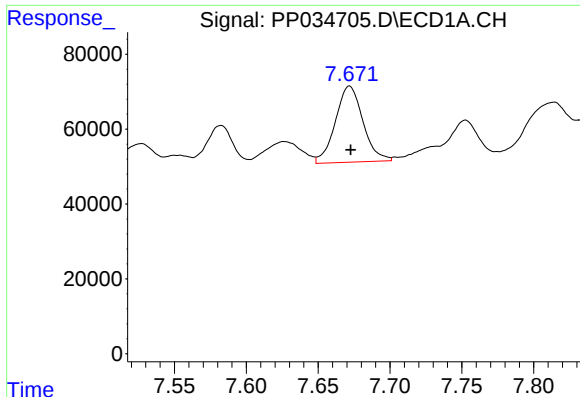


#28 AR-1254-3

R.T.: 7.672 min
Delta R.T.: 0.000 min
Response: 272123
Conc: 59.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:36 PM

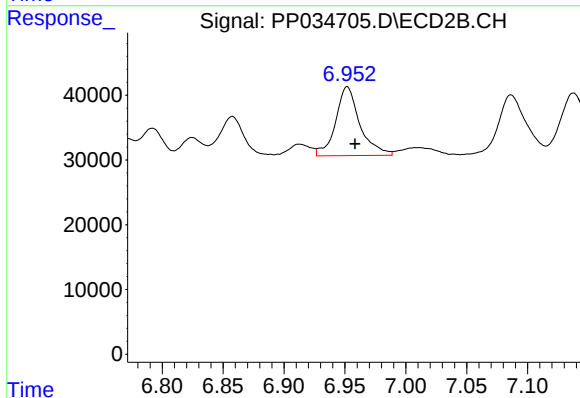


#28 AR-1254-3

R.T.: 6.952 min
Delta R.T.: -0.007 min
Response: 147592
Conc: 59.14 ng/ml

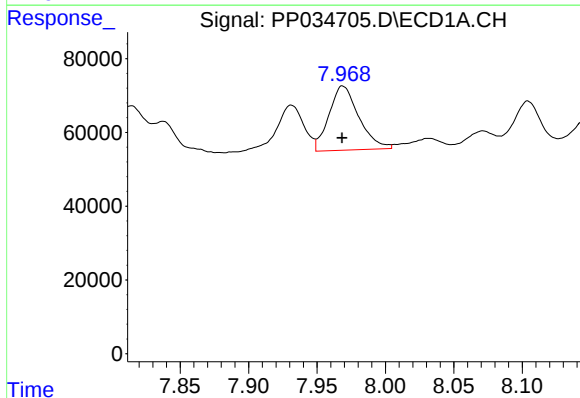


#29 AR-1254-4

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 265365
Conc: 85.83 ng/ml

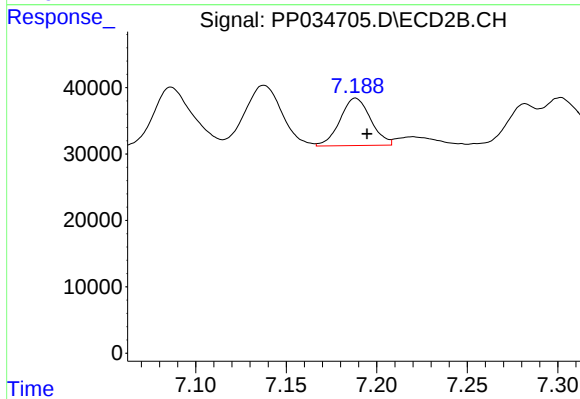

#29 AR-1254-4

R.T.: 7.188 min
Delta R.T.: -0.006 min
Response: 84299
Conc: 64.13 ng/ml

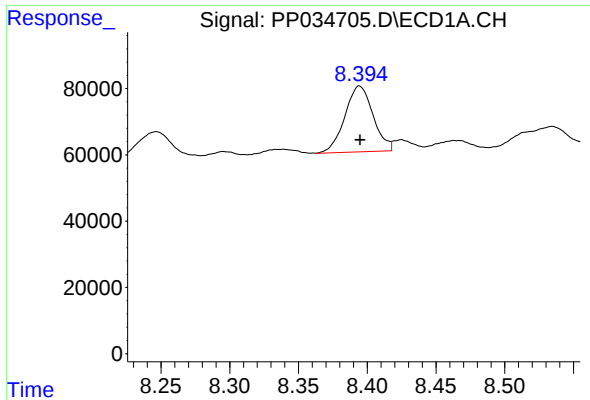


#30 AR-1254-5

R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 284434
Conc: 80.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1

Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:36 PM

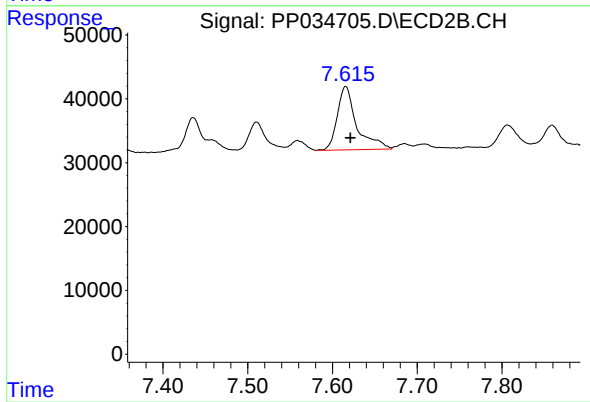

#30 AR-1254-5

R.T.: 7.616 min
Delta R.T.: -0.006 min
Response: 158620
Conc: 78.04 ng/ml