

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040622\
 Data File : PP045565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2022 13:44
 Operator : YP\AJ
 Sample : N2236-03RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RO-VNJ-204RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/07/2022
 Supervised By :mohammad ahmed 04/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:47:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 31 07:54:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.901	3.175f	39446254	22975325	16.349	14.520m
2) SA Decachlor...	9.996	8.493	32971671	30463659	23.012m	20.089m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040622\
Data File : PP045565.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2022 13:44
Operator : YP\AJ
Sample : N2236-03RE
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RO-VNJ-204RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2022
Supervised By :mohammad ahmed 04/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:47:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 31 07:54:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

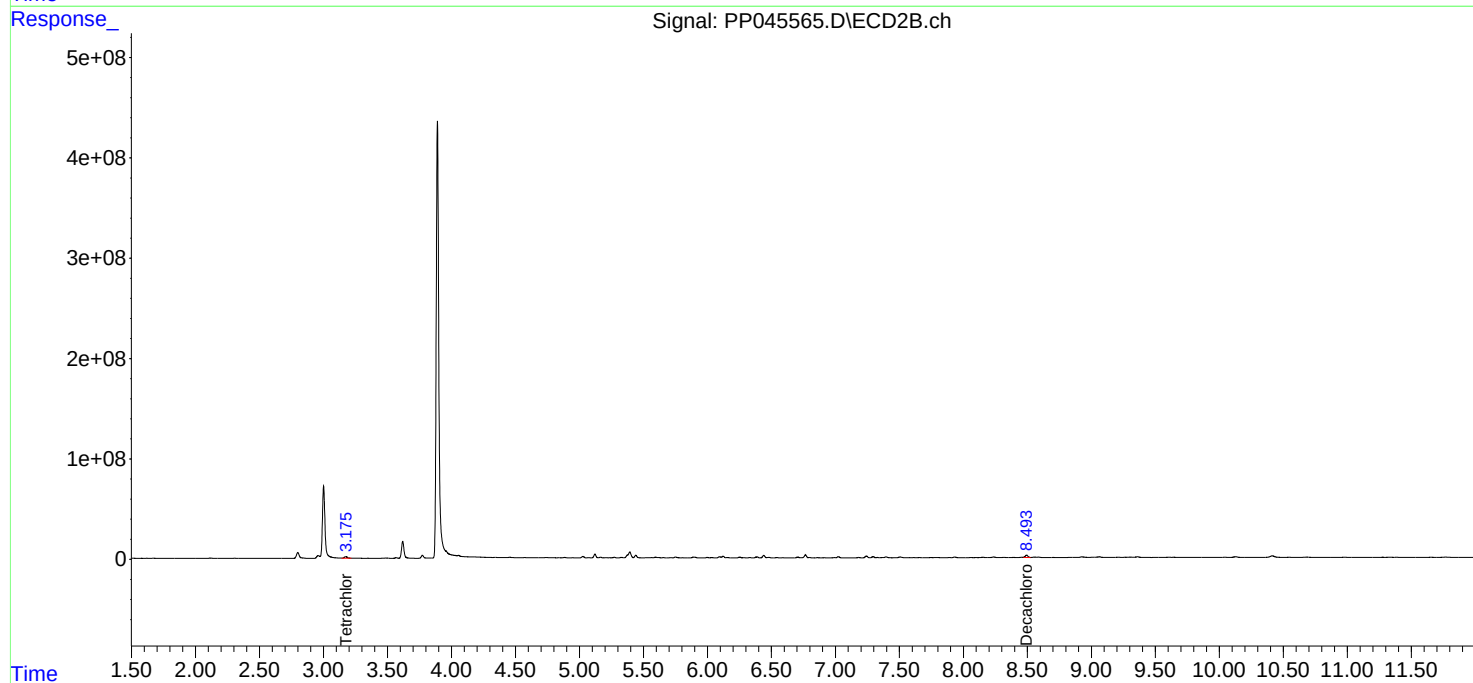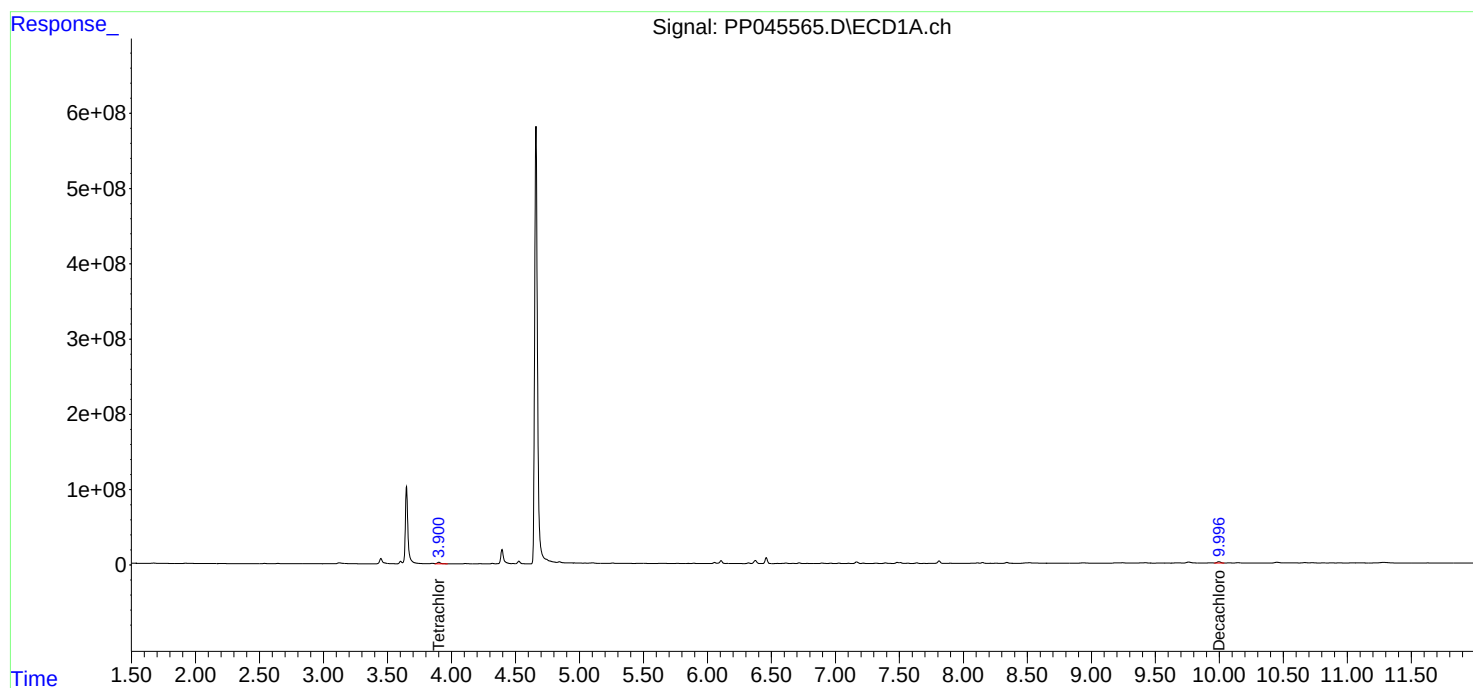

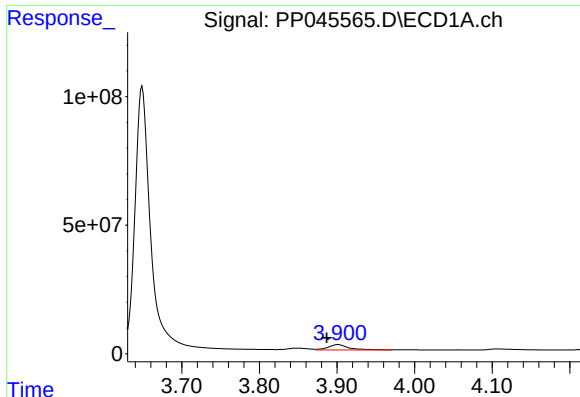


#1 Tetrachloro-m-xylene

R.T.: 3.901 min
Delta R.T.: 0.014 min
Response: 39446254
Conc: 16.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-VNJ-204RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2022
Supervised By :mohammad ahmed 04/07/2022

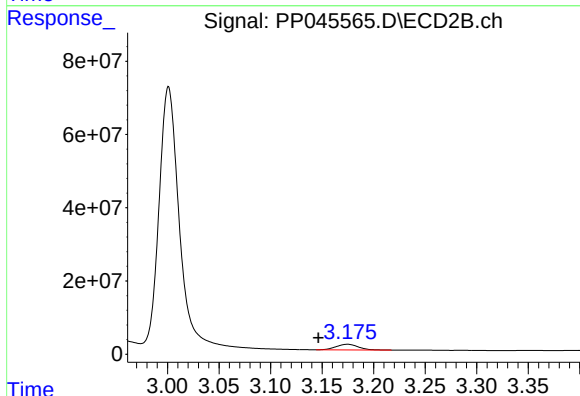


#1 Tetrachloro-m-xylene

R.T.: 3.175 min
Delta R.T.: 0.028 min
Response: 22975325
Conc: 14.52 ng/ml m

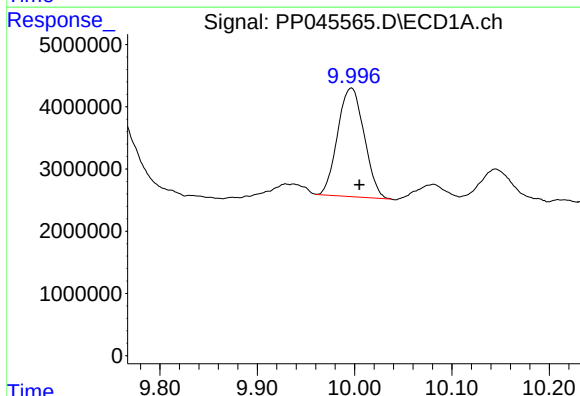

#2 Decachlorobiphenyl

R.T.: 9.996 min
Delta R.T.: -0.008 min
Response: 32971671
Conc: 23.01 ng/ml m

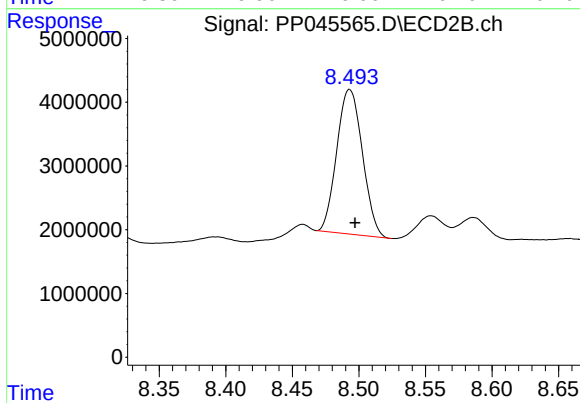

#2 Decachlorobiphenyl

R.T.: 8.493 min
Delta R.T.: -0.005 min
Response: 30463659
Conc: 20.09 ng/ml m