

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040622\
 Data File : PP045613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2022 10:50
 Operator : YP\AJ
 Sample : N2260-06 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-47

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/08/2022
 Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 11:51:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 31 07:54:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.886	3.145	3165005	2684199	1.312m	1.696 #
2) SA Decachlor...	9.995	8.492	3151789	3252772	2.200	2.145
Target Compounds						
26) L6 AR-1254-1	6.060	5.135	45892884	62639193	644.584	643.700
27) L6 AR-1254-2	6.298	5.295	79789257	64088852	738.624	785.863
28) L6 AR-1254-3	6.698	5.725	89331461	106.9E6	805.660	864.259
29) L6 AR-1254-4	7.011	5.974	65849282	65420970	819.288	815.902
30) L6 AR-1254-5	7.471	6.424	92238600	99808487	1153.526	913.536

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040622\
Data File : PP045613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2022 10:50
Operator : YP\AJ
Sample : N2260-06 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-47


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2022
Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 11:51:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 31 07:54:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

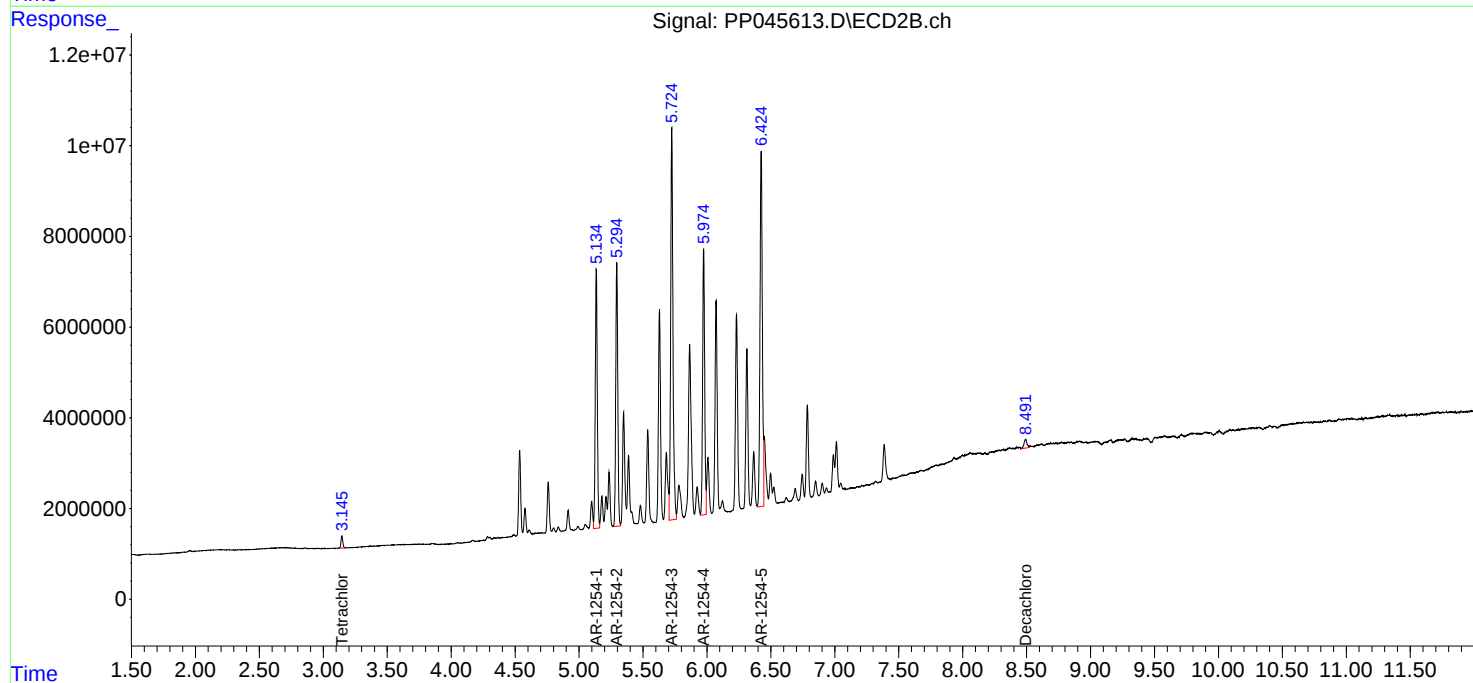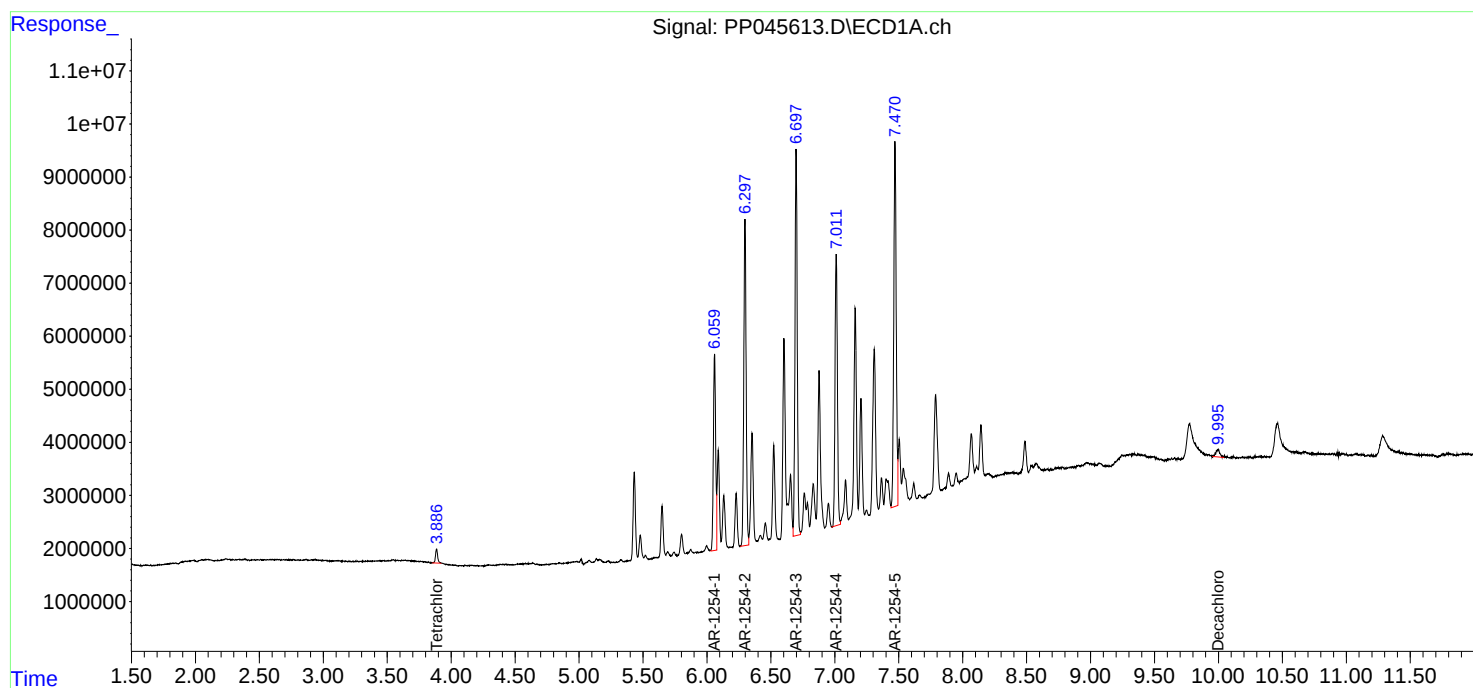

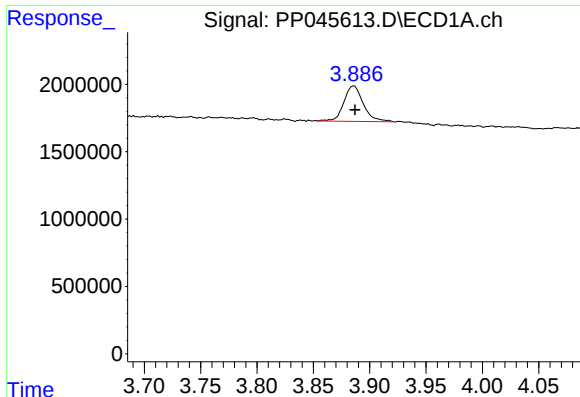


#1 Tetrachloro-m-xylene

R.T.: 3.886 min
Delta R.T.: -0.001 min
Response: 3165005
Conc: 1.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-47


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2022
Supervised By :mohammad ahmed 04/11/2022

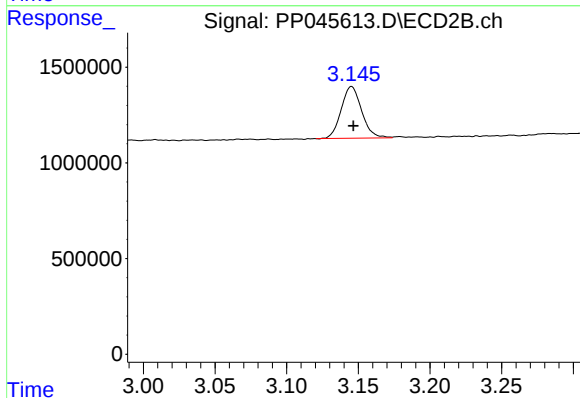


#1 Tetrachloro-m-xylene

R.T.: 3.145 min
Delta R.T.: -0.001 min
Response: 2684199
Conc: 1.70 ng/ml

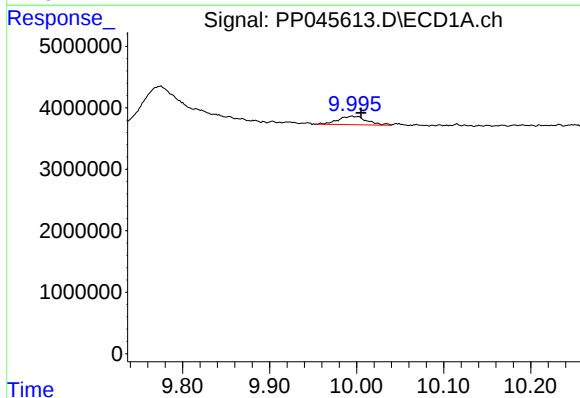


#2 Decachlorobiphenyl

R.T.: 9.995 min
Delta R.T.: -0.010 min
Response: 3151789
Conc: 2.20 ng/ml

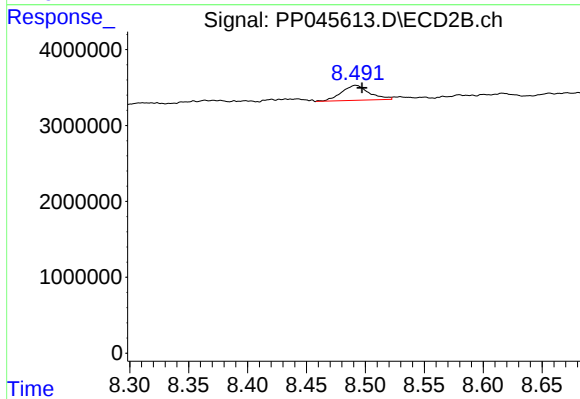

#2 Decachlorobiphenyl

R.T.: 8.492 min
Delta R.T.: -0.005 min
Response: 3252772
Conc: 2.15 ng/ml

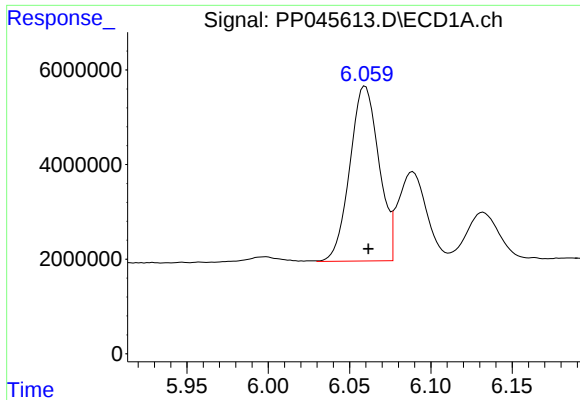


#26 AR-1254-1

R.T.: 6.060 min
Delta R.T.: -0.002 min
Response: 45892884
Conc: 644.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-47


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2022
Supervised By :mohammad ahmed 04/11/2022

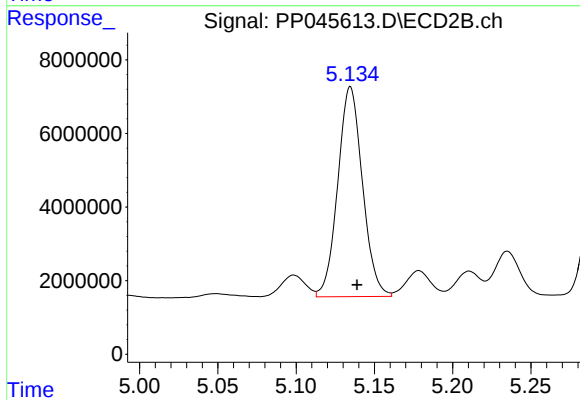


#26 AR-1254-1

R.T.: 5.135 min
Delta R.T.: -0.004 min
Response: 62639193
Conc: 643.70 ng/ml

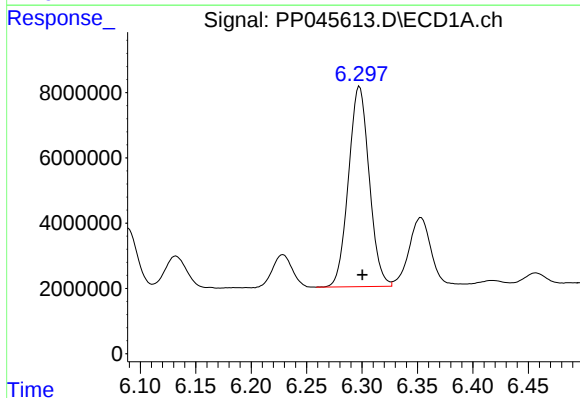


#27 AR-1254-2

R.T.: 6.298 min
Delta R.T.: -0.003 min
Response: 79789257
Conc: 738.62 ng/ml

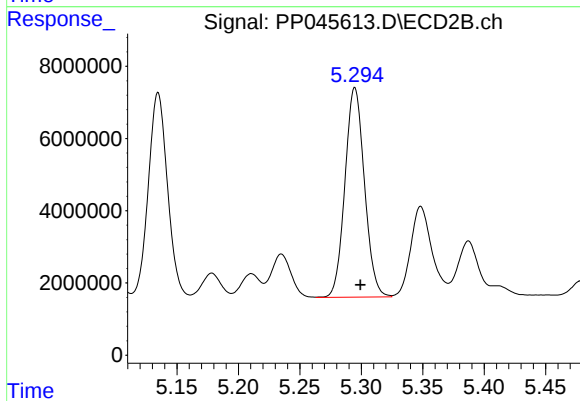

#27 AR-1254-2

R.T.: 5.295 min
Delta R.T.: -0.004 min
Response: 64088852
Conc: 785.86 ng/ml

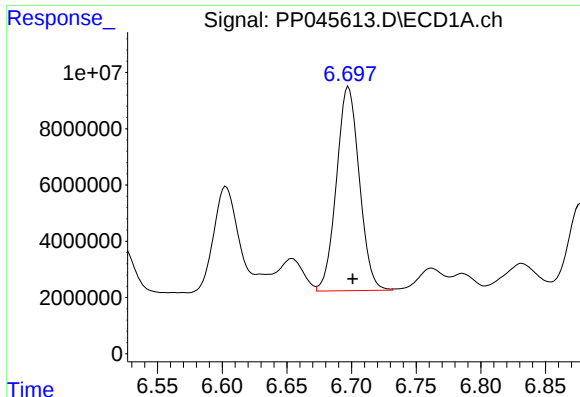


#28 AR-1254-3

R.T.: 6.698 min
Delta R.T.: -0.003 min
Response: 89331461
Conc: 805.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-47


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2022
Supervised By :mohammad ahmed 04/11/2022

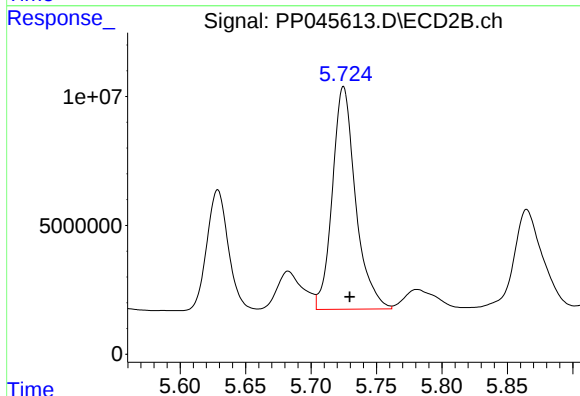


#28 AR-1254-3

R.T.: 5.725 min
Delta R.T.: -0.005 min
Response: 106855984
Conc: 864.26 ng/ml

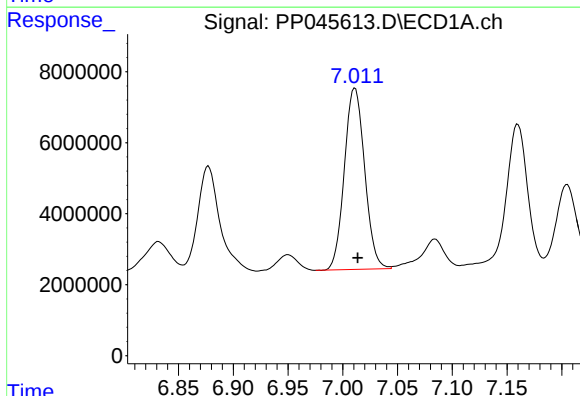


#29 AR-1254-4

R.T.: 7.011 min
Delta R.T.: -0.003 min
Response: 65849282
Conc: 819.29 ng/ml

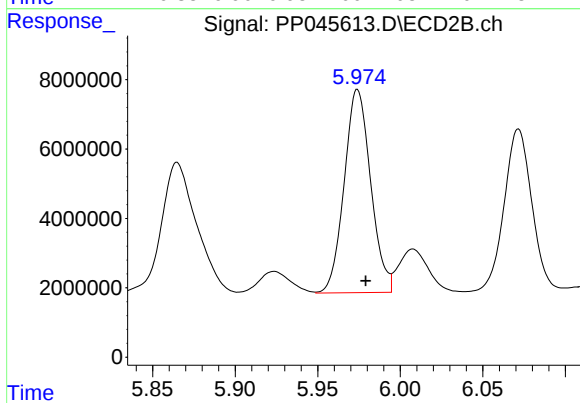

#29 AR-1254-4

R.T.: 5.974 min
Delta R.T.: -0.005 min
Response: 65420970
Conc: 815.90 ng/ml

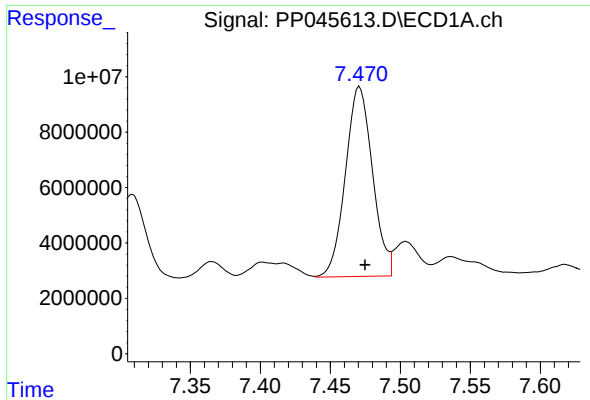


#30 AR-1254-5

R.T.: 7.471 min
Delta R.T.: -0.004 min
Response: 92238600
Conc: 1153.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-47

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2022
Supervised By :mohammad ahmed 04/11/2022

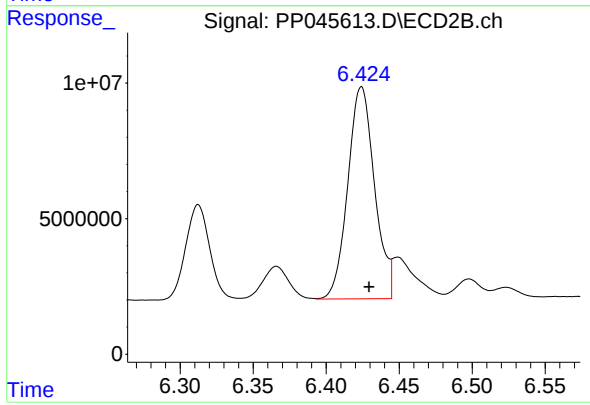

#30 AR-1254-5

R.T.: 6.424 min
Delta R.T.: -0.005 min
Response: 99808487
Conc: 913.54 ng/ml