

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040622\
 Data File : PP045626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2022 15:07
 Operator : YP\AJ
 Sample : N2254-01RE
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-14A-1A-4-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/08/2022
 Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 16:54:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 31 07:54:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.885	3.148	30857321	19491560	12.789m	12.318
2) SA Decachlor...	9.997	8.492	24689624	19580946	17.231	12.913 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040622\
Data File : PP045626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2022 15:07
Operator : YP\AJ
Sample : N2254-01RE
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-14A-1A-4-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2022
Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 16:54:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 31 07:54:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

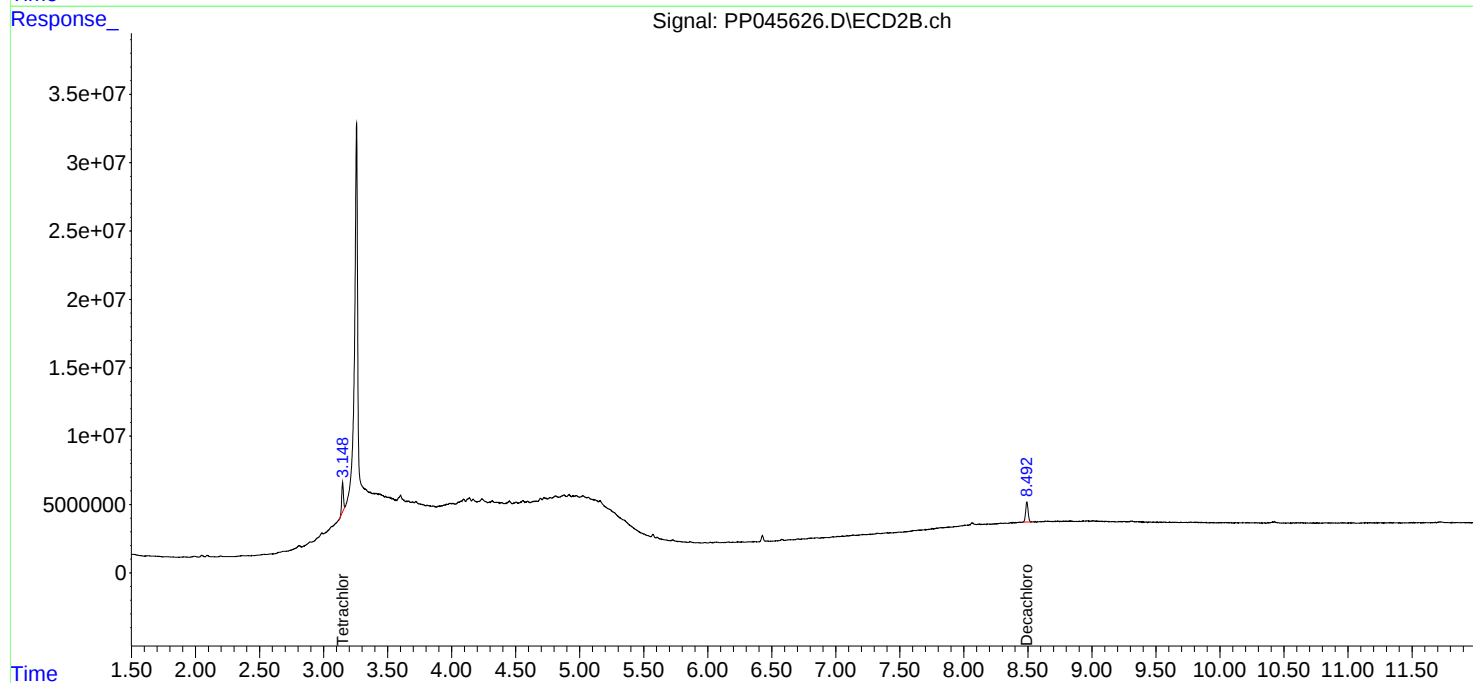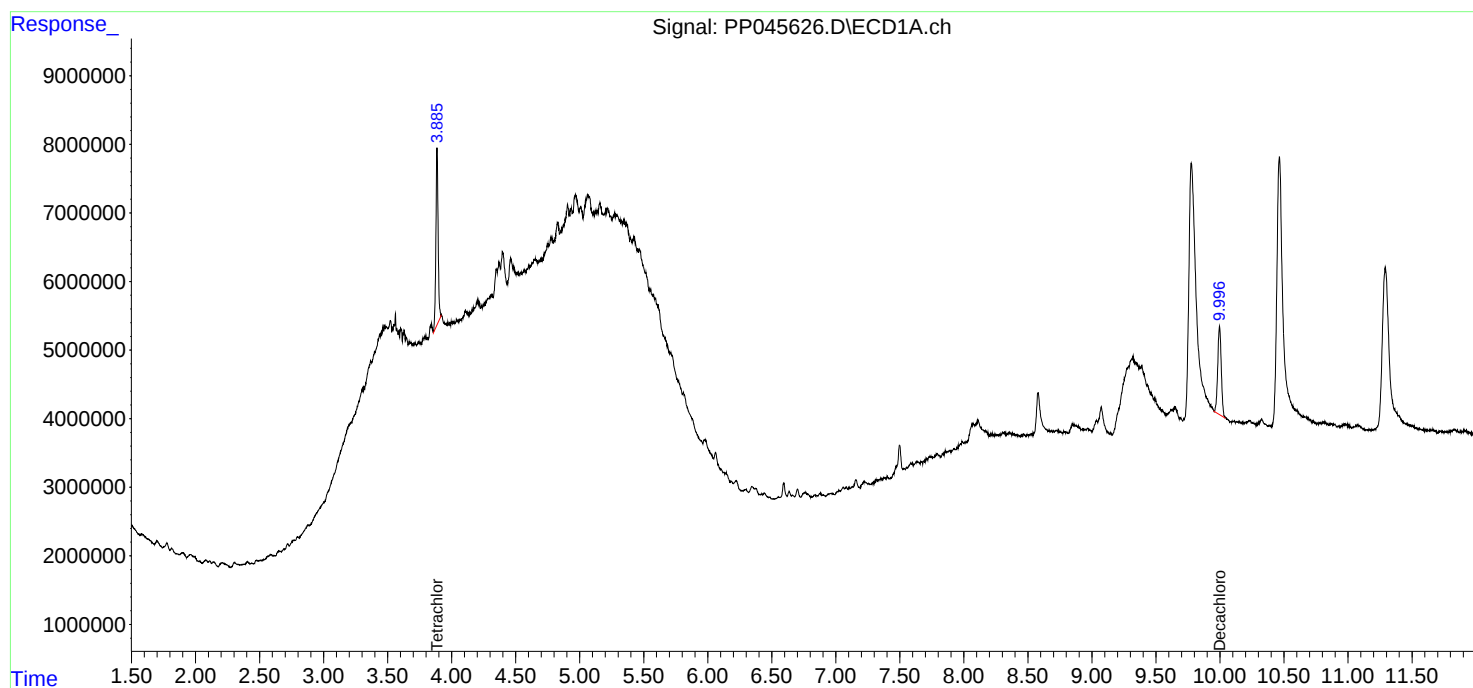

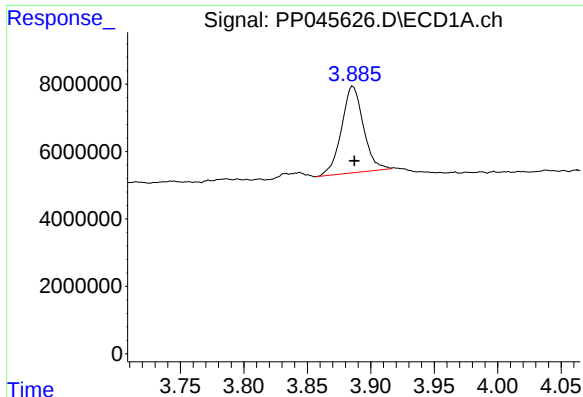

#1 Tetrachloro-m-xylene

R.T.: 3.885 min
Delta R.T.: -0.002 min
Response: 30857321
Conc: 12.79 ng/ml

Instrument :

ECD_P

ClientSampleId :


WC-14A-1A-4-1

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 04/08/2022

Supervised By :mohammad ahmed 04/11/2022

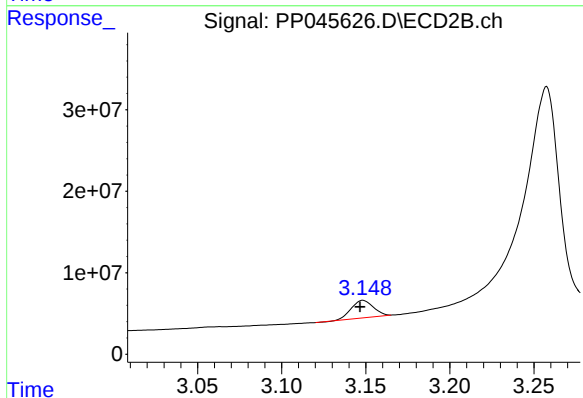


#1 Tetrachloro-m-xylene

R.T.: 3.148 min
Delta R.T.: 0.002 min
Response: 19491560
Conc: 12.32 ng/ml

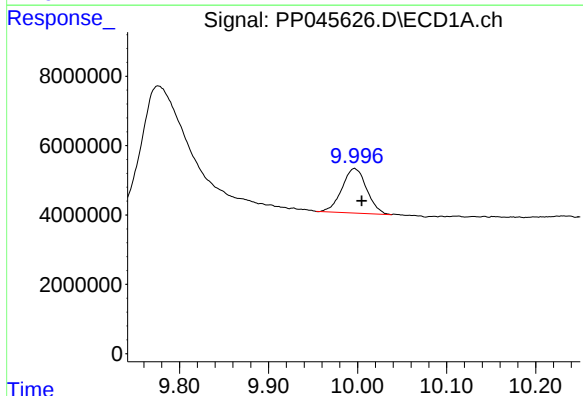

#2 Decachlorobiphenyl

R.T.: 9.997 min
Delta R.T.: -0.008 min
Response: 24689624
Conc: 17.23 ng/ml

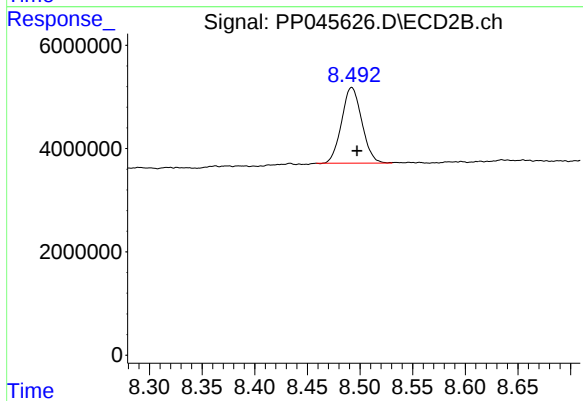

#2 Decachlorobiphenyl

R.T.: 8.492 min
Delta R.T.: -0.005 min
Response: 19580946
Conc: 12.91 ng/ml