

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040622\
 Data File : PP045648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2022 01:11
 Operator : YP\AJ
 Sample : N2287-01 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2022-22-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/08/2022
 Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 03:38:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 31 07:54:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.883	3.144	4627458	3583339	1.918m	2.265
2) SA Decachlor...	9.989f	8.487	3645137	2883013	2.544m	1.901 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040622\
Data File : PP045648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2022 01:11
Operator : YP\AJ
Sample : N2287-01 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MOO-2022-22-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2022
Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 03:38:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 31 07:54:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

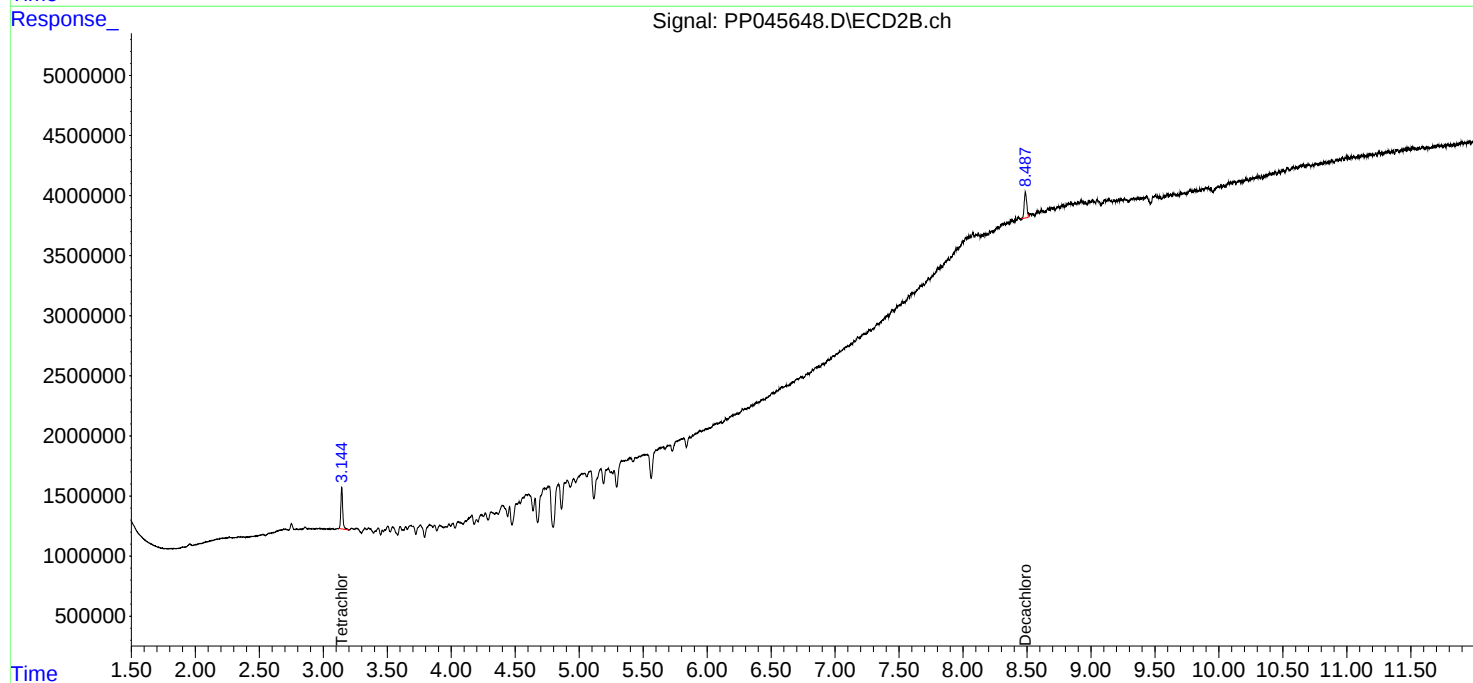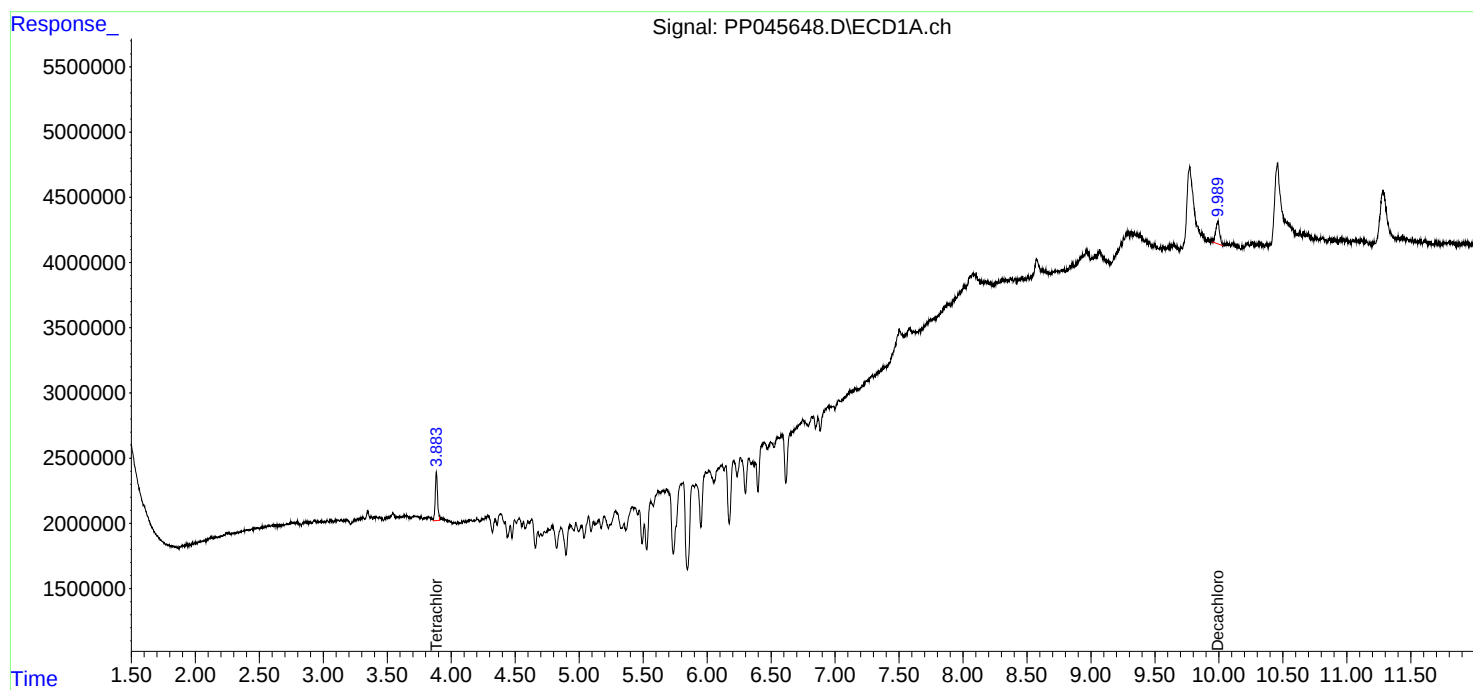

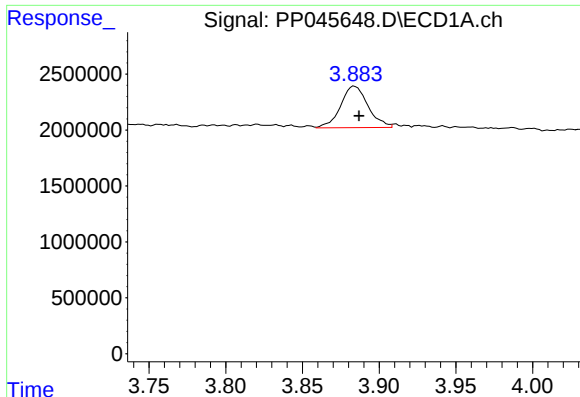


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: -0.004 min
Response: 4627458
Conc: 1.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-22-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2022
Supervised By :mohammad ahmed 04/11/2022

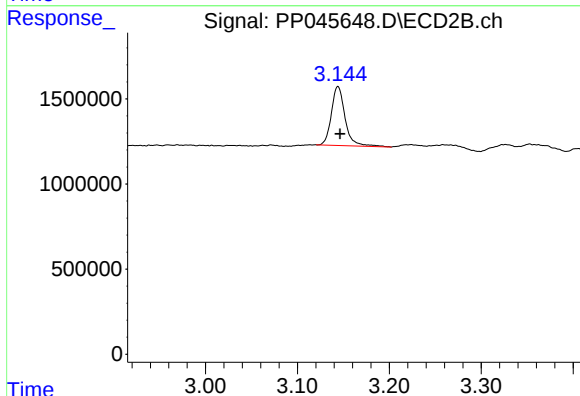


#1 Tetrachloro-m-xylene

R.T.: 3.144 min
Delta R.T.: -0.002 min
Response: 3583339
Conc: 2.26 ng/ml

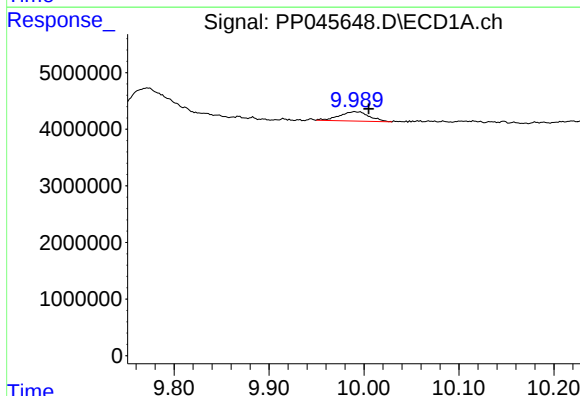

#2 Decachlorobiphenyl

R.T.: 9.989 min
Delta R.T.: -0.015 min
Response: 3645137
Conc: 2.54 ng/ml m

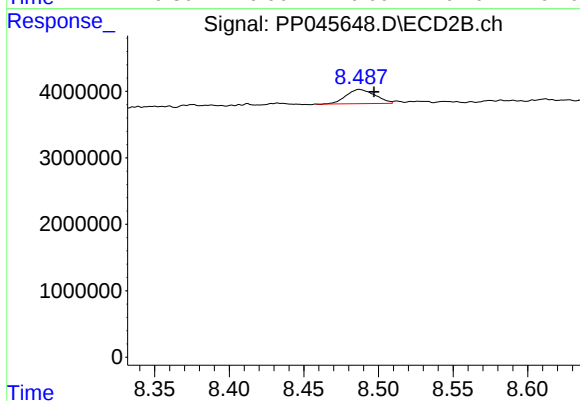

#2 Decachlorobiphenyl

R.T.: 8.487 min
Delta R.T.: -0.010 min
Response: 2883013
Conc: 1.90 ng/ml