

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040623\
 Data File : PP056683.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2023 22:02
 Operator : YP\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/07/2023
 Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 00:32:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 00:00:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.436	3.663	9735730	8153484	4.657	4.812
2) SA Decachlor...	10.273	8.749	5668746	7508548	4.452m	4.868m
Target Compounds						
21) L5 AR-1248-1	5.611	4.765	1940546	1646604	51.721	50.022
22) L5 AR-1248-2	5.887	5.004	3088849	2688105	52.447	52.153
23) L5 AR-1248-3	6.092	5.047	3298418	2767714	51.771	51.558
24) L5 AR-1248-4	6.498	5.221	2937489	3192818	50.581	51.601
25) L5 AR-1248-5	6.537	5.619	2824342	2527043	50.000	49.218

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040623\
Data File : PP056683.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2023 22:02
Operator : YP\AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 00:32:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 00:00:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

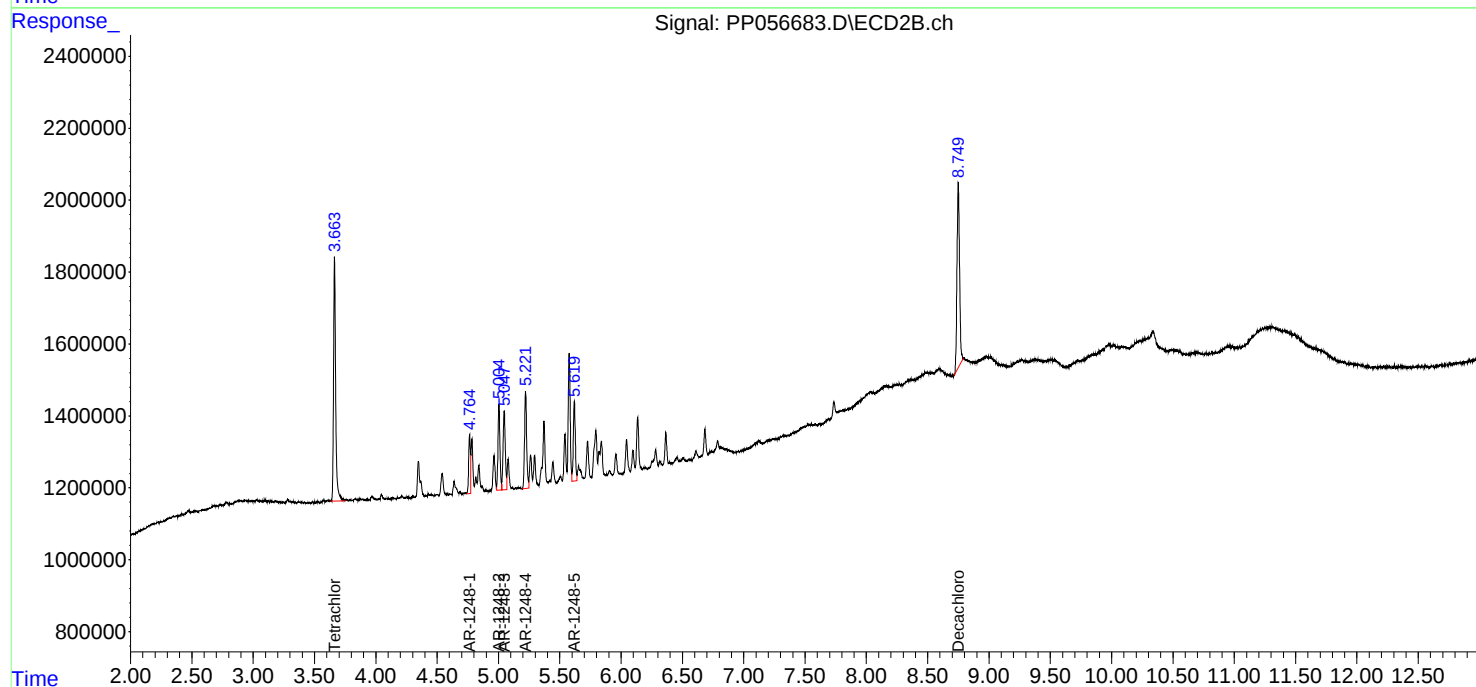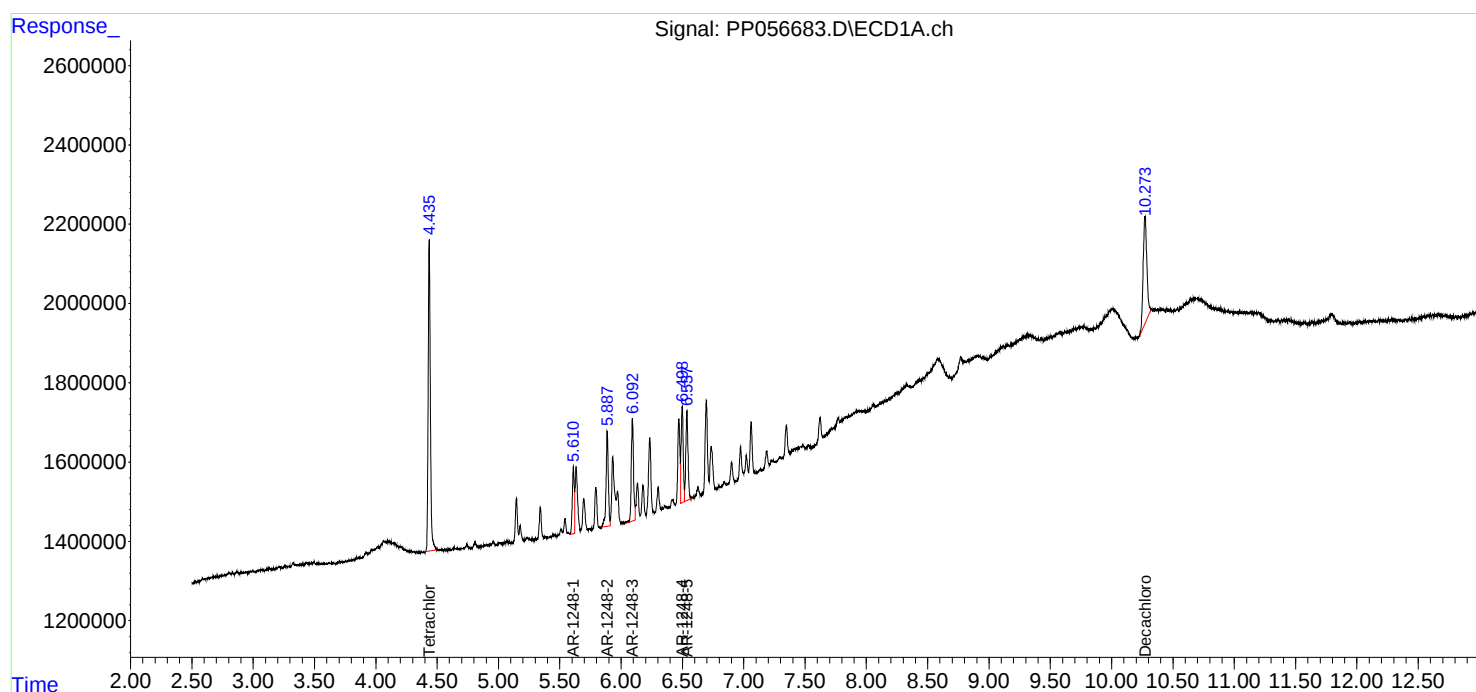

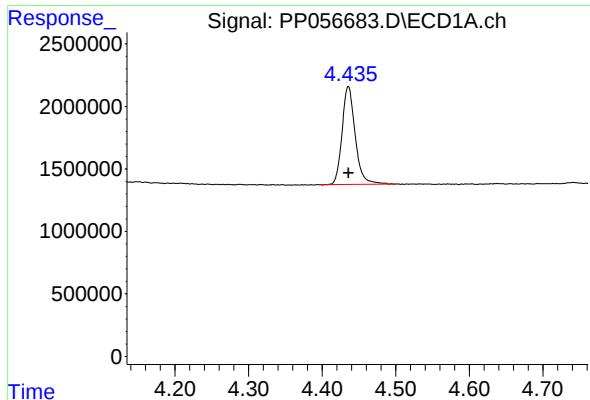


#1 Tetrachloro-m-xylene

R.T.: 4.436 min
Delta R.T.: 0.000 min
Response: 9735730
Conc: 4.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248IC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

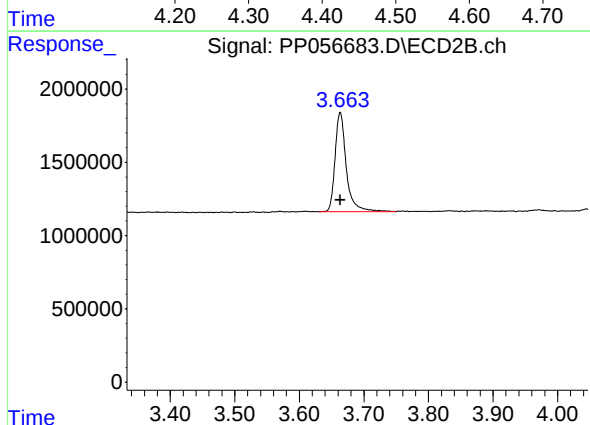


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 8153484
Conc: 4.81 ng/ml

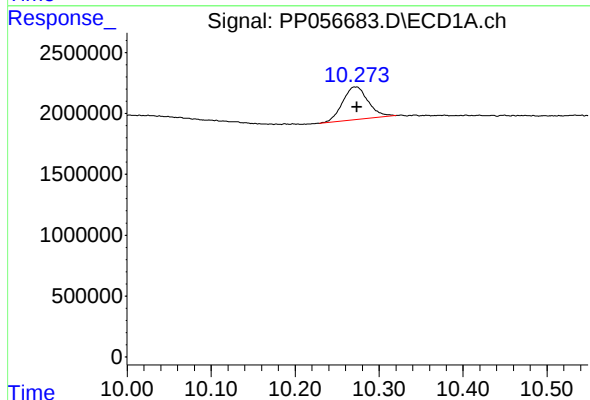


#2 Decachlorobiphenyl

R.T.: 10.273 min
Delta R.T.: 0.000 min
Response: 5668746
Conc: 4.45 ng/ml m

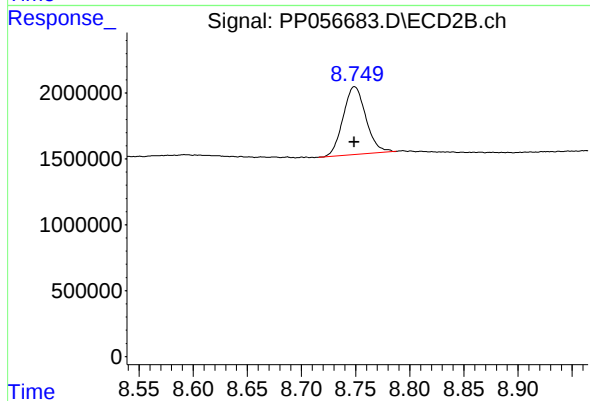

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: 0.000 min
Response: 7508548
Conc: 4.87 ng/ml m

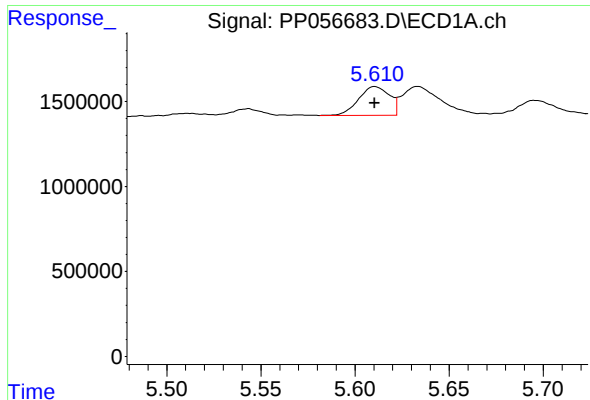


#21 AR-1248-1

R.T.: 5.611 min
Delta R.T.: 0.000 min
Response: 1940546
Conc: 51.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

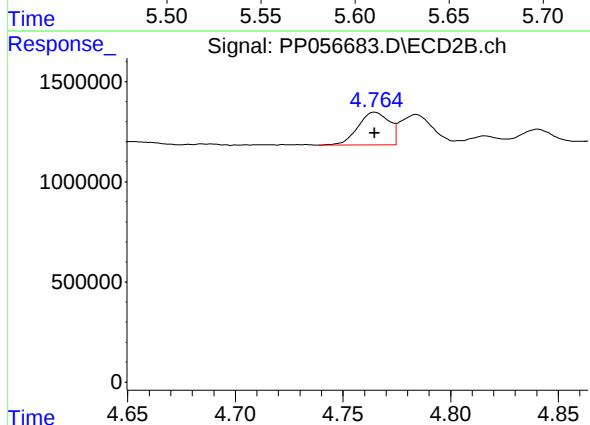


#21 AR-1248-1

R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 1646604
Conc: 50.02 ng/ml

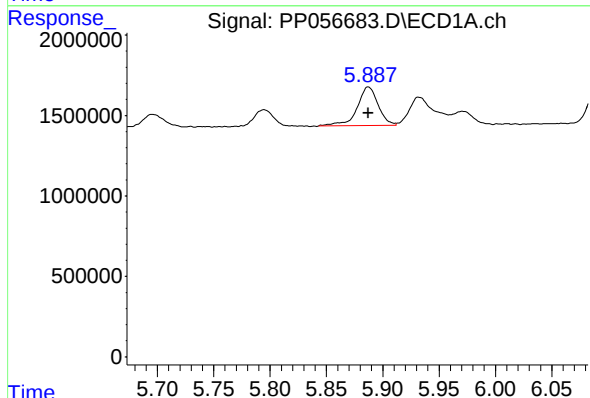


#22 AR-1248-2

R.T.: 5.887 min
Delta R.T.: 0.000 min
Response: 3088849
Conc: 52.45 ng/ml

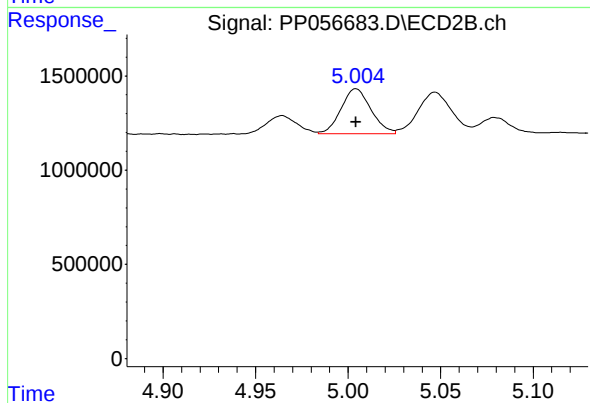

#22 AR-1248-2

R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 2688105
Conc: 52.15 ng/ml

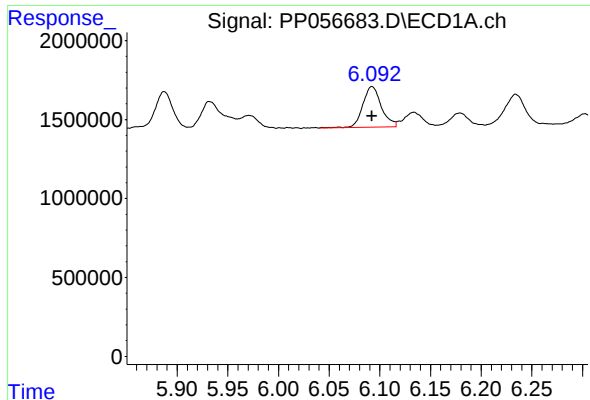


#23 AR-1248-3

R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 3298418
Conc: 51.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

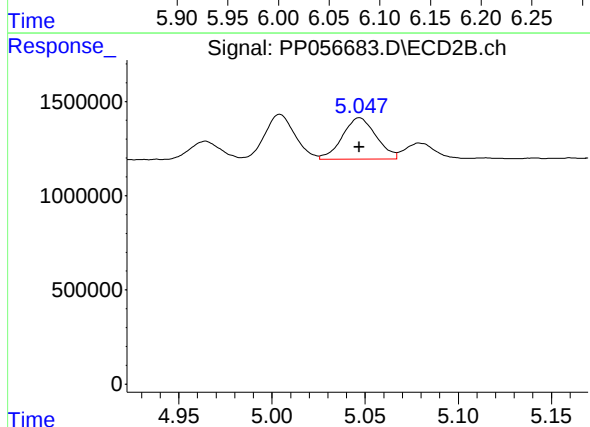


#23 AR-1248-3

R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 2767714
Conc: 51.56 ng/ml

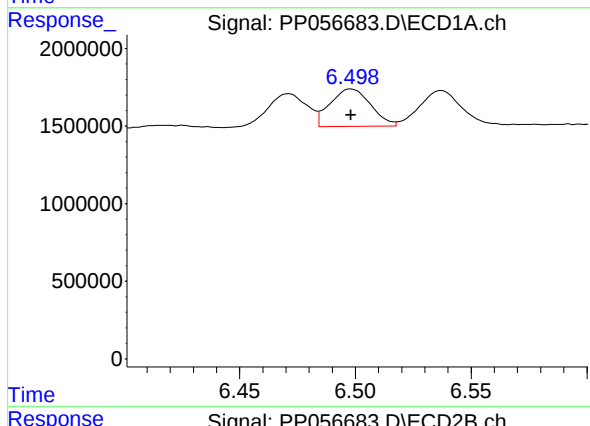


#24 AR-1248-4

R.T.: 6.498 min
Delta R.T.: 0.000 min
Response: 2937489
Conc: 50.58 ng/ml

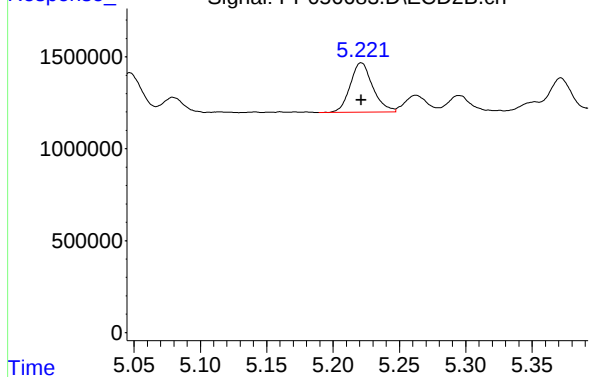

#24 AR-1248-4

R.T.: 5.221 min
Delta R.T.: 0.000 min
Response: 3192818
Conc: 51.60 ng/ml

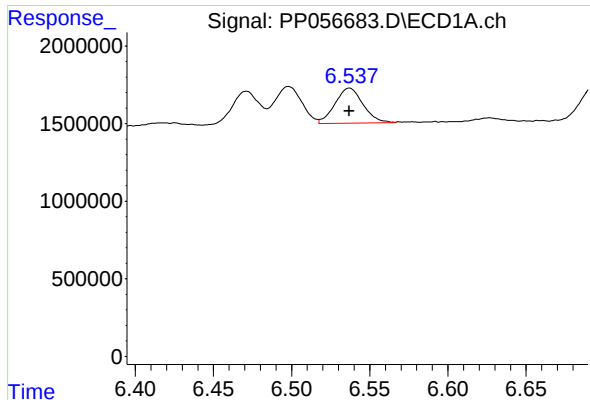


#25 AR-1248-5

R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 2824342
Conc: 50.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

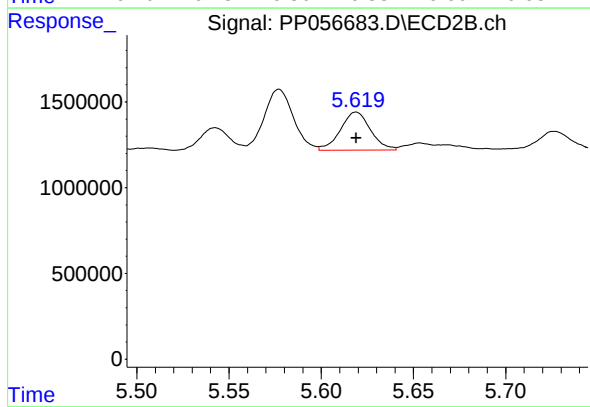

#25 AR-1248-5

R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 2527043
Conc: 49.22 ng/ml