

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040723\
 Data File : PP056789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 10:23
 Operator : YP\AJ
 Sample : 02213-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:38:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 04:14:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.660	40749617	32794961	18.966	18.856
2) SA Decachlor...	10.264	8.741	27788317	32714467	21.230	20.807
Target Compounds						
11) L3 AR-1232-1	4.804	4.041	1200301	991635	24.921	24.104
12) L3 AR-1232-2	5.339	4.780	596085	835153	23.863	24.368
13) L3 AR-1232-3	5.630	4.958	1084738	403011	26.905	21.902
14) L3 AR-1232-4	5.791	5.041	488388	508369	24.239	26.529
15) L3 AR-1232-5	5.883	5.217	385973	536401	21.959	25.235



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040723\
Data File : PP056789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 10:23
Operator : YP\AJ
Sample : 02213-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 74 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:38:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 04:14:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

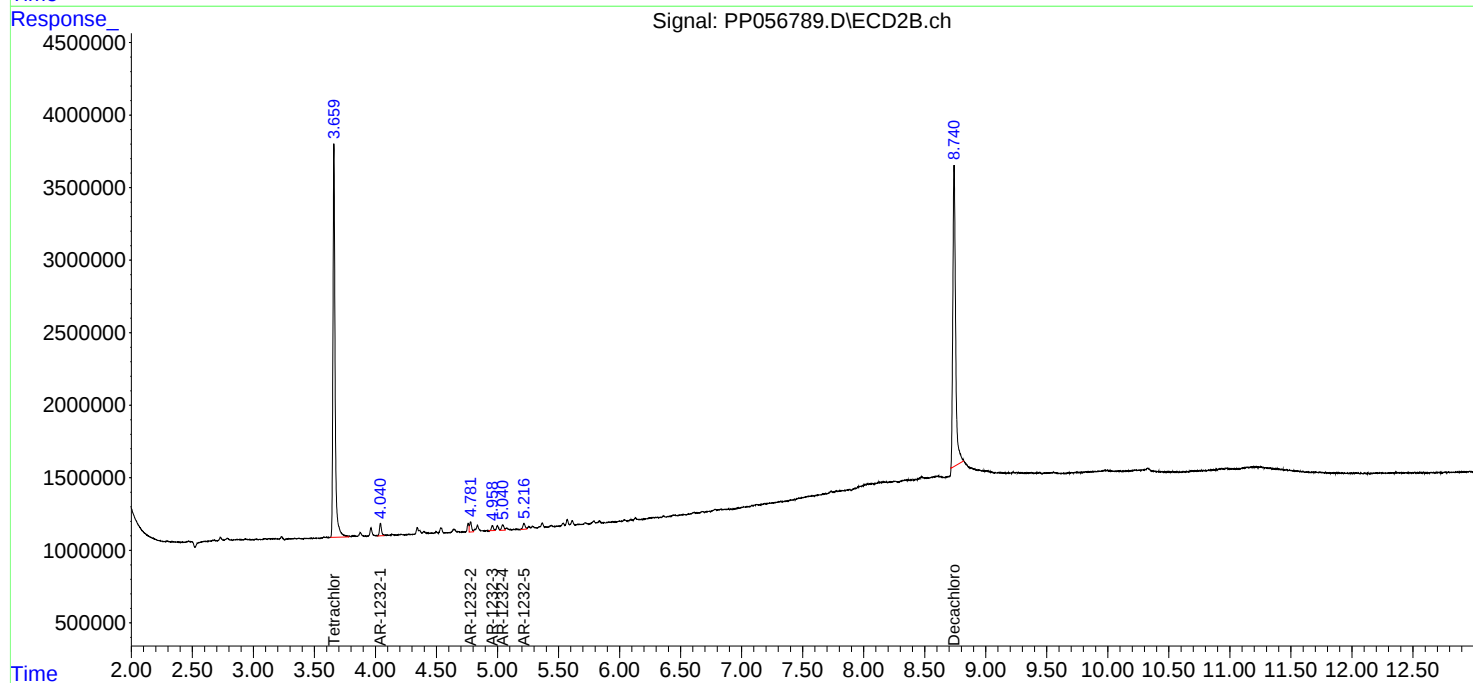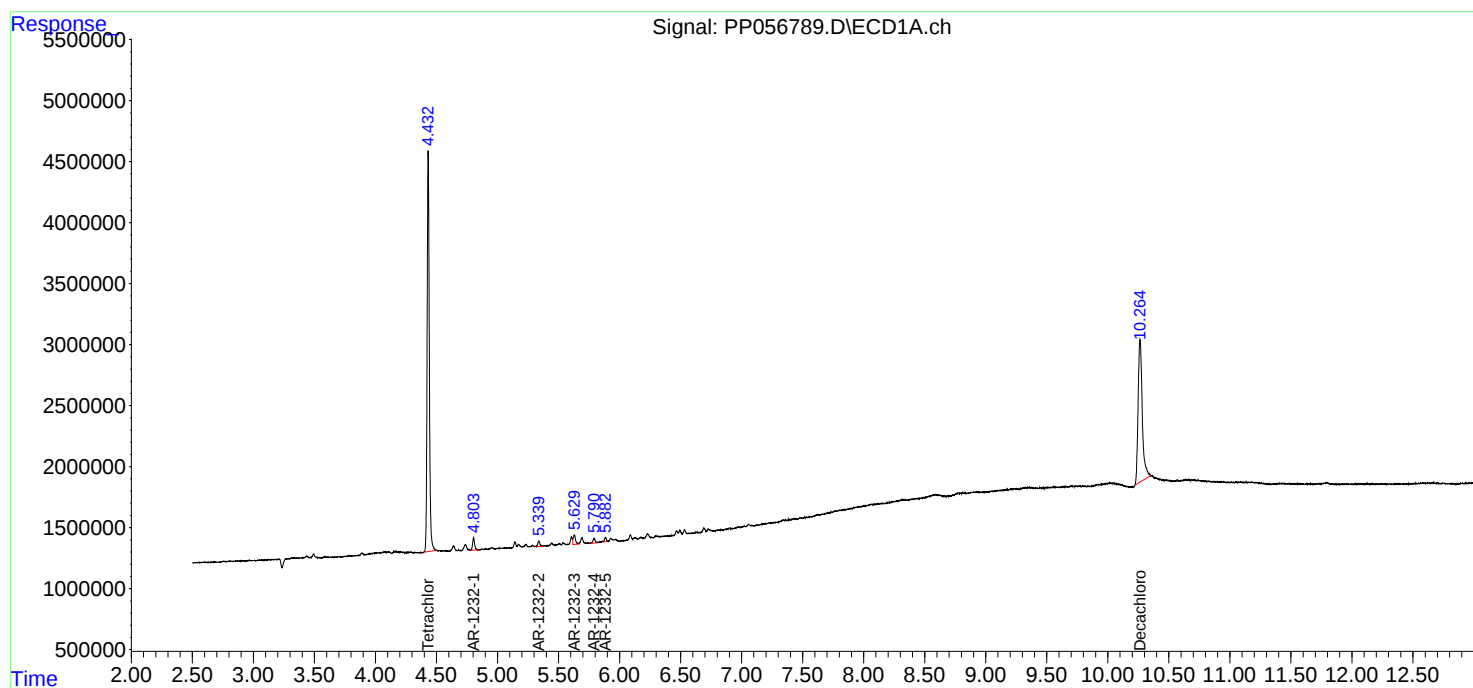


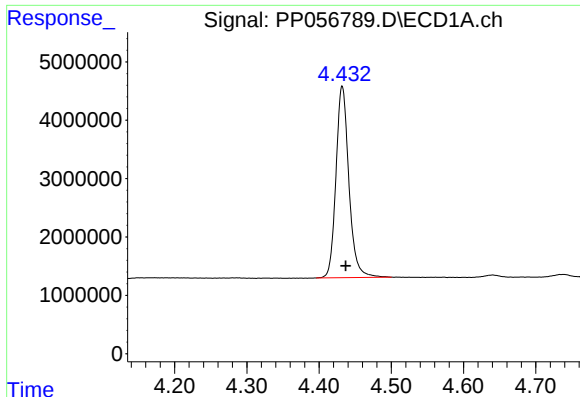

#1 Tetrachloro-m-xylene


R.T.: 4.432 min
Delta R.T.: -0.005 min
Response: 40749617
Conc: 18.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

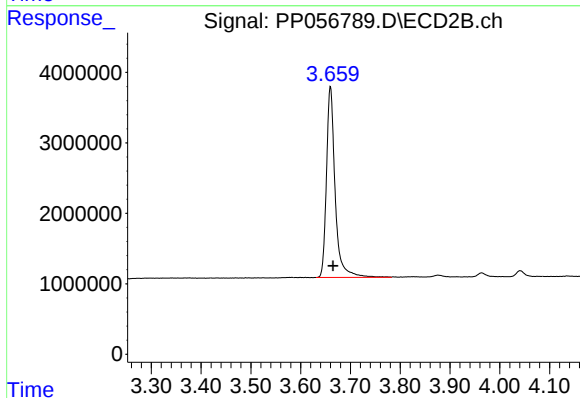


#1 Tetrachloro-m-xylene

R.T.: 3.660 min
Delta R.T.: -0.005 min
Response: 32794961
Conc: 18.86 ng/ml

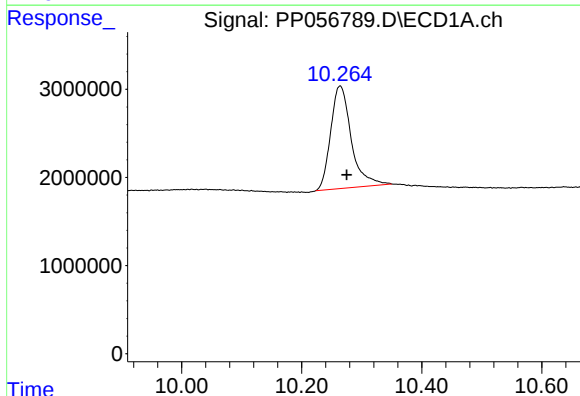


#2 Decachlorobiphenyl

R.T.: 10.264 min
Delta R.T.: -0.011 min
Response: 27788317
Conc: 21.23 ng/ml

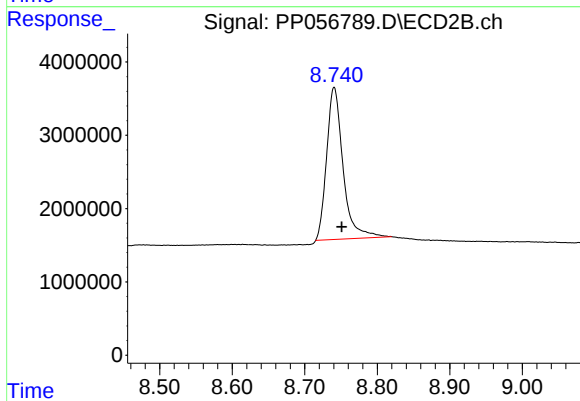

#2 Decachlorobiphenyl


R.T.: 8.741 min
Delta R.T.: -0.011 min
Response: 32714467
Conc: 20.81 ng/ml

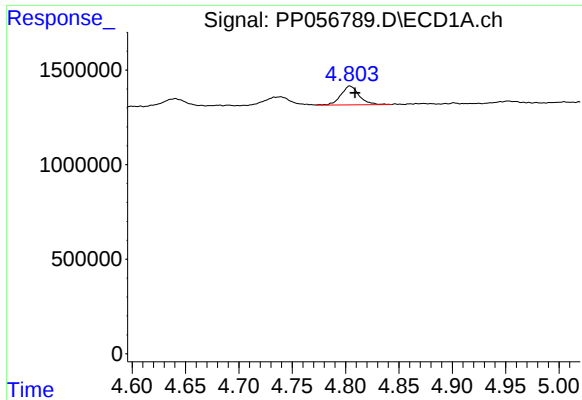

#11 AR-1232-1


R.T.: 4.804 min
Delta R.T.: -0.005 min
Response: 1200301
Conc: 24.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

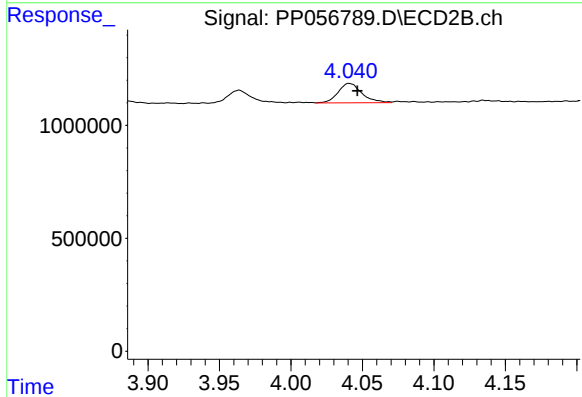


#11 AR-1232-1

R.T.: 4.041 min
Delta R.T.: -0.006 min
Response: 991635
Conc: 24.10 ng/ml

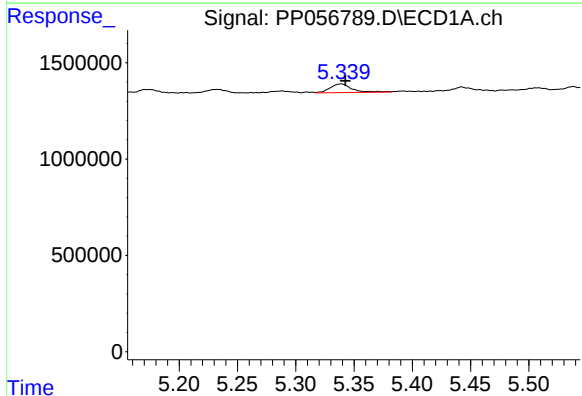


#12 AR-1232-2

R.T.: 5.339 min
Delta R.T.: -0.004 min
Response: 596085
Conc: 23.86 ng/ml

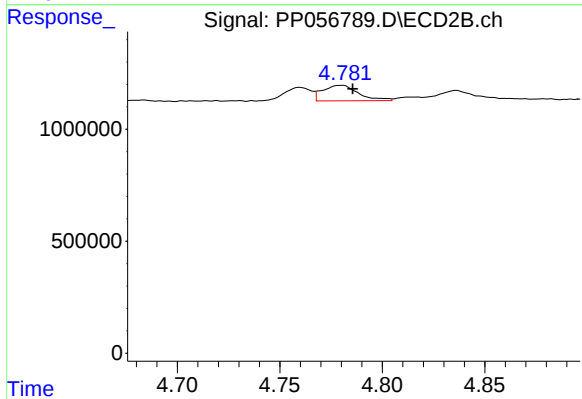

#12 AR-1232-2


R.T.: 4.780 min
Delta R.T.: -0.006 min
Response: 835153
Conc: 24.37 ng/ml

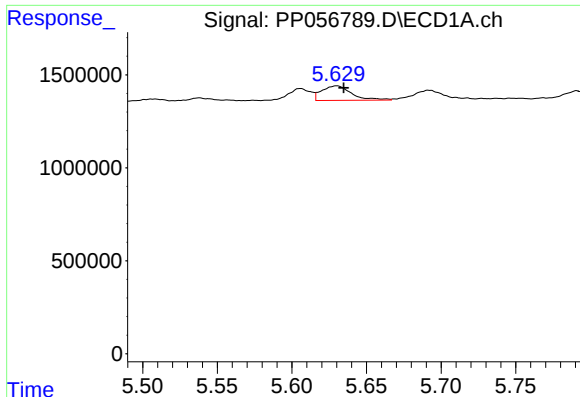

#13 AR-1232-3


R.T.: 5.630 min
Delta R.T.: -0.005 min
Response: 1084738
Conc: 26.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

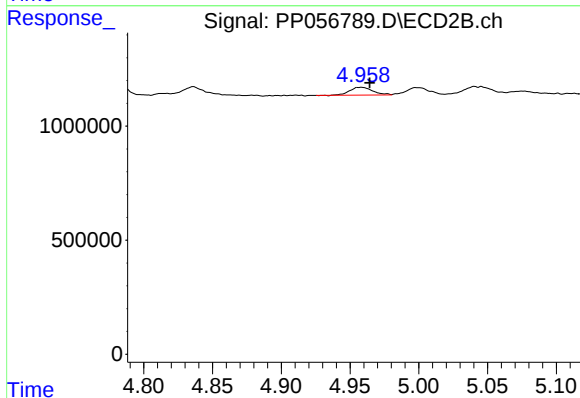


#13 AR-1232-3

R.T.: 4.958 min
Delta R.T.: -0.006 min
Response: 403011
Conc: 21.90 ng/ml

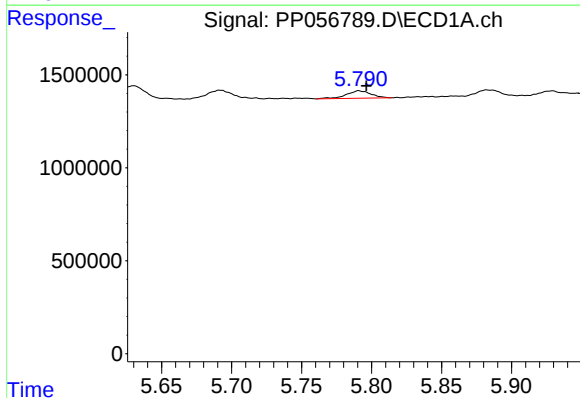


#14 AR-1232-4

R.T.: 5.791 min
Delta R.T.: -0.005 min
Response: 488388
Conc: 24.24 ng/ml

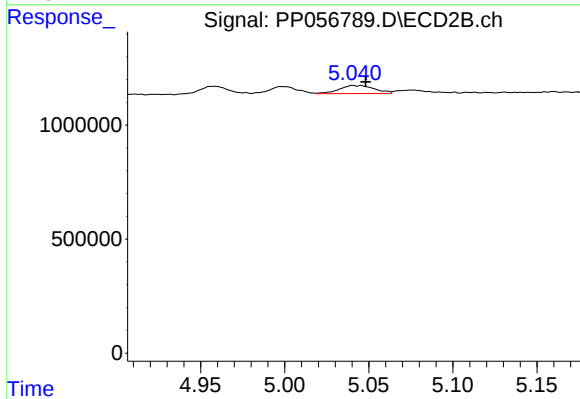

#14 AR-1232-4


R.T.: 5.041 min
Delta R.T.: -0.007 min
Response: 508369
Conc: 26.53 ng/ml

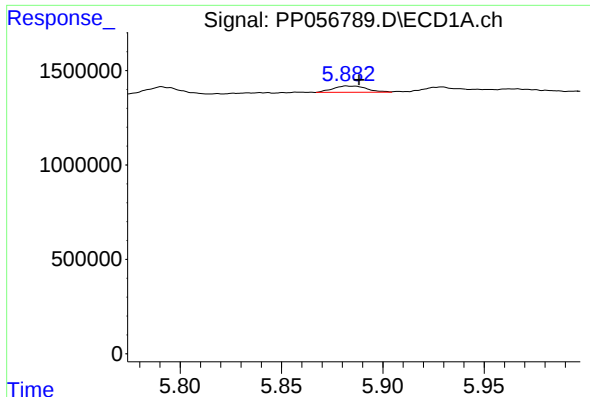

#15 AR-1232-5

R.T.: 5.883 min
Delta R.T.: -0.005 min
Response: 385973
Conc: 21.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

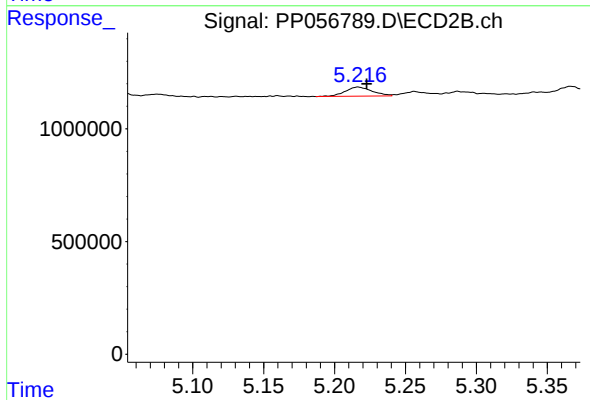

#15 AR-1232-5

R.T.: 5.217 min
Delta R.T.: -0.006 min
Response: 536401
Conc: 25.23 ng/ml