

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040723\
 Data File : PP056792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 11:12
 Operator : YP\AJ
 Sample : 02213-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:42:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 04:14:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.660	40581307	32551200	18.888	18.716
2) SA Decachlor...	10.264	8.740	27188727	32376570	20.772	20.592
Target Compounds						
26) L6 AR-1254-1	6.467	5.572	2680406	2768571	37.802	30.055
27) L6 AR-1254-2	6.687	5.721	3184802	2284649	31.405	28.427
28) L6 AR-1254-3	7.055	6.129	2916800	3389510	30.091	27.420
29) L6 AR-1254-4	7.342	6.359	1886239	1632192	30.904	25.681
30) L6 AR-1254-5	7.764	6.781	1945446	2989069	28.550	28.430



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040723\
Data File : PP056792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 11:12
Operator : YP\AJ
Sample : 02213-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 77 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:42:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 04:14:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

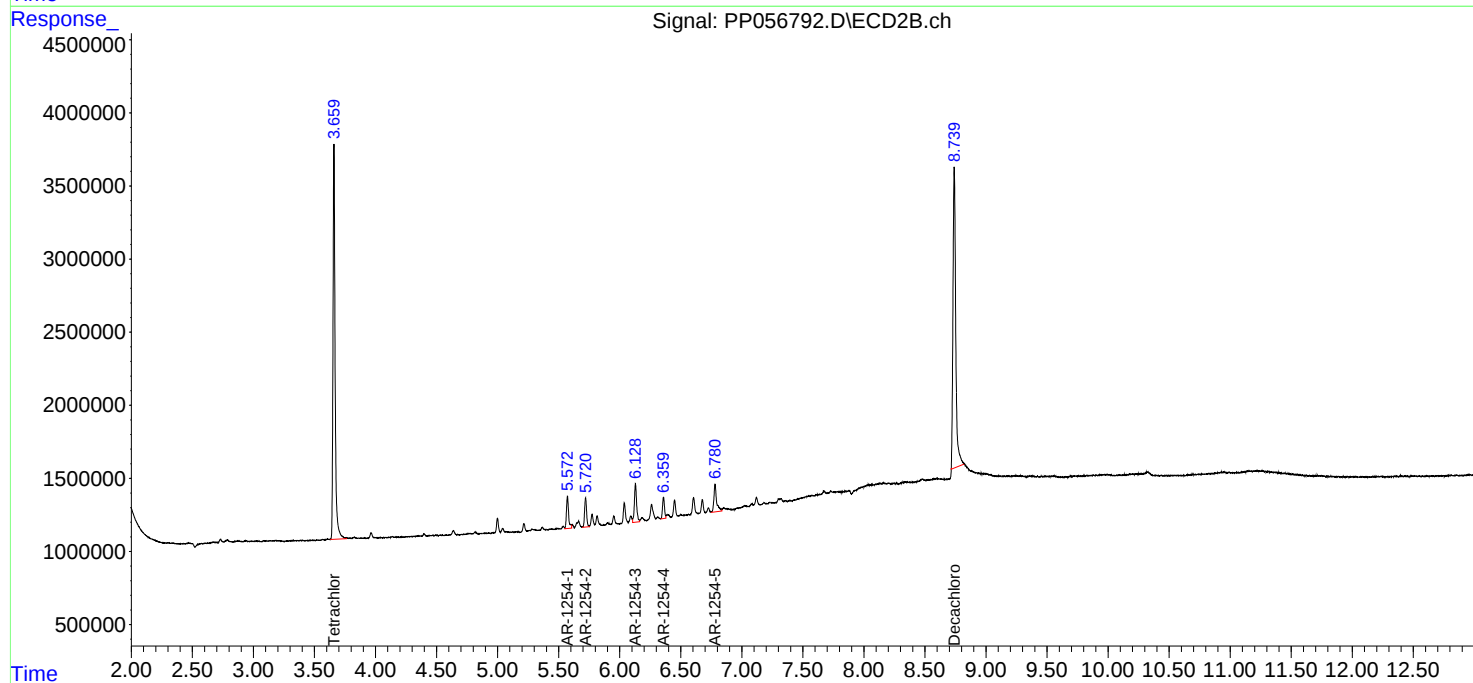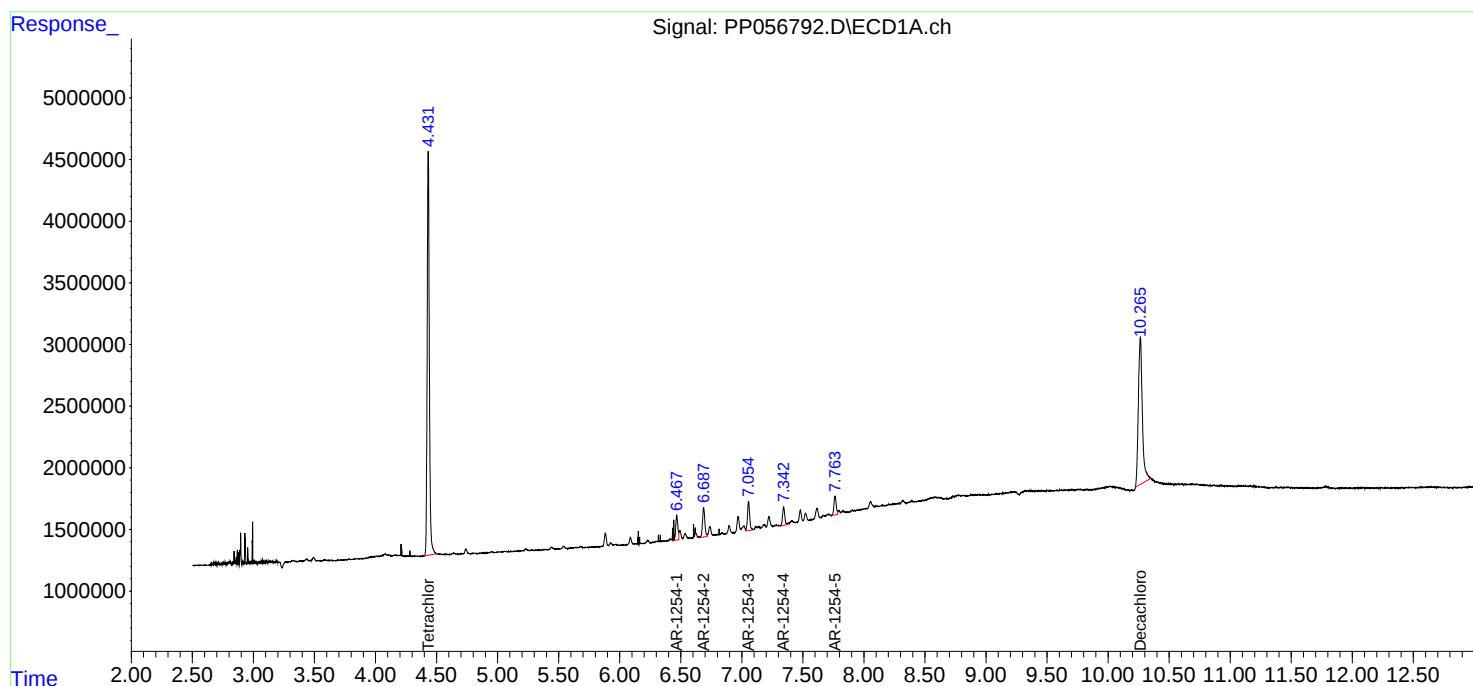


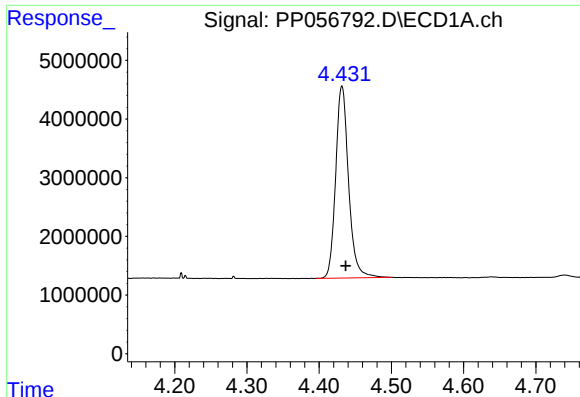

#1 Tetrachloro-m-xylene


R.T.: 4.432 min
Delta R.T.: -0.005 min
Response: 40581307
Conc: 18.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

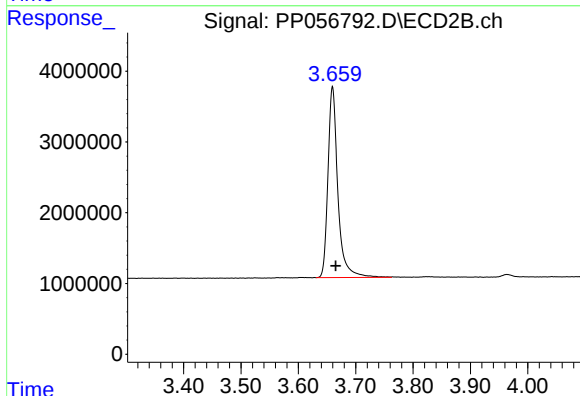


#1 Tetrachloro-m-xylene

R.T.: 3.660 min
Delta R.T.: -0.006 min
Response: 32551200
Conc: 18.72 ng/ml

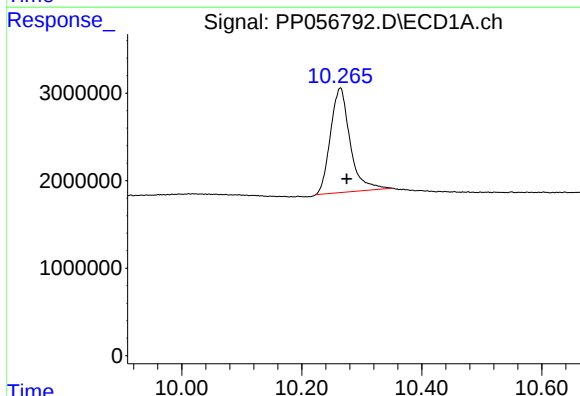


#2 Decachlorobiphenyl

R.T.: 10.264 min
Delta R.T.: -0.011 min
Response: 27188727
Conc: 20.77 ng/ml

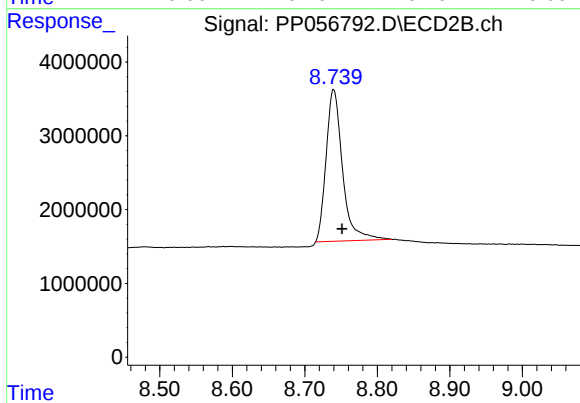

#2 Decachlorobiphenyl


R.T.: 8.740 min
Delta R.T.: -0.011 min
Response: 32376570
Conc: 20.59 ng/ml

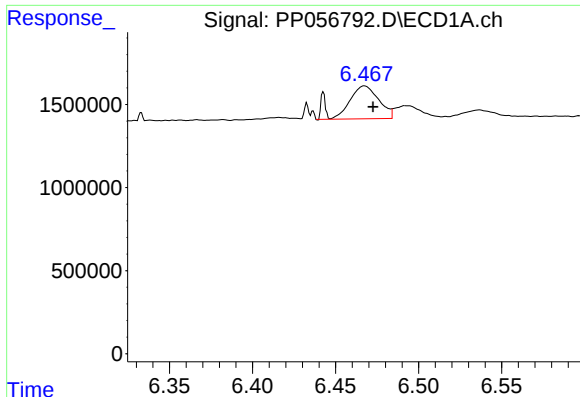

#26 AR-1254-1


R.T.: 6.467 min
Delta R.T.: -0.005 min
Response: 2680406
Conc: 37.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

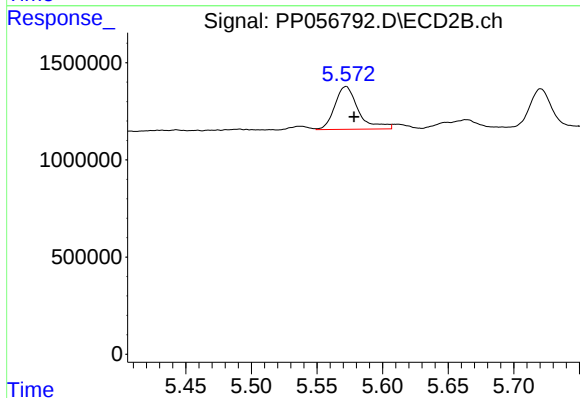


#26 AR-1254-1

R.T.: 5.572 min
Delta R.T.: -0.006 min
Response: 2768571
Conc: 30.05 ng/ml

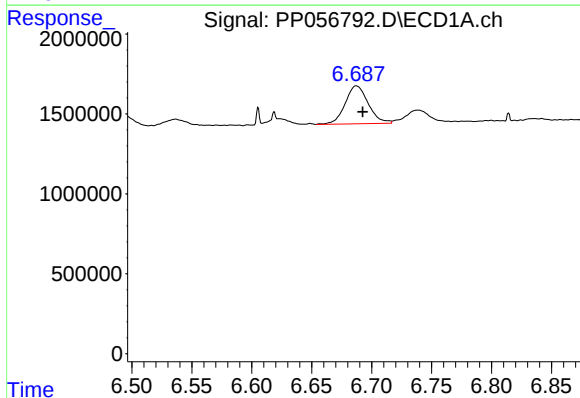


#27 AR-1254-2

R.T.: 6.687 min
Delta R.T.: -0.005 min
Response: 3184802
Conc: 31.41 ng/ml

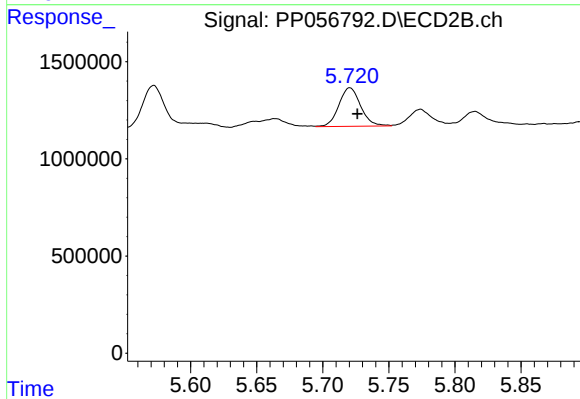

#27 AR-1254-2


R.T.: 5.721 min
Delta R.T.: -0.006 min
Response: 2284649
Conc: 28.43 ng/ml

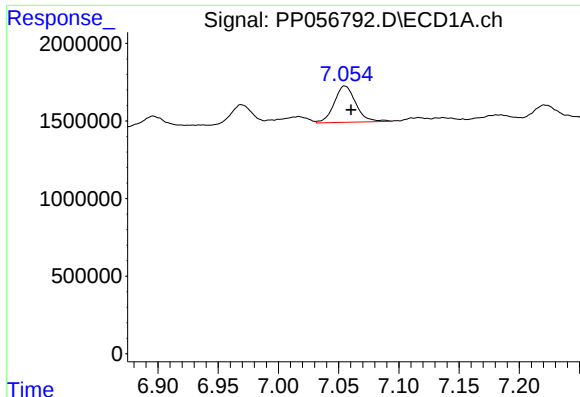

#28 AR-1254-3


R.T.: 7.055 min
Delta R.T.: -0.005 min
Response: 2916800
Conc: 30.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

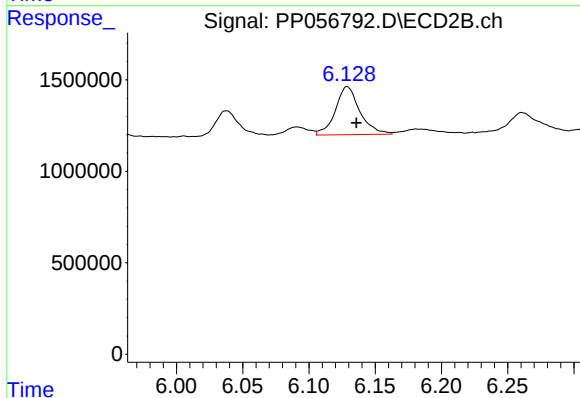


#28 AR-1254-3

R.T.: 6.129 min
Delta R.T.: -0.007 min
Response: 3389510
Conc: 27.42 ng/ml

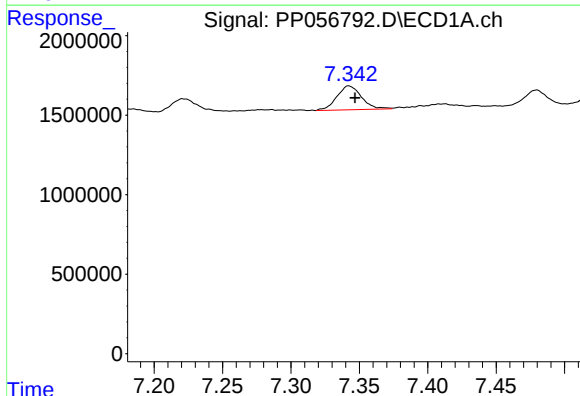


#29 AR-1254-4

R.T.: 7.342 min
Delta R.T.: -0.005 min
Response: 1886239
Conc: 30.90 ng/ml

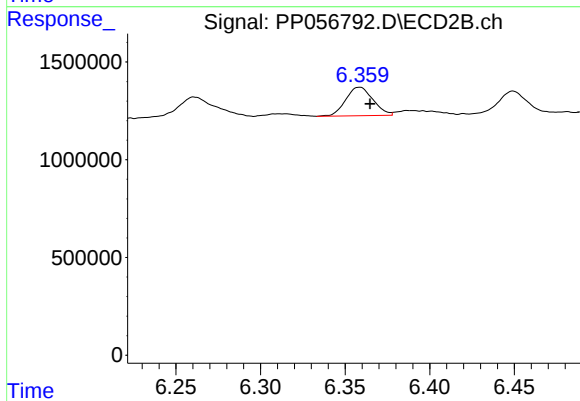

#29 AR-1254-4


R.T.: 6.359 min
Delta R.T.: -0.006 min
Response: 1632192
Conc: 25.68 ng/ml

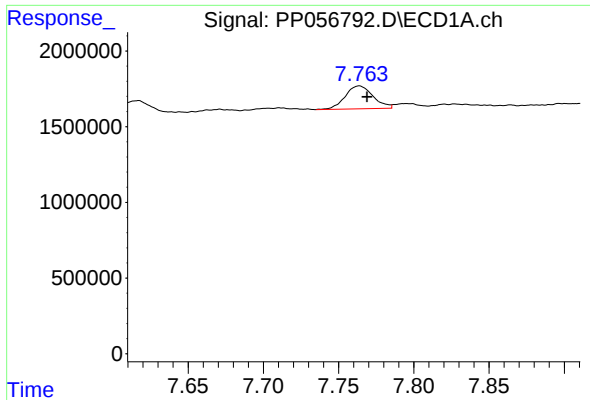

#30 AR-1254-5

R.T.: 7.764 min
Delta R.T.: -0.005 min
Response: 1945446
Conc: 28.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

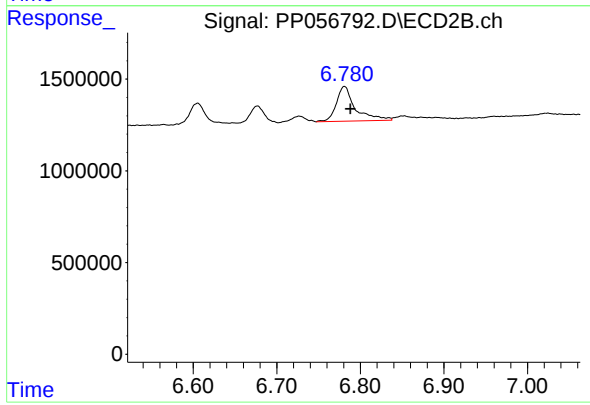

#30 AR-1254-5

R.T.: 6.781 min
Delta R.T.: -0.007 min
Response: 2989069
Conc: 28.43 ng/ml