

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040723\
 Data File : PP056794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 11:45
 Operator : YP\AJ
 Sample : 02213-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:44:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 04:14:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.660	42095238	33726748	19.593	19.392
2) SA Decachlor...	10.265	8.741	30786963	36619123	23.521	23.290
Target Compounds						
41) L9 AR-1268-1	8.712	7.610	5133053	6374920	27.559	28.757
42) L9 AR-1268-2	8.808	7.674	4896656	5589537	29.507	28.782
43) L9 AR-1268-3	9.045	7.884	4688480	5770288	29.463	29.110
44) L9 AR-1268-4	9.480	8.173	1320192	1653041	28.434	28.578
45) L9 AR-1268-5	9.911	8.475	11981368	15179759	27.897	29.891



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040723\
Data File : PP056794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 11:45
Operator : YP\AJ
Sample : 02213-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 79 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:44:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 04:14:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

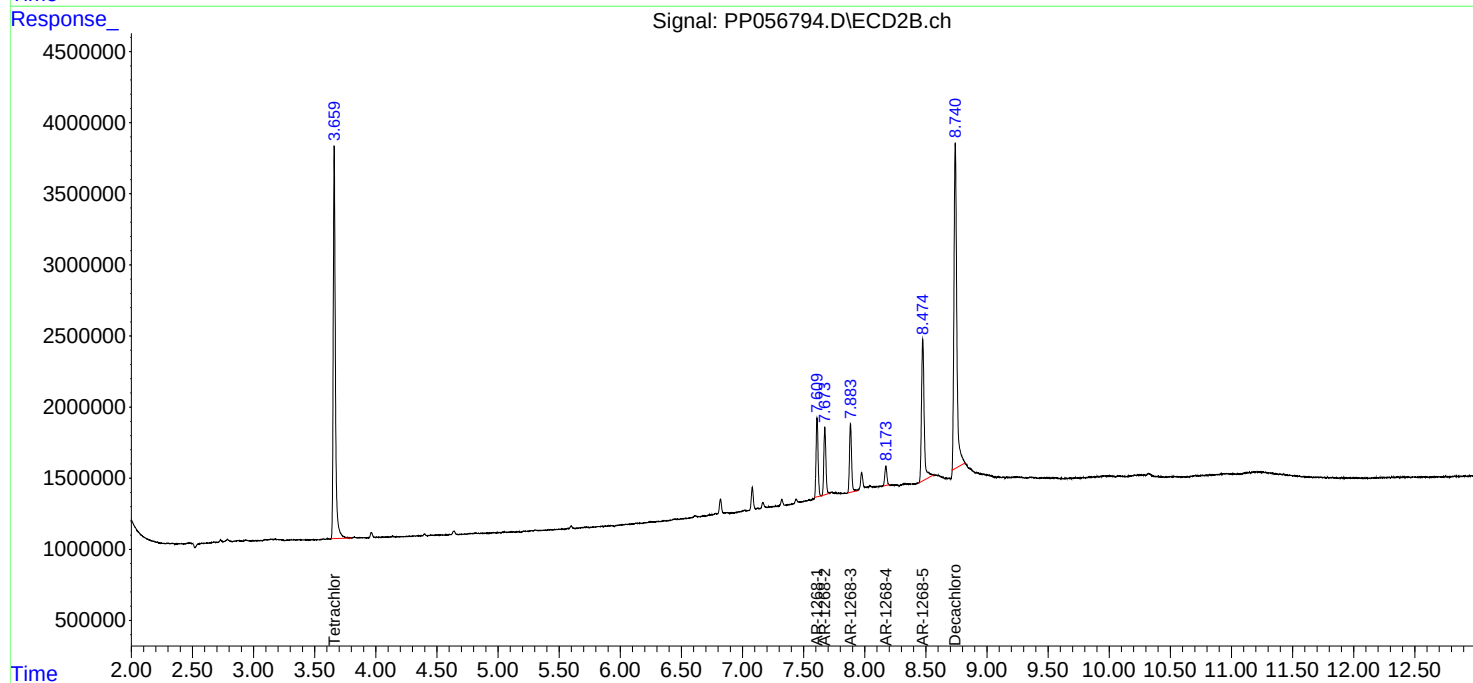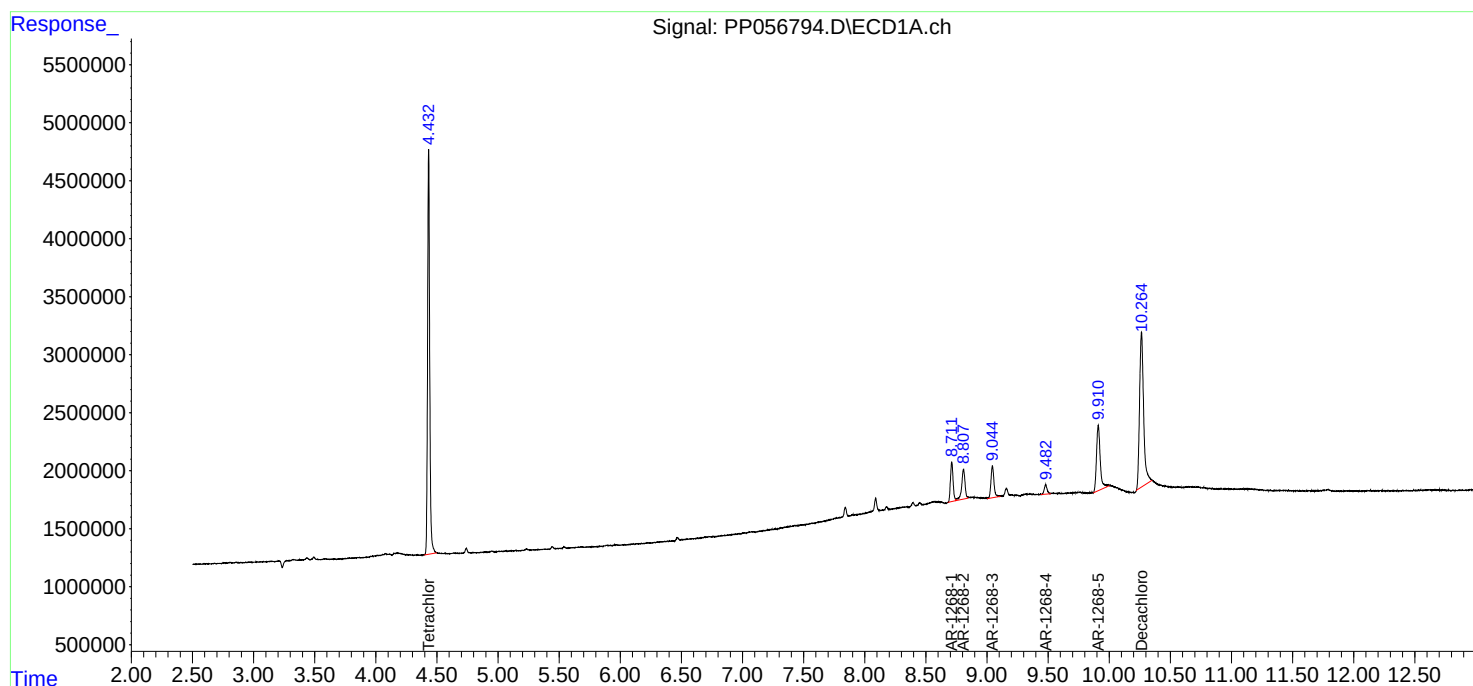


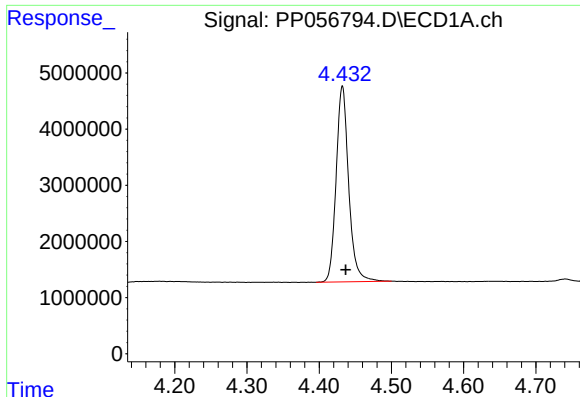

#1 Tetrachloro-m-xylene


R.T.: 4.432 min
Delta R.T.: -0.005 min
Response: 42095238
Conc: 19.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

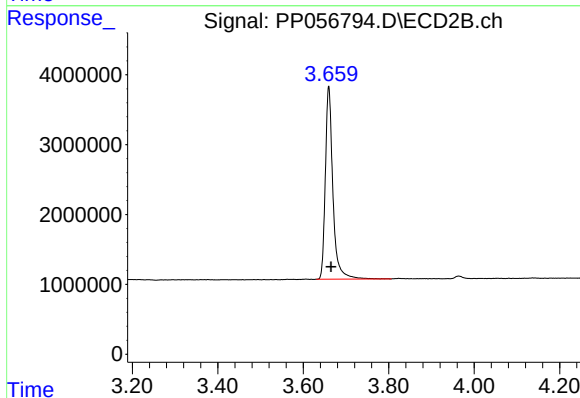


#1 Tetrachloro-m-xylene

R.T.: 3.660 min
Delta R.T.: -0.005 min
Response: 33726748
Conc: 19.39 ng/ml

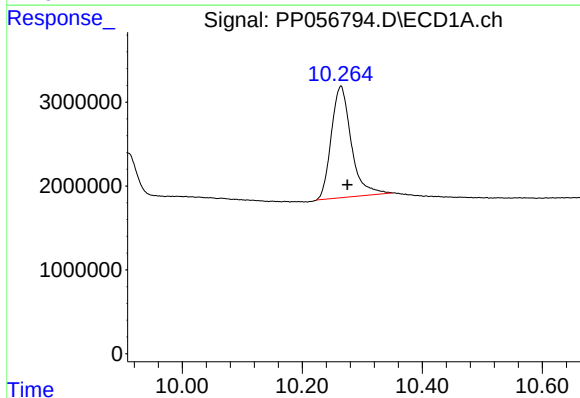


#2 Decachlorobiphenyl

R.T.: 10.265 min
Delta R.T.: -0.010 min
Response: 30786963
Conc: 23.52 ng/ml

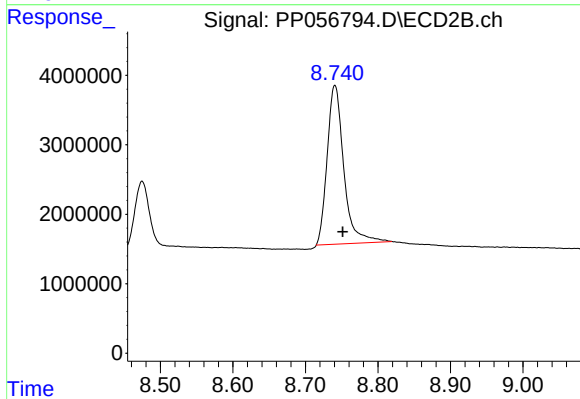

#2 Decachlorobiphenyl


R.T.: 8.741 min
Delta R.T.: -0.011 min
Response: 36619123
Conc: 23.29 ng/ml

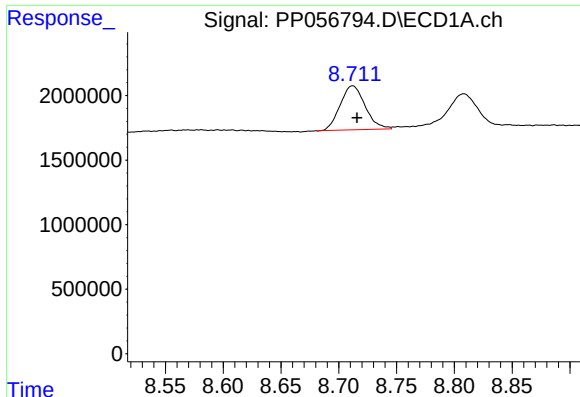

#41 AR-1268-1


R.T.: 8.712 min
Delta R.T.: -0.004 min
Response: 5133053
Conc: 27.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

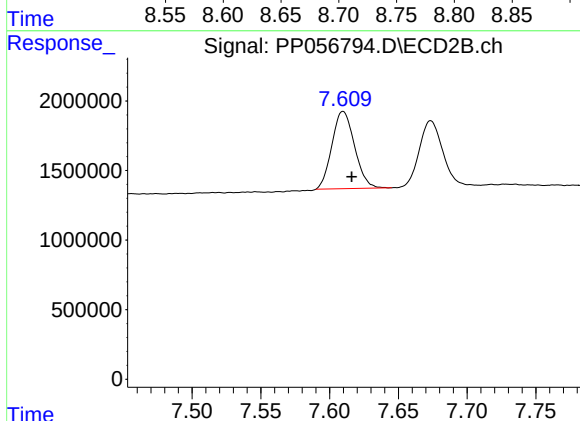


#41 AR-1268-1

R.T.: 7.610 min
Delta R.T.: -0.006 min
Response: 6374920
Conc: 28.76 ng/ml

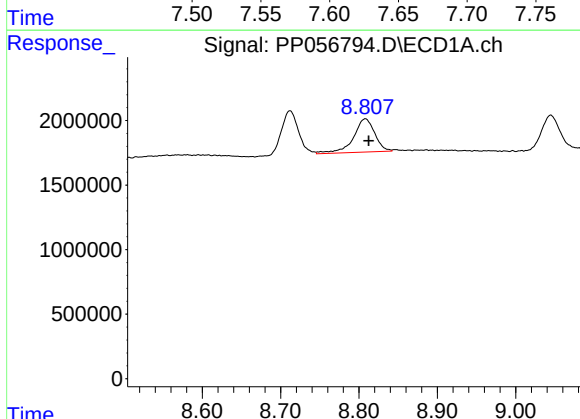


#42 AR-1268-2

R.T.: 8.808 min
Delta R.T.: -0.004 min
Response: 4896656
Conc: 29.51 ng/ml

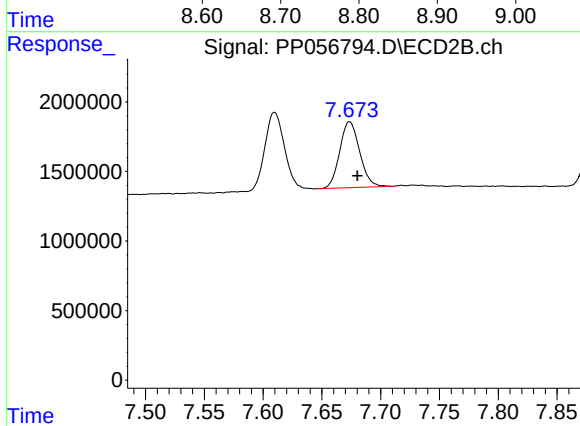

#42 AR-1268-2


R.T.: 7.674 min
Delta R.T.: -0.007 min
Response: 5589537
Conc: 28.78 ng/ml

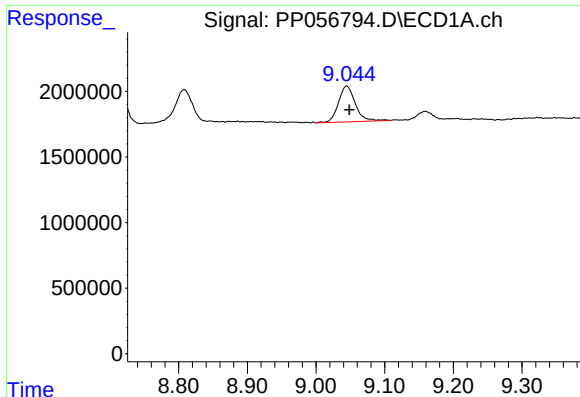

#43 AR-1268-3


R.T.: 9.045 min
Delta R.T.: -0.004 min
Response: 4688480
Conc: 29.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

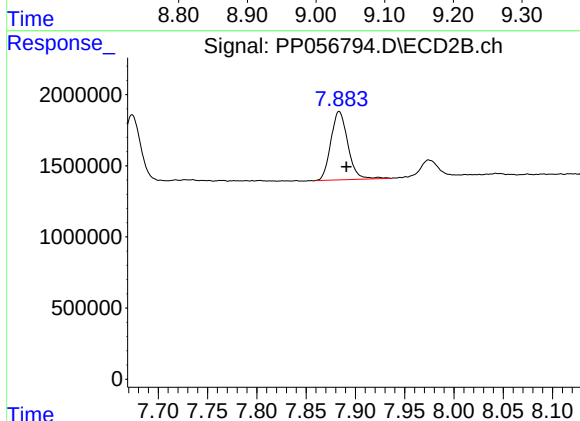


#43 AR-1268-3

R.T.: 7.884 min
Delta R.T.: -0.007 min
Response: 5770288
Conc: 29.11 ng/ml

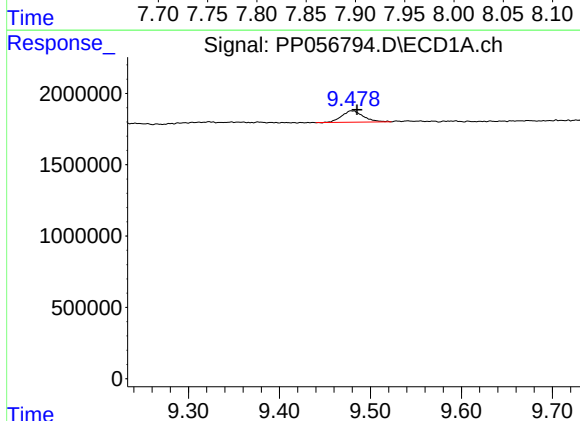


#44 AR-1268-4

R.T.: 9.480 min
Delta R.T.: -0.006 min
Response: 1320192
Conc: 28.43 ng/ml

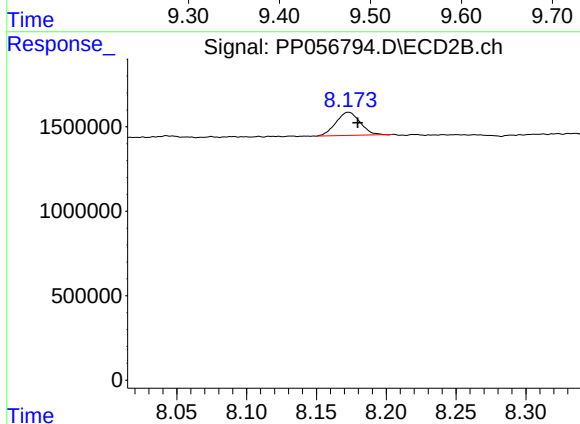

#44 AR-1268-4


R.T.: 8.173 min
Delta R.T.: -0.007 min
Response: 1653041
Conc: 28.58 ng/ml

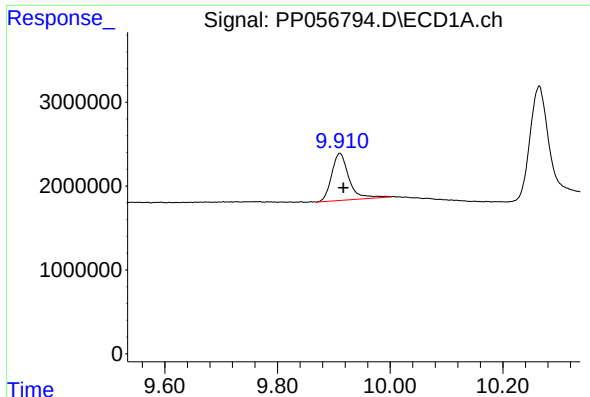

#45 AR-1268-5

R.T.: 9.911 min
Delta R.T.: -0.006 min
Response: 11981368
Conc: 27.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2023

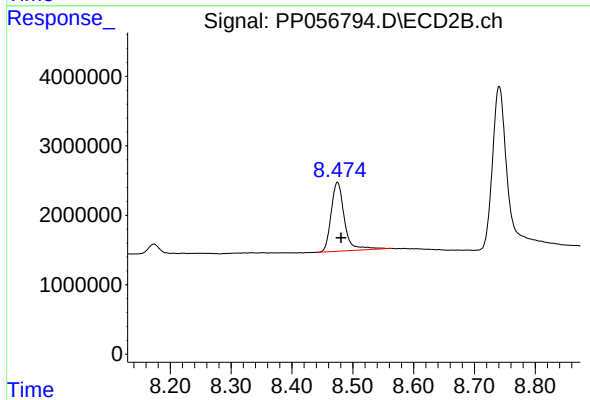

#45 AR-1268-5

R.T.: 8.475 min
Delta R.T.: -0.006 min
Response: 15179759
Conc: 29.89 ng/ml