

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040822\
 Data File : PP045713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2022 01:00
 Operator : YP\AJ
 Sample : N2314-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 149TH-ST-STATION-DRUM-4-PPE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/09/2022
 Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 02:37:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 31 07:54:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.882	3.144	60671463	44175497	25.146m	27.918
2) SA Decachlor...	9.991	8.489	43147238	36069345	30.113	23.786

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040822\
Data File : PP045713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2022 01:00
Operator : YP\AJ
Sample : N2314-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
149TH-ST-STATION-DRUM-4-PPE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/09/2022
Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 02:37:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 31 07:54:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

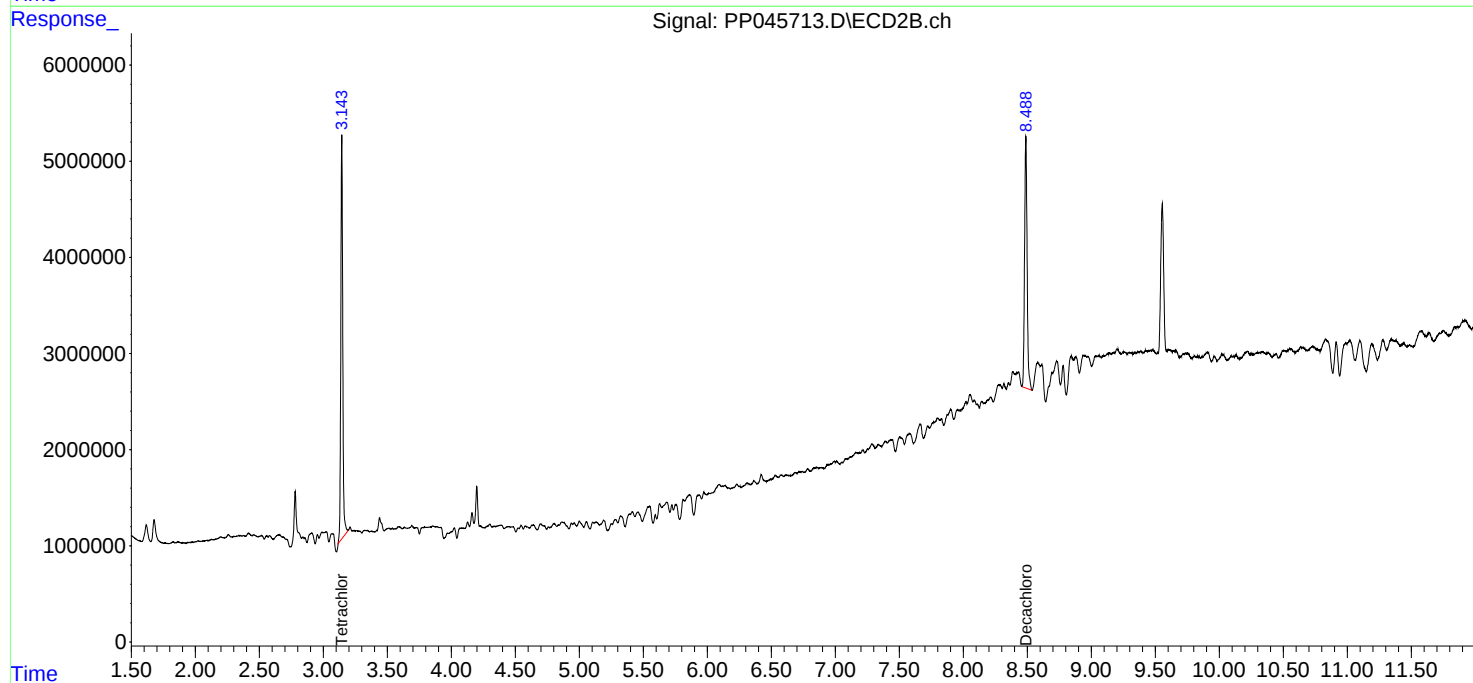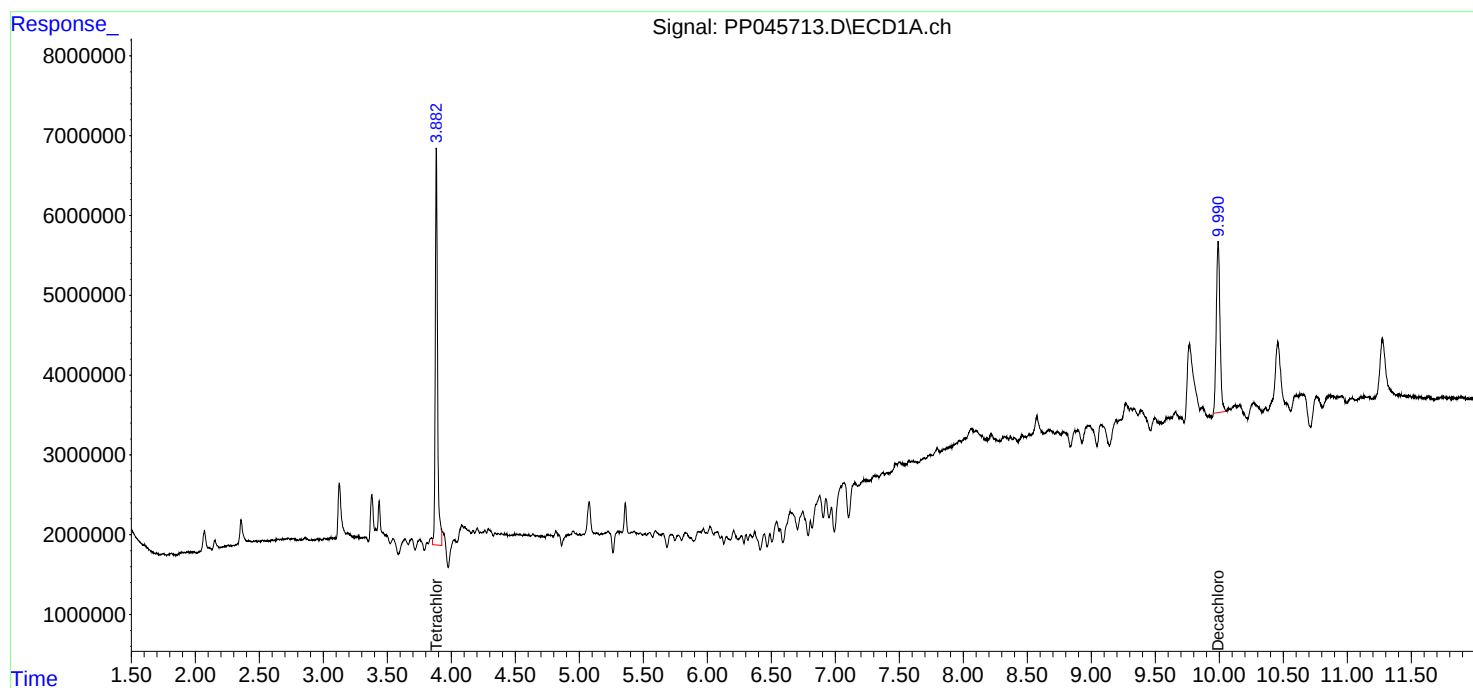

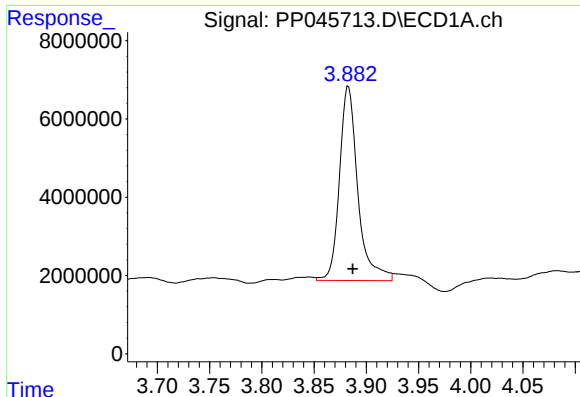


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: -0.005 min
Response: 60671463
Conc: 25.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
149TH-ST-STATION-DRUM-4-PPE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/09/2022
Supervised By :mohammad ahmed 04/11/2022

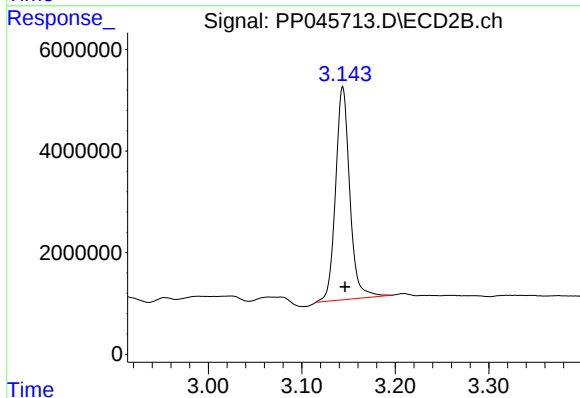


#1 Tetrachloro-m-xylene

R.T.: 3.144 min
Delta R.T.: -0.003 min
Response: 44175497
Conc: 27.92 ng/ml

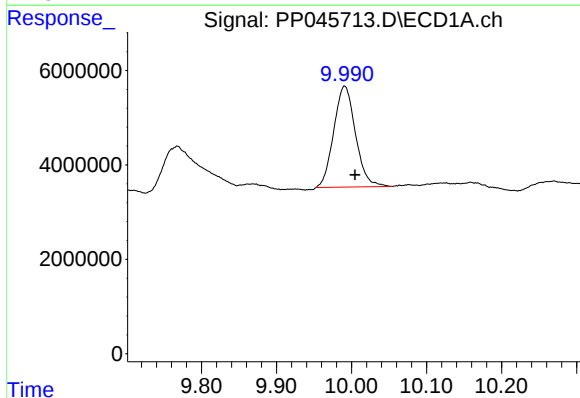

#2 Decachlorobiphenyl

R.T.: 9.991 min
Delta R.T.: -0.014 min
Response: 43147238
Conc: 30.11 ng/ml

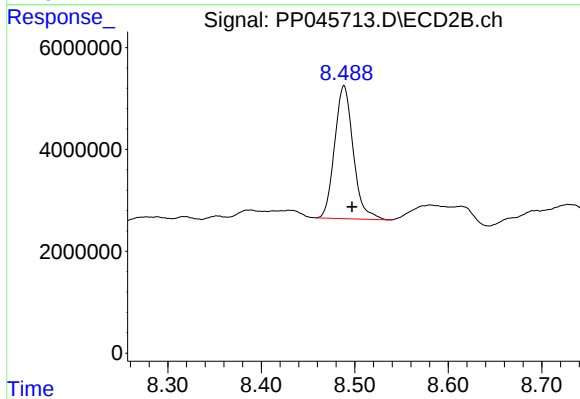

#2 Decachlorobiphenyl

R.T.: 8.489 min
Delta R.T.: -0.009 min
Response: 36069345
Conc: 23.79 ng/ml