

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040822\
 Data File : PP045778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2022 03:00
 Operator : YP\AJ
 Sample : N2337-02
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B250-CU

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/11/2022
 Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 02:24:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 09 07:55:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.882	3.142	41755709	28997389	17.306	18.326
2) SA Decachlor...	9.985	8.483	16822637	15478578	11.741m	10.207
Target Compounds						
26) L6 AR-1254-1	6.057	5.130	4374025	5643726	61.435	57.997
27) L6 AR-1254-2	6.294	5.289	6052868	3795397	56.033	46.539
28) L6 AR-1254-3	6.693	5.720	5834513	6975403	52.620	56.418
29) L6 AR-1254-4	7.006	5.968	3335620	3698419	41.501	46.125
30) L6 AR-1254-5	7.468	6.418	4260063	14287004	53.276	130.767 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040822\
Data File : PP045778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2022 03:00
Operator : YP\AJ
Sample : N2337-02
Misc :
ALS Vial : 73 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
B250-CU


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 02:24:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 09 07:55:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

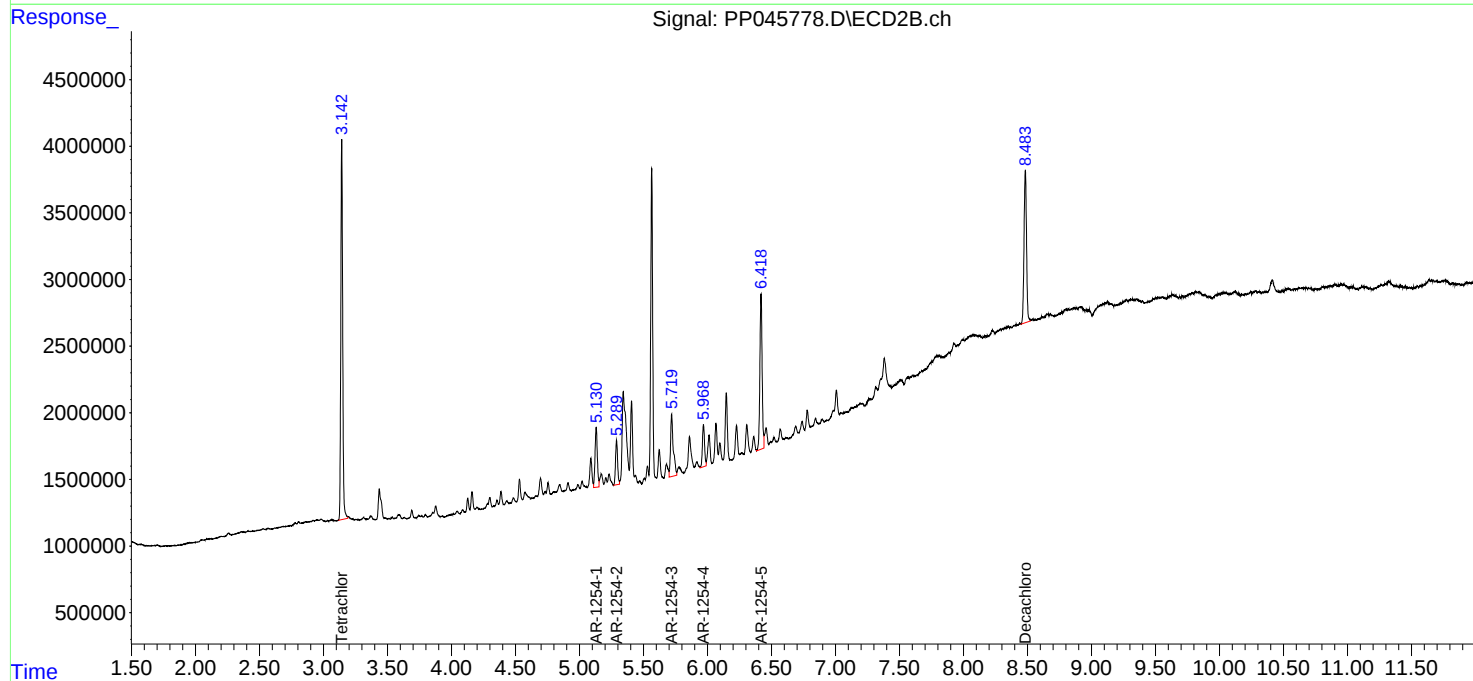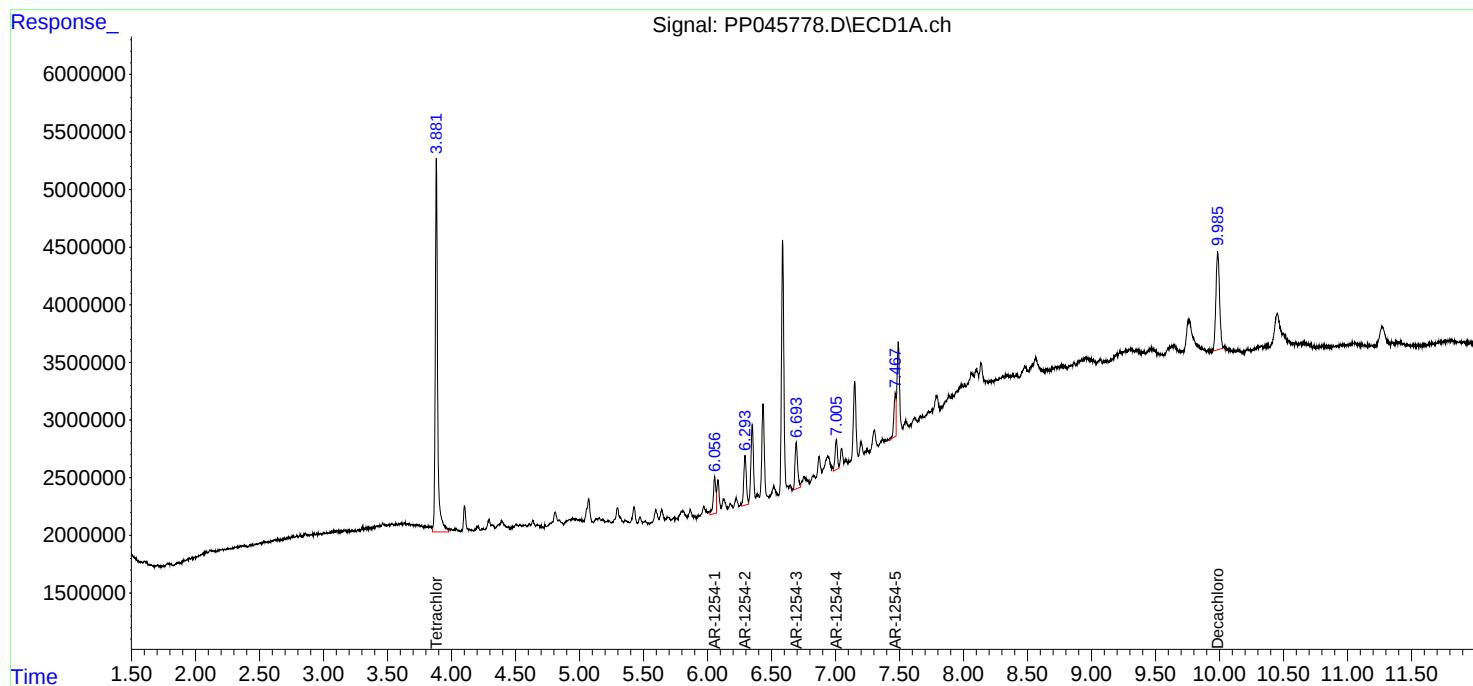

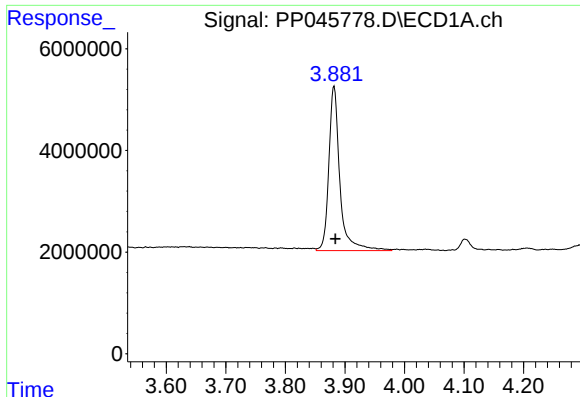


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: -0.002 min
Response: 41755709
Conc: 17.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
B250-CU


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

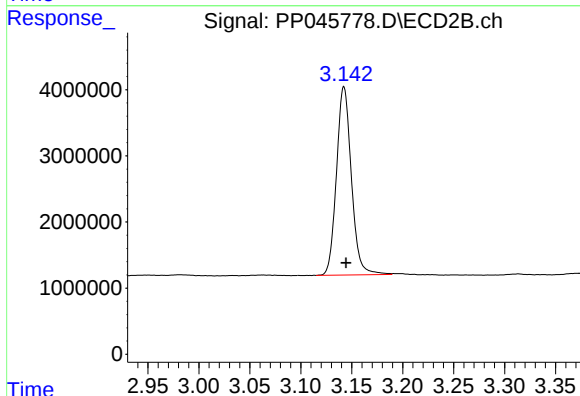


#1 Tetrachloro-m-xylene

R.T.: 3.142 min
Delta R.T.: -0.002 min
Response: 28997389
Conc: 18.33 ng/ml

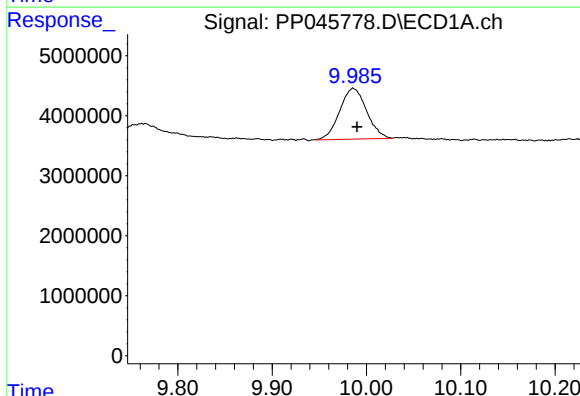


#2 Decachlorobiphenyl

R.T.: 9.985 min
Delta R.T.: -0.005 min
Response: 16822637
Conc: 11.74 ng/ml m

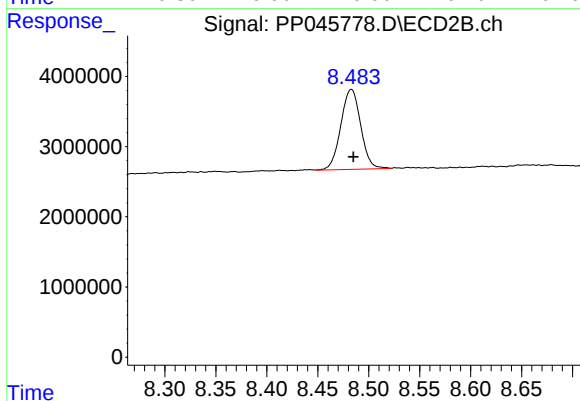

#2 Decachlorobiphenyl

R.T.: 8.483 min
Delta R.T.: -0.002 min
Response: 15478578
Conc: 10.21 ng/ml

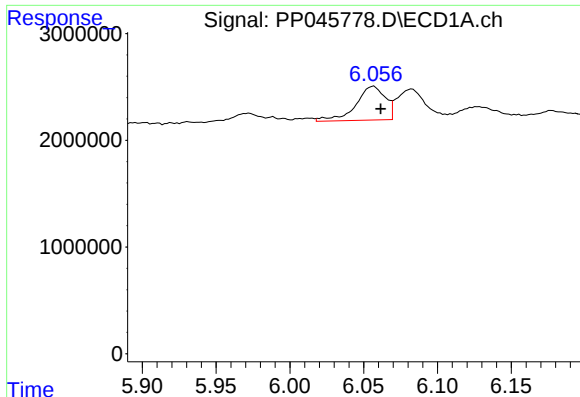


#26 AR-1254-1

R.T.: 6.057 min
Delta R.T.: -0.005 min
Response: 4374025
Conc: 61.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
B250-CU


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

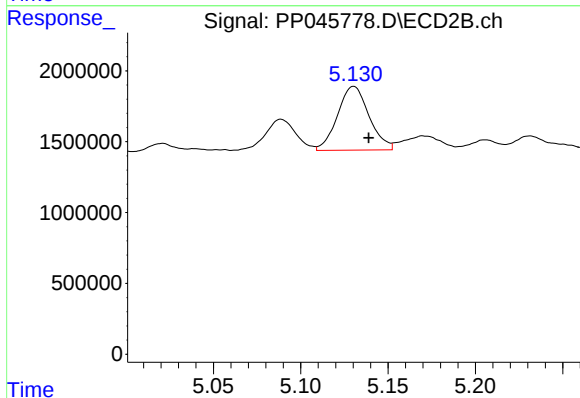


#26 AR-1254-1

R.T.: 5.130 min
Delta R.T.: -0.008 min
Response: 5643726
Conc: 58.00 ng/ml

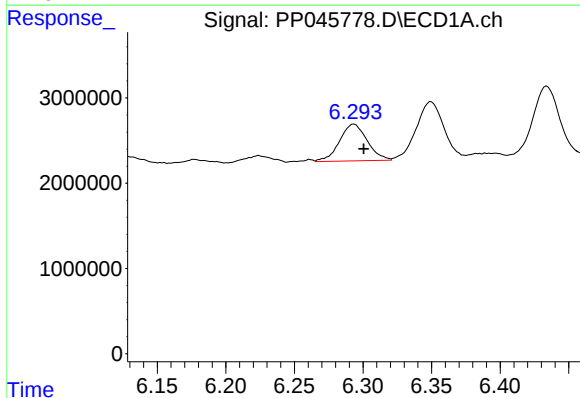


#27 AR-1254-2

R.T.: 6.294 min
Delta R.T.: -0.007 min
Response: 6052868
Conc: 56.03 ng/ml

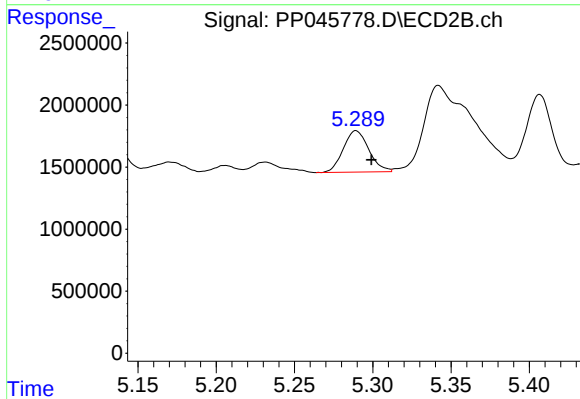

#27 AR-1254-2

R.T.: 5.289 min
Delta R.T.: -0.010 min
Response: 3795397
Conc: 46.54 ng/ml

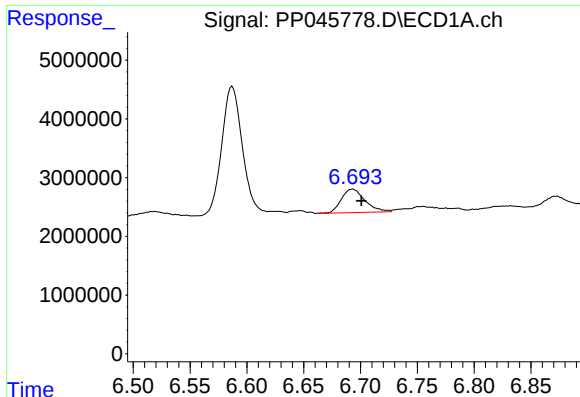


#28 AR-1254-3

R.T.: 6.693 min
Delta R.T.: -0.008 min
Response: 5834513
Conc: 52.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
B250-CU


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

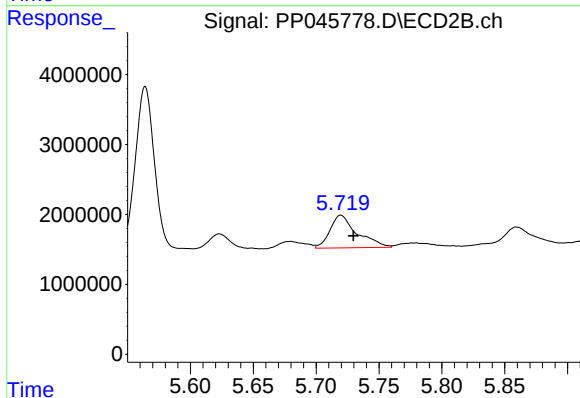


#28 AR-1254-3

R.T.: 5.720 min
Delta R.T.: -0.010 min
Response: 6975403
Conc: 56.42 ng/ml

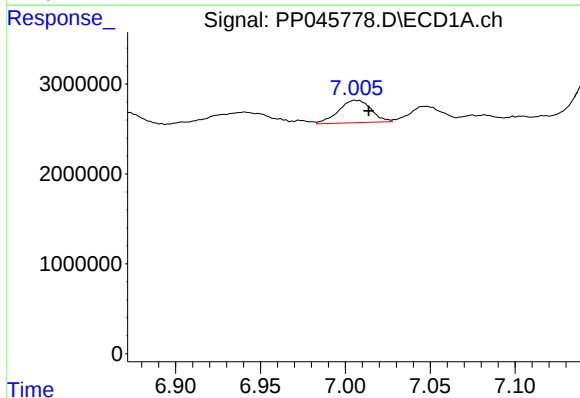


#29 AR-1254-4

R.T.: 7.006 min
Delta R.T.: -0.007 min
Response: 3335620
Conc: 41.50 ng/ml

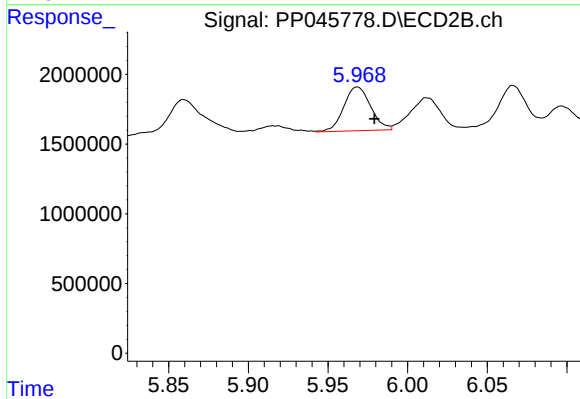

#29 AR-1254-4

R.T.: 5.968 min
Delta R.T.: -0.011 min
Response: 3698419
Conc: 46.13 ng/ml

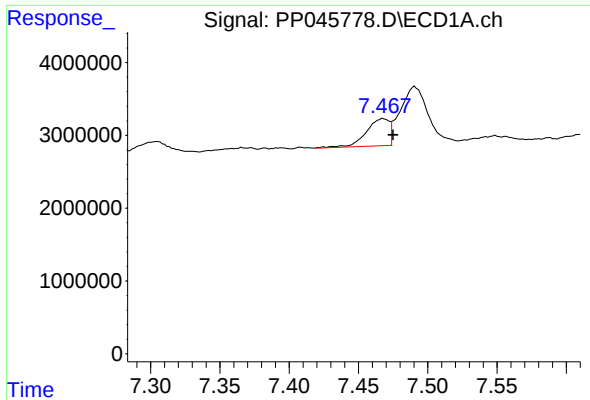


#30 AR-1254-5

R.T.: 7.468 min
Delta R.T.: -0.007 min
Response: 4260063
Conc: 53.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
B250-CU

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

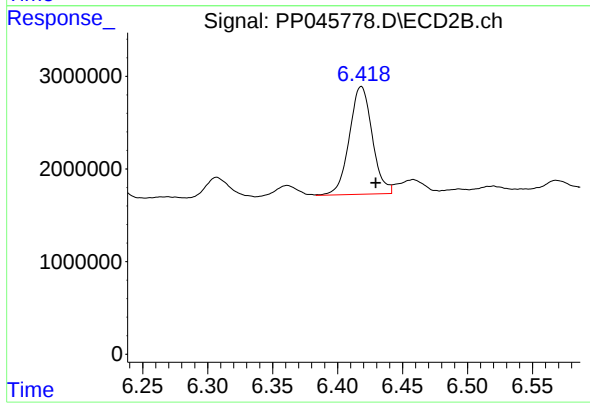

#30 AR-1254-5

R.T.: 6.418 min
Delta R.T.: -0.011 min
Response: 14287004
Conc: 130.77 ng/ml