

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040822\
 Data File : PP045801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2022 11:33
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

04/11/2022
 Supervised By :mohammad
 ahmed

04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 06:13:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 09 07:55:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.881	3.142	61652397	41400343	25.552	26.164
2) SA Decachlor...	9.985	8.482	36551576	35858926	25.510m	23.647

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040822\
Data File : PP045801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2022 11:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Manual Integrations
APPROVED



Reviewed By :Yogesh
Patel


04/11/2022
Supervised By :mohammad
ahmed

04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 06:13:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 09 07:55:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

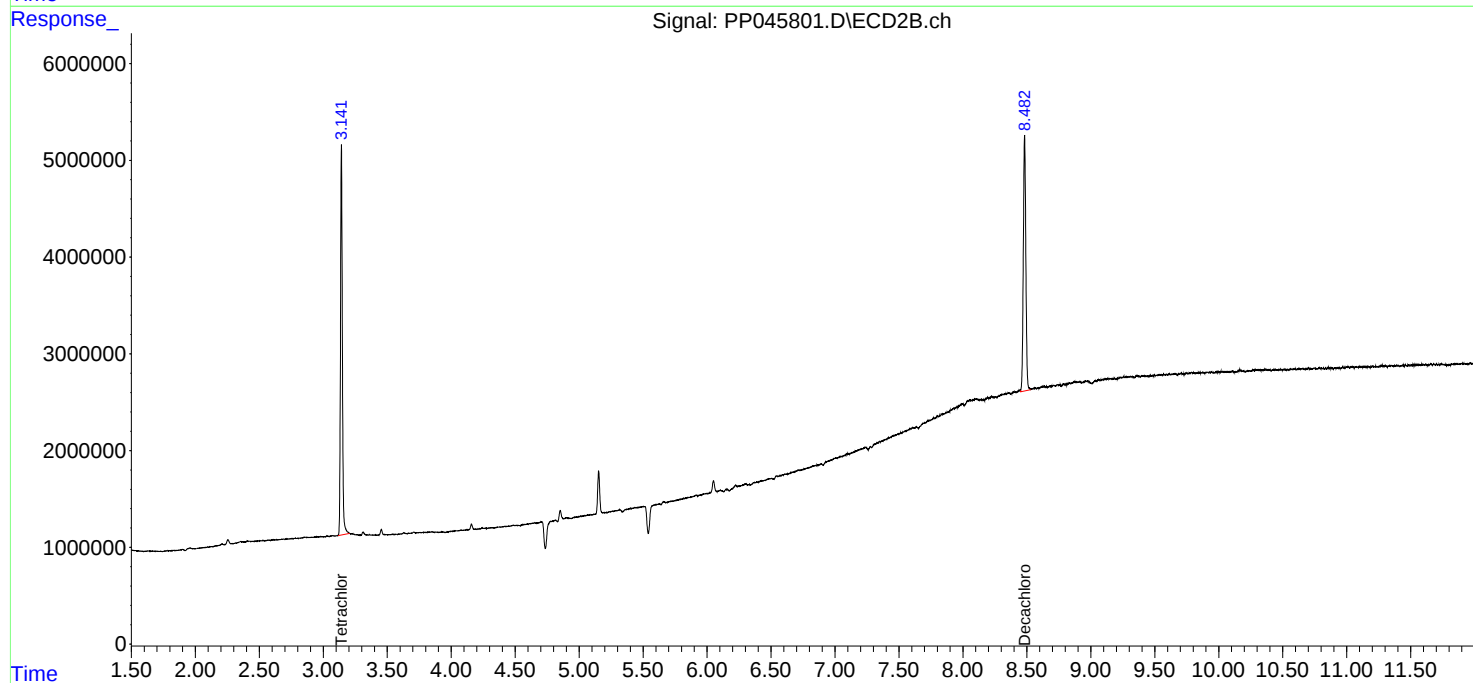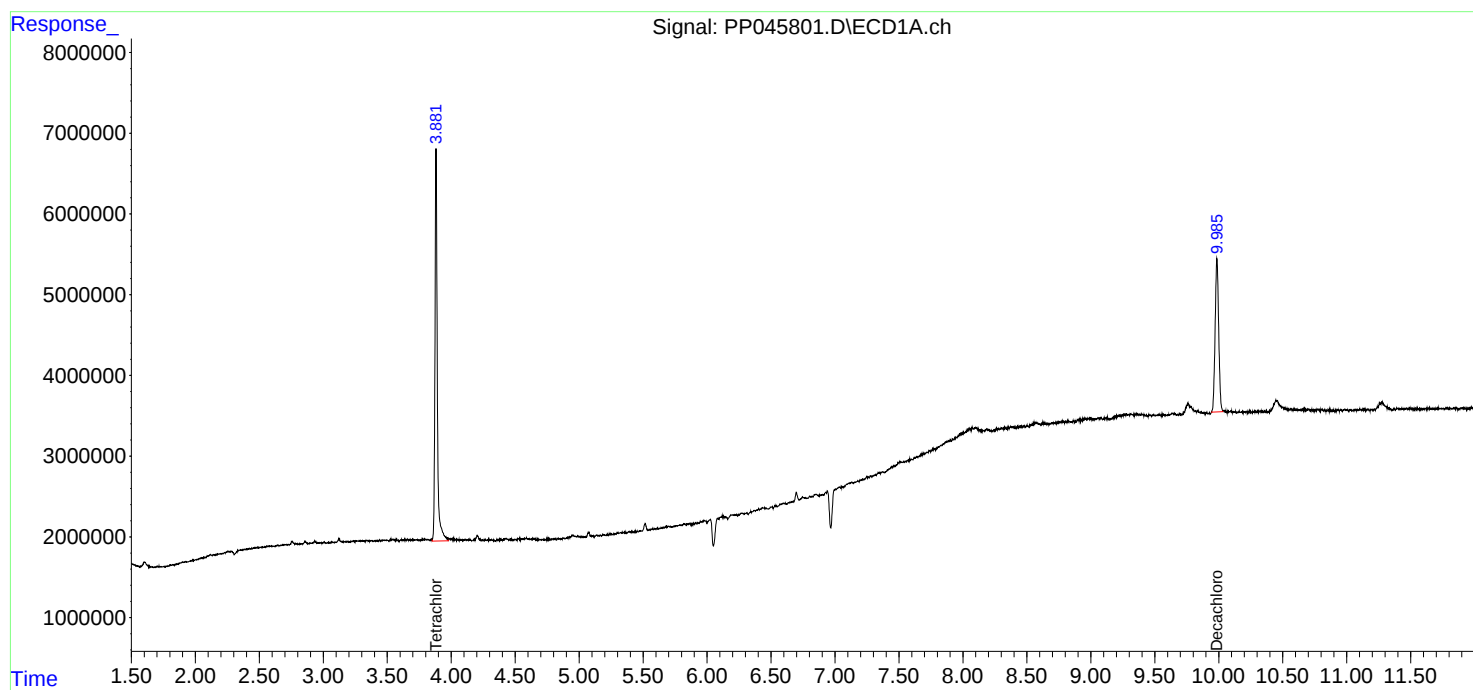

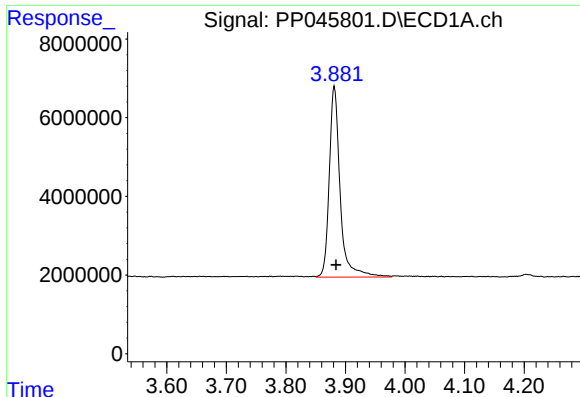

#1 Tetrachloro-m-xylene

R.T.: 3.881 min
Delta R.T.: -0.003 min
Response: 61652397
Conc: 25.55 ng/ml


Instrument :
ECD_P
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel


04/11/2022
Supervised By :mohammad
ahmed

04/11/2022

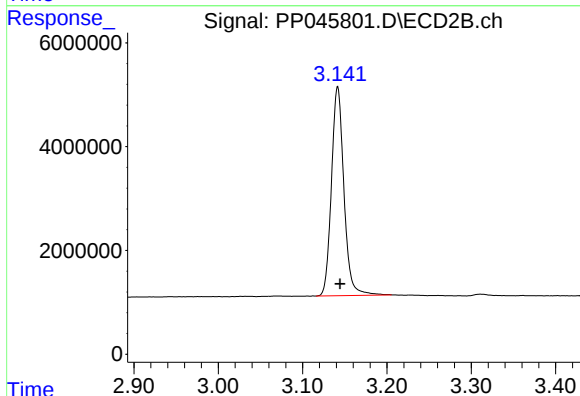


#1 Tetrachloro-m-xylene

R.T.: 3.142 min
Delta R.T.: -0.003 min
Response: 41400343
Conc: 26.16 ng/ml

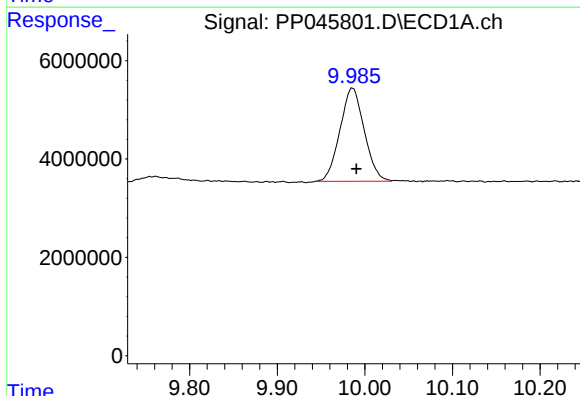

#2 Decachlorobiphenyl

R.T.: 9.985 min
Delta R.T.: -0.005 min
Response: 36551576
Conc: 25.51 ng/ml m

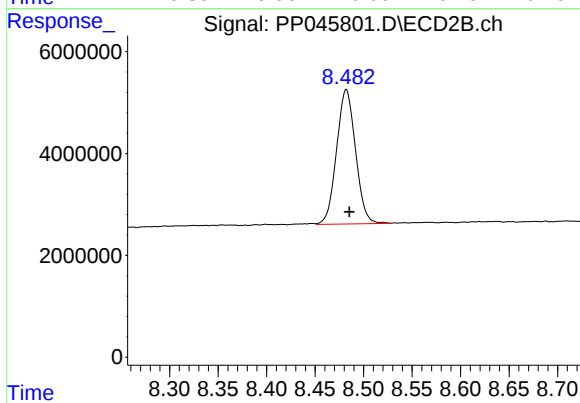

#2 Decachlorobiphenyl

R.T.: 8.482 min
Delta R.T.: -0.003 min
Response: 35858926
Conc: 23.65 ng/ml