

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040824\
 Data File : PP064174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2024 18:04
 Operator : YP\AJ
 Sample : P2019-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NB205-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 21:41:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.636	40850365	40912792	17.120	17.136
2) SA Decachlor...	10.349	8.664	33016571	32453785	13.004	12.009
Target Compounds						
9) L2 AR-1221-2	0.000	3.935	0	742499	N.D.	36.230 #
33) L7 AR-1260-3	0.000	6.544f	0	403248	N.D.	2.509 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040824\
Data File : PP064174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2024 18:04
Operator : YP\AJ
Sample : P2019-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
NB205-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 21:41:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

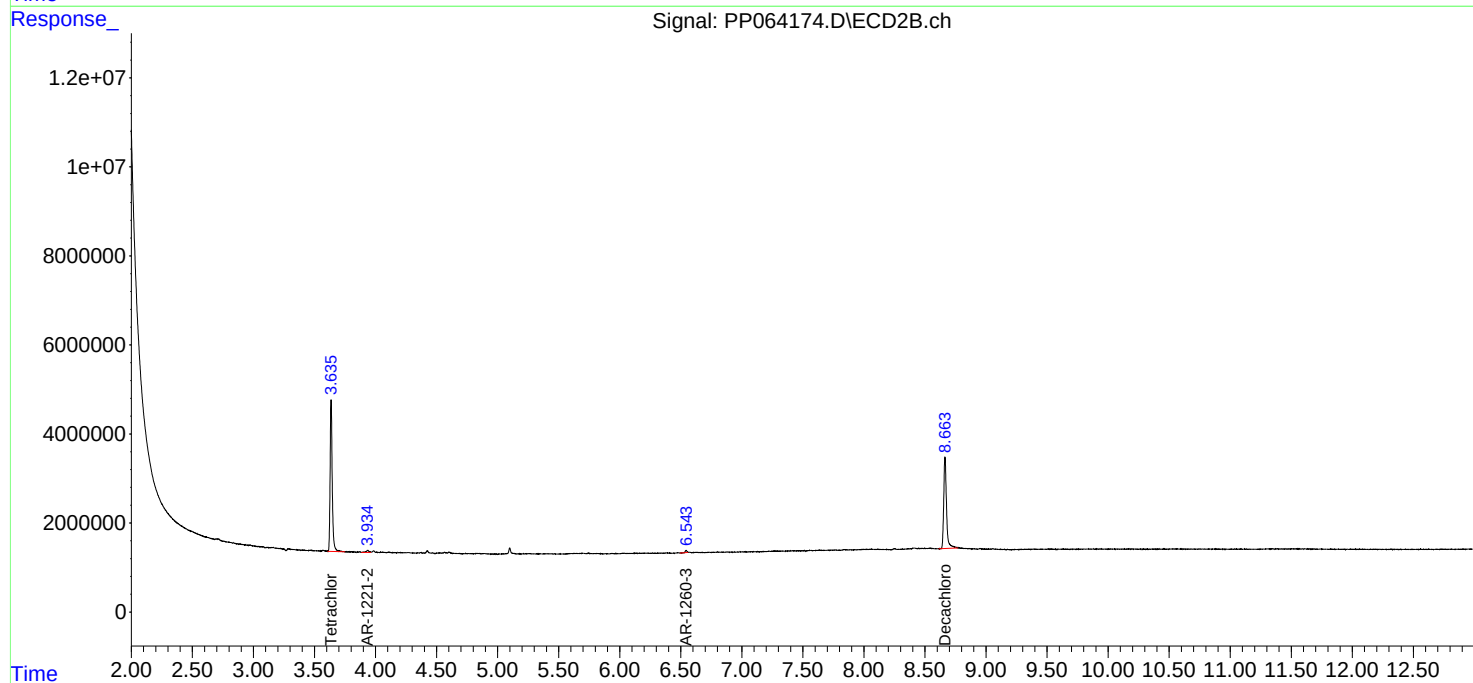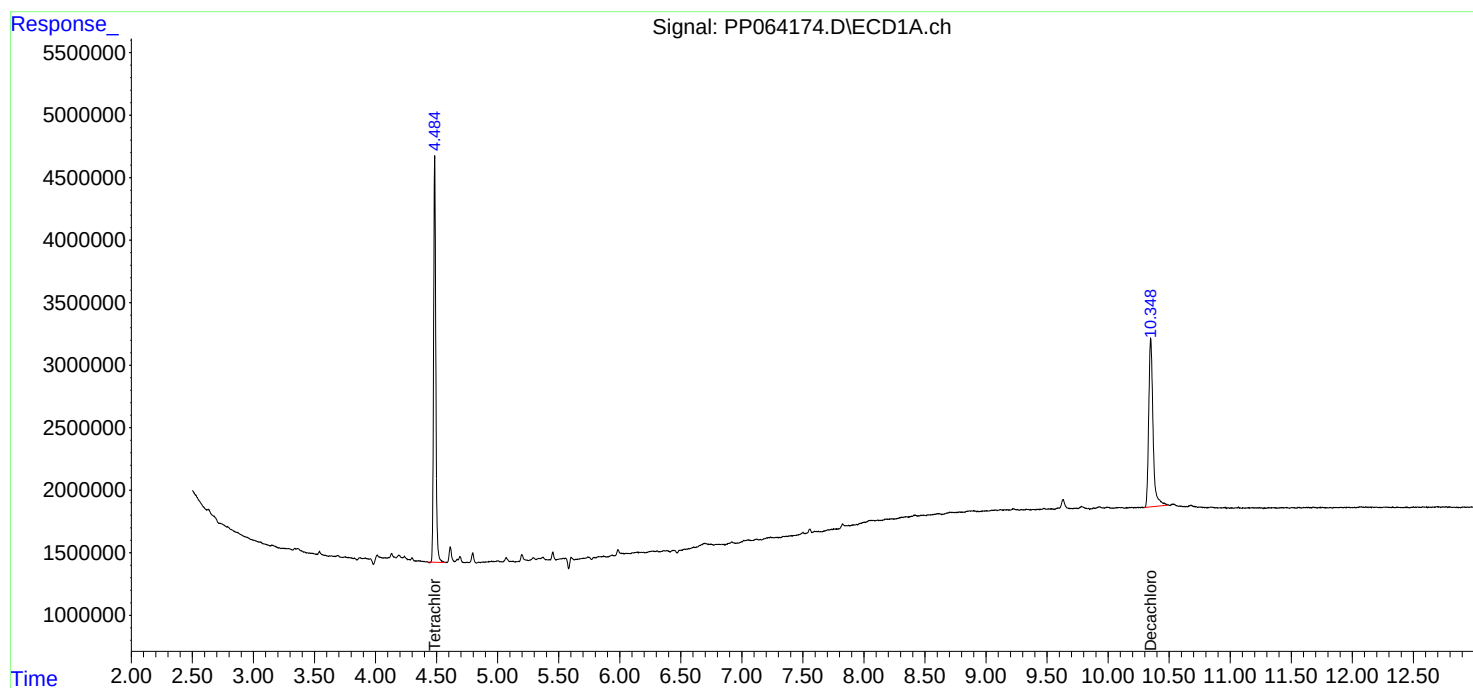


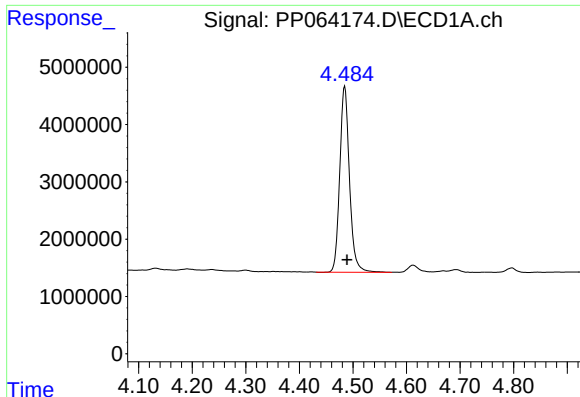

#1 Tetrachloro-m-xylene


R.T.: 4.485 min
Delta R.T.: -0.004 min
Response: 40850365
Conc: 17.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
NB205-WATER

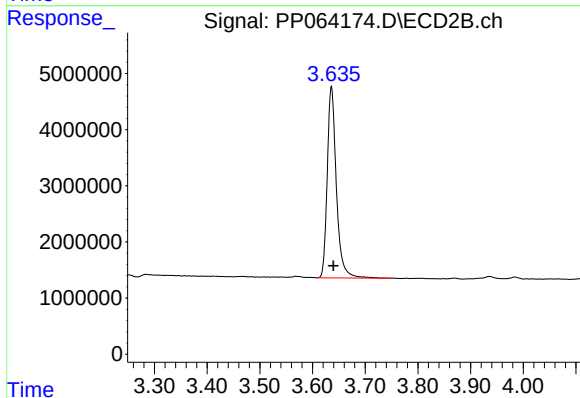


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.003 min
Response: 40912792
Conc: 17.14 ng/ml

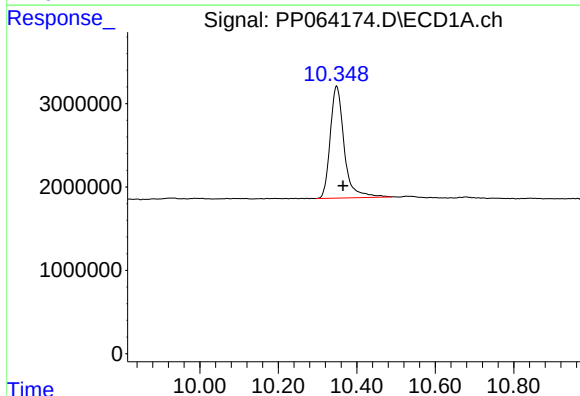


#2 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: -0.017 min
Response: 33016571
Conc: 13.00 ng/ml

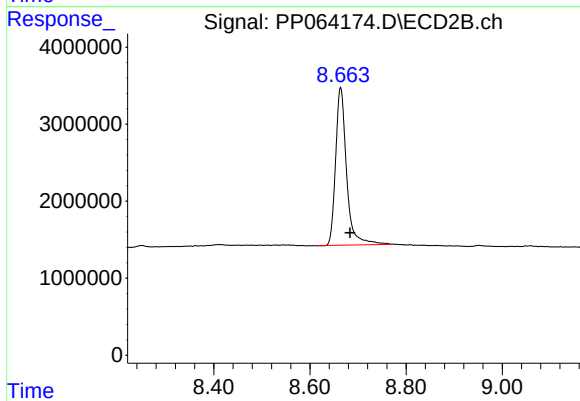

#2 Decachlorobiphenyl


R.T.: 8.664 min
Delta R.T.: -0.020 min
Response: 32453785
Conc: 12.01 ng/ml

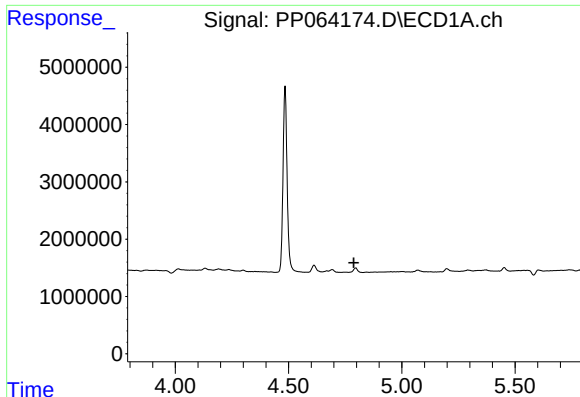

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
NB205-WATER

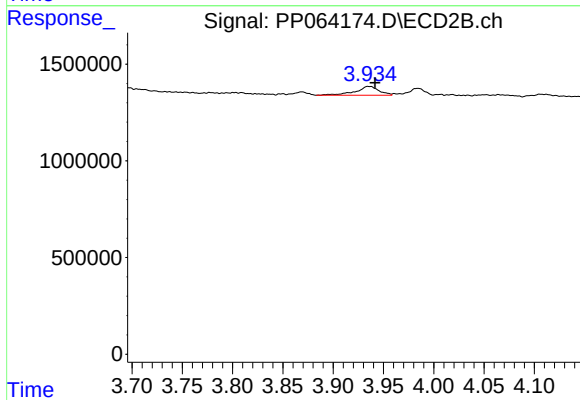


#9 AR-1221-2

R.T.: 3.935 min
Delta R.T.: -0.006 min
Response: 742499
Conc: 36.23 ng/ml

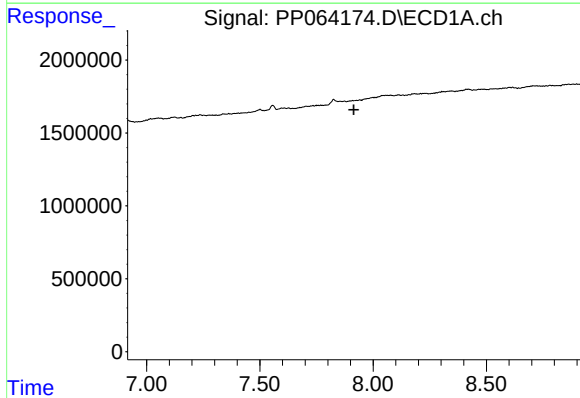

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.915 min
Response: 0
Conc: N.D.

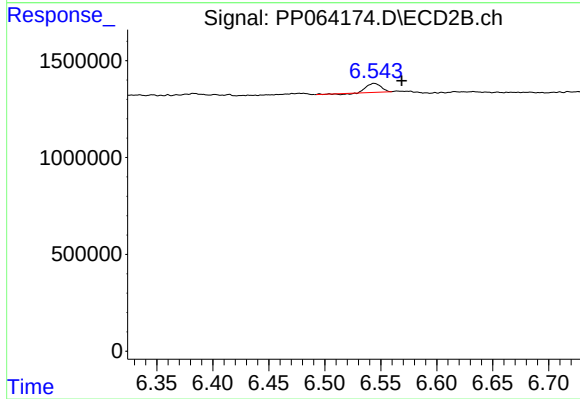

#33 AR-1260-3

R.T.: 6.544 min
Delta R.T.: -0.025 min
Response: 403248
Conc: 2.51 ng/ml