

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040921\
 Data File : PP034760.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2021 10:47
 Operator : DD\AJ
 Sample : M1946-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FS-SB10

Manual Integrations
 APPROVED

Ankita
 4/12/2021 2:24:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 15:33:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.843	4.256	1576058	947502	20.660	21.092m
2) SA Decachlor...	10.756	9.553	1346063	554635	17.486	19.643

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040921\
Data File : PP034760.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2021 10:47
Operator : DD\AJ
Sample : M1946-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FS-SB10


Manual Integrations
APPROVED

Ankita
4/12/2021 2:24:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 15:33:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

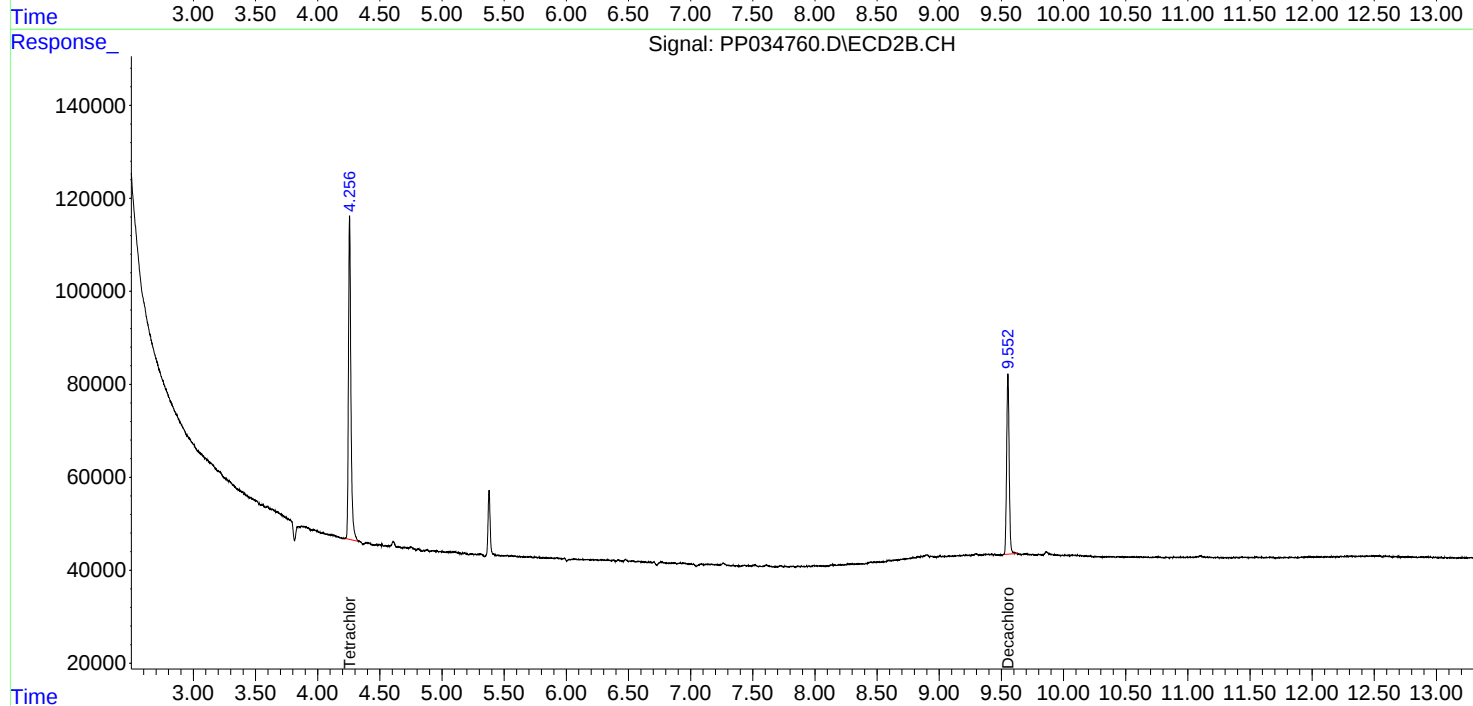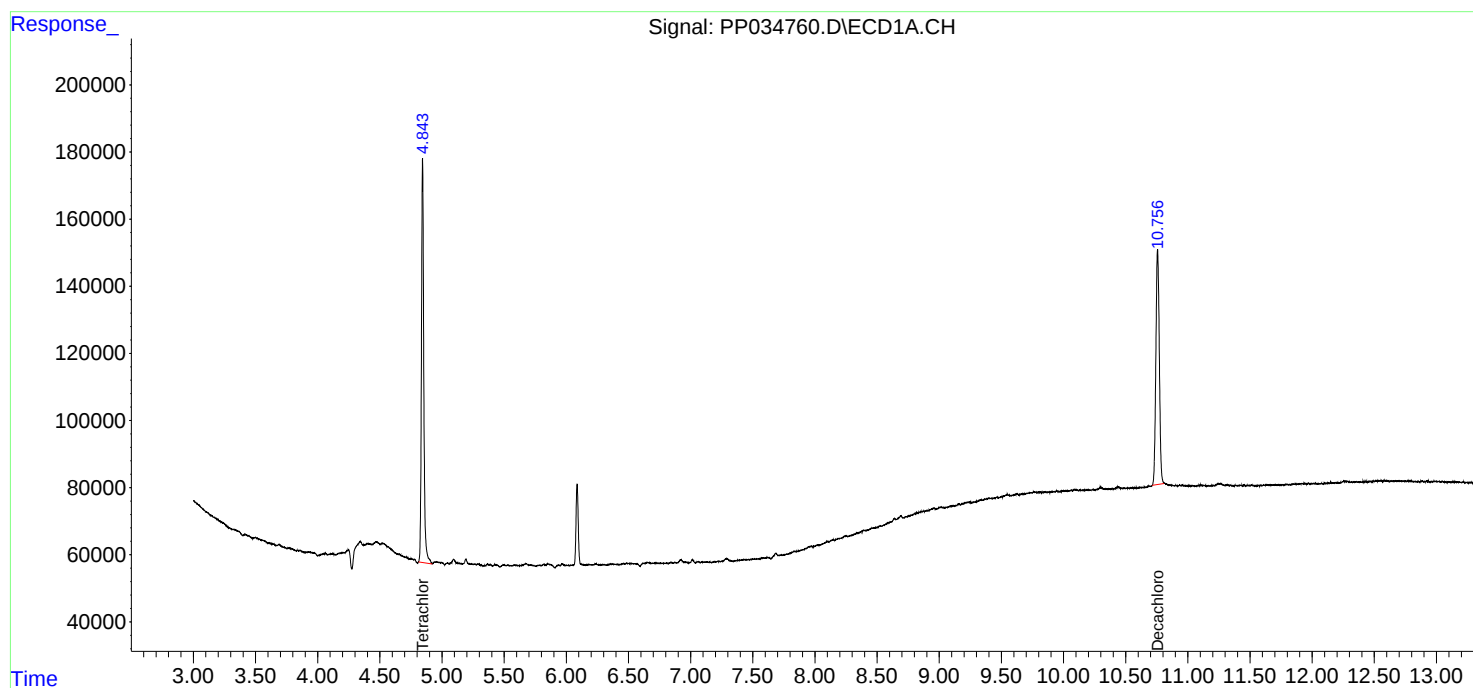

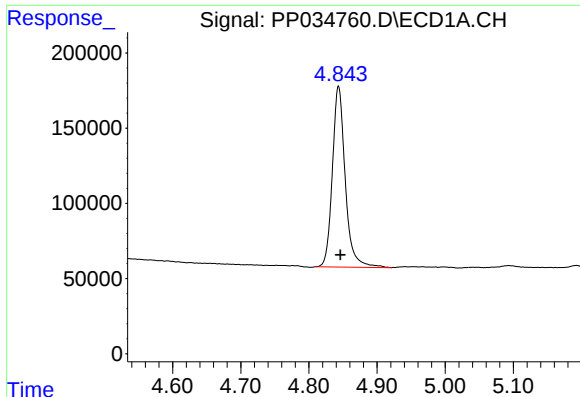


#1 Tetrachloro-m-xylene

R.T.: 4.843 min
Delta R.T.: -0.003 min
Response: 1576058
Conc: 20.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
FS-SB10


Manual Integrations
APPROVED

Ankita
4/12/2021 2:24:00 PM

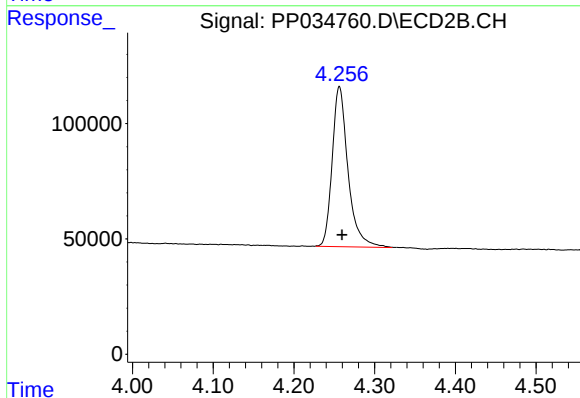


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.004 min
Response: 947502
Conc: 21.09 ng/ml m

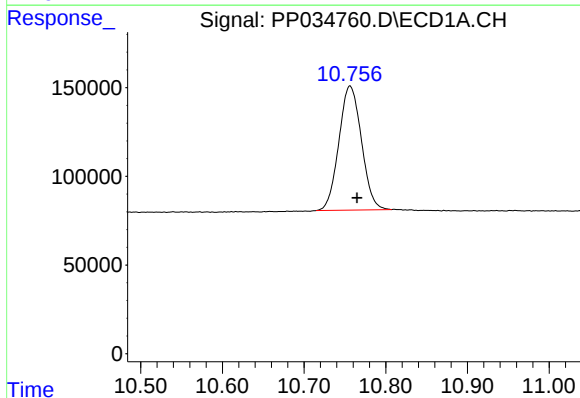

#2 Decachlorobiphenyl

R.T.: 10.756 min
Delta R.T.: -0.009 min
Response: 1346063
Conc: 17.49 ng/ml

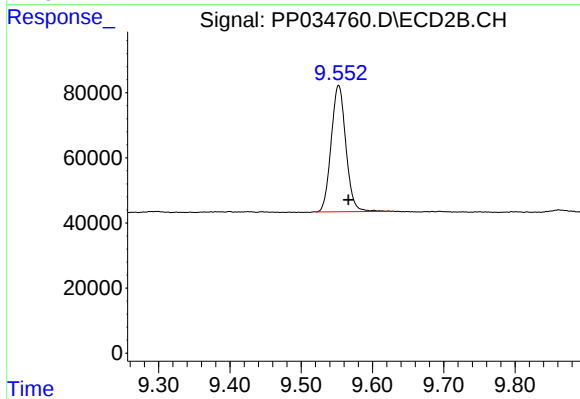

#2 Decachlorobiphenyl

R.T.: 9.553 min
Delta R.T.: -0.014 min
Response: 554635
Conc: 19.64 ng/ml