

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040924\
 Data File : PP064216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 22:42
 Operator : YP\AJ
 Sample : P2025-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TOTE-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 23:36:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.486	3.637	45424471	44949108	19.037	18.827
2) SA Decachlor...	10.351	8.664	39233260	35832331	15.452	13.259
Target Compounds						
9) L2 AR-1221-2	0.000	3.937	0	951172	N.D.	46.412 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040924\
Data File : PP064216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 22:42
Operator : YP\AJ
Sample : P2025-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 23:36:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

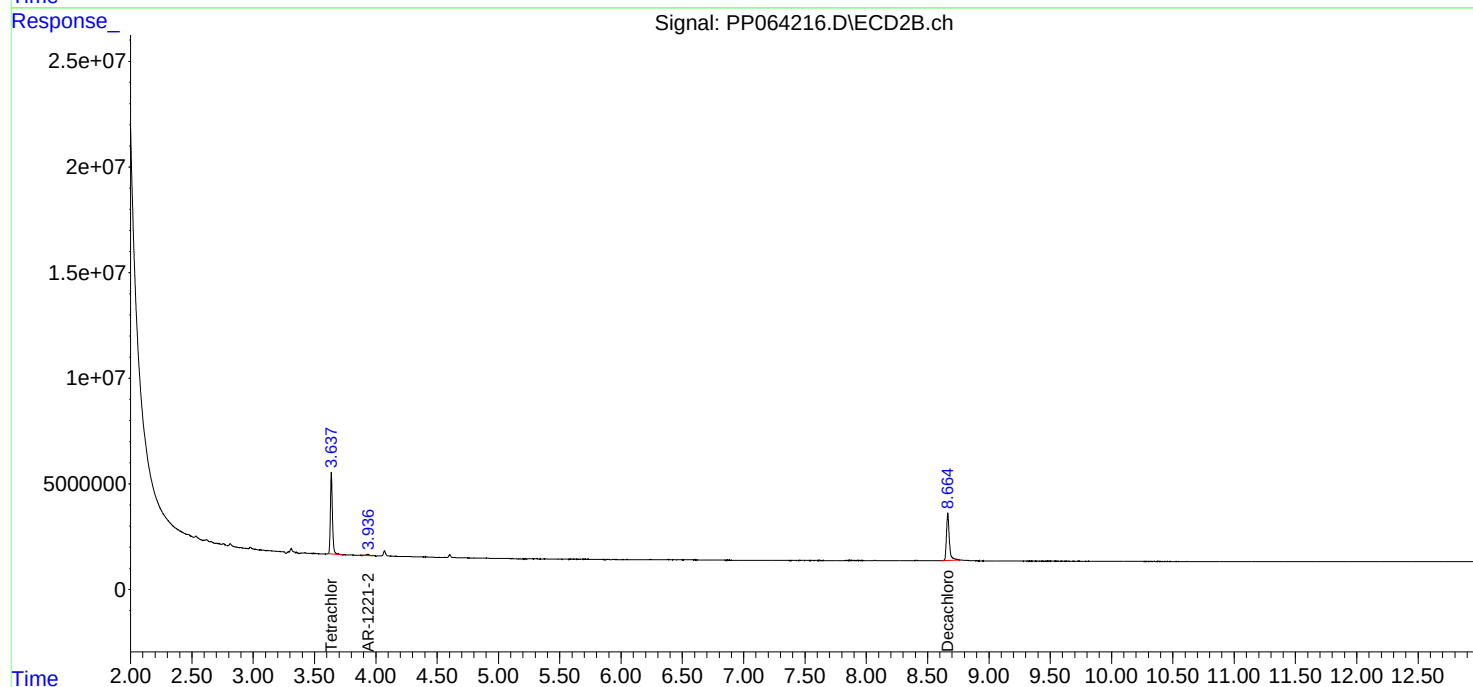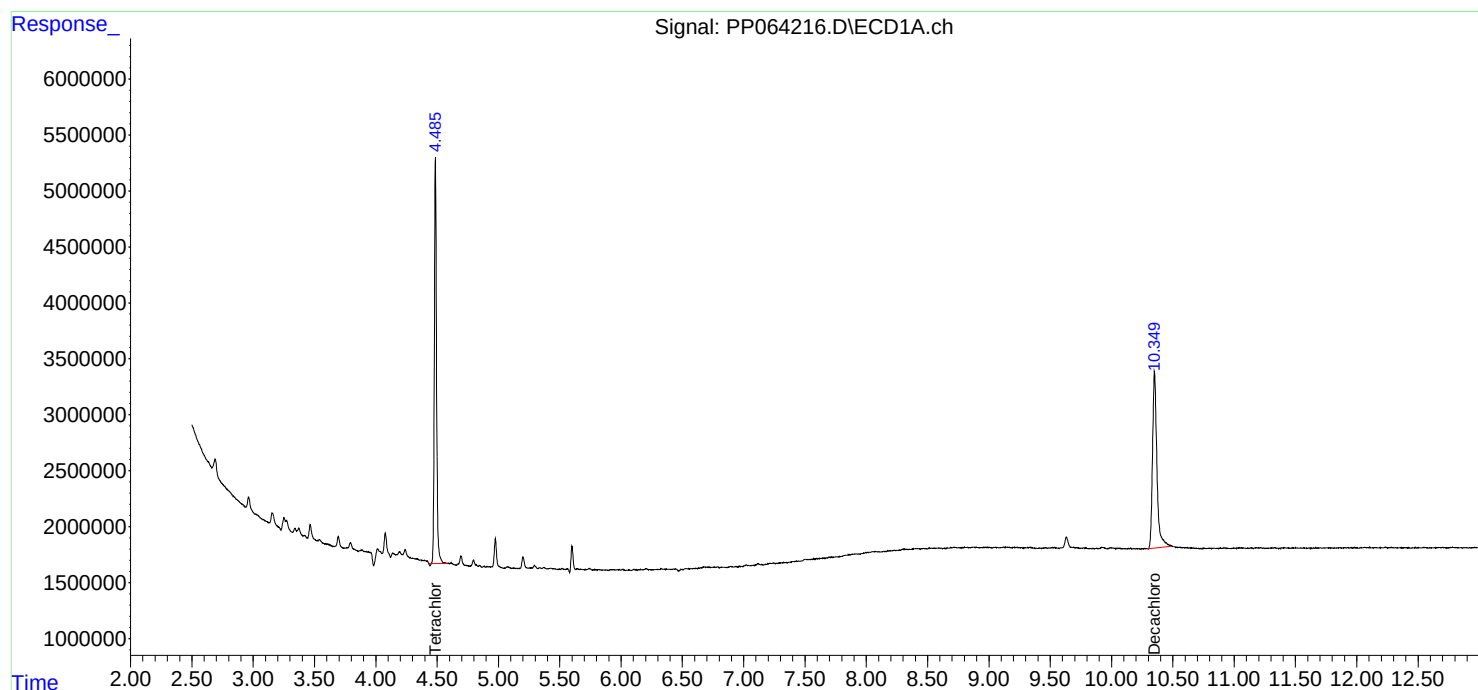


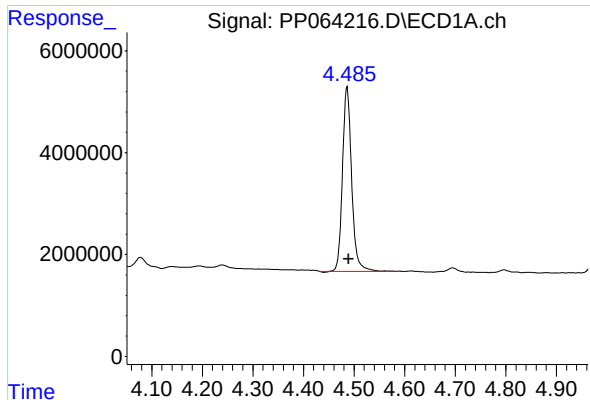

#1 Tetrachloro-m-xylene


R.T.: 4.486 min
Delta R.T.: -0.003 min
Response: 45424471
Conc: 19.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP

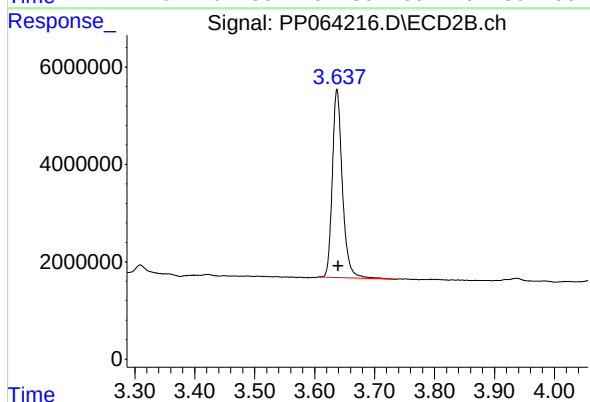


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 44949108
Conc: 18.83 ng/ml

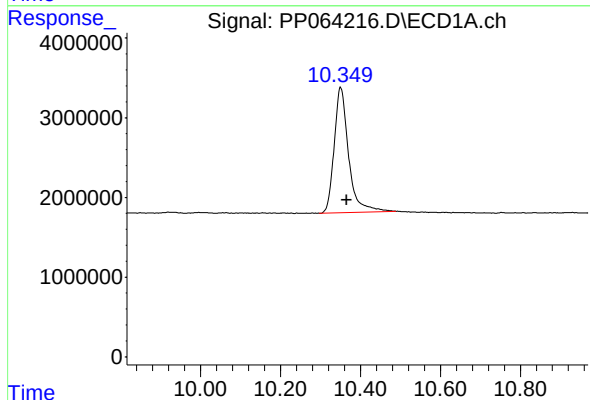


#2 Decachlorobiphenyl

R.T.: 10.351 min
Delta R.T.: -0.015 min
Response: 39233260
Conc: 15.45 ng/ml

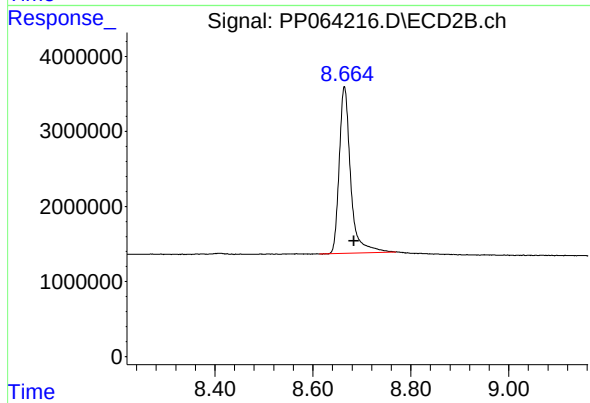

#2 Decachlorobiphenyl


R.T.: 8.664 min
Delta R.T.: -0.019 min
Response: 35832331
Conc: 13.26 ng/ml

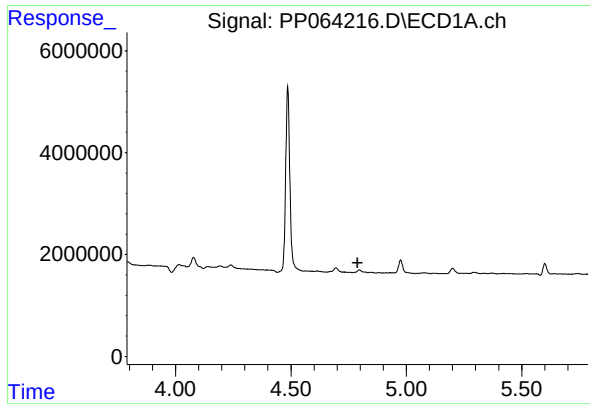

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP

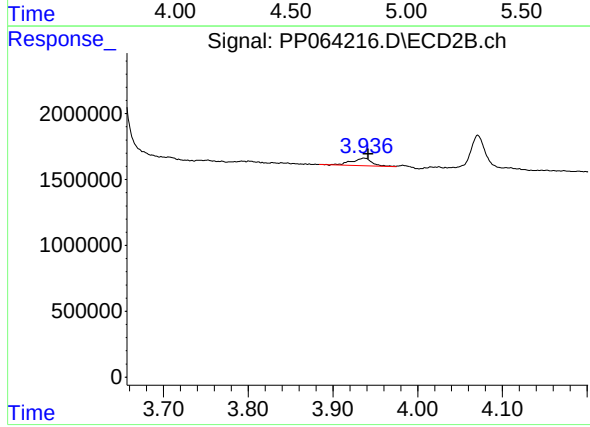

#9 AR-1221-2

R.T.: 3.937 min
Delta R.T.: -0.005 min
Response: 951172
Conc: 46.41 ng/ml