

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040924\
 Data File : PP064217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 22:58
 Operator : YP\AJ
 Sample : P2025-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TOTE-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 23:36:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.637	43572970	42969780	18.261	17.998
2) SA Decachlor...	10.350	8.664	39996357	36716630	15.753	13.586
Target Compounds						
9) L2 AR-1221-2	0.000	3.936	0	988690	N.D.	48.243 #
33) L7 AR-1260-3	0.000	6.544f	0	107729	N.D.	0.670 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040924\
Data File : PP064217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 22:58
Operator : YP\AJ
Sample : P2025-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 23:36:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

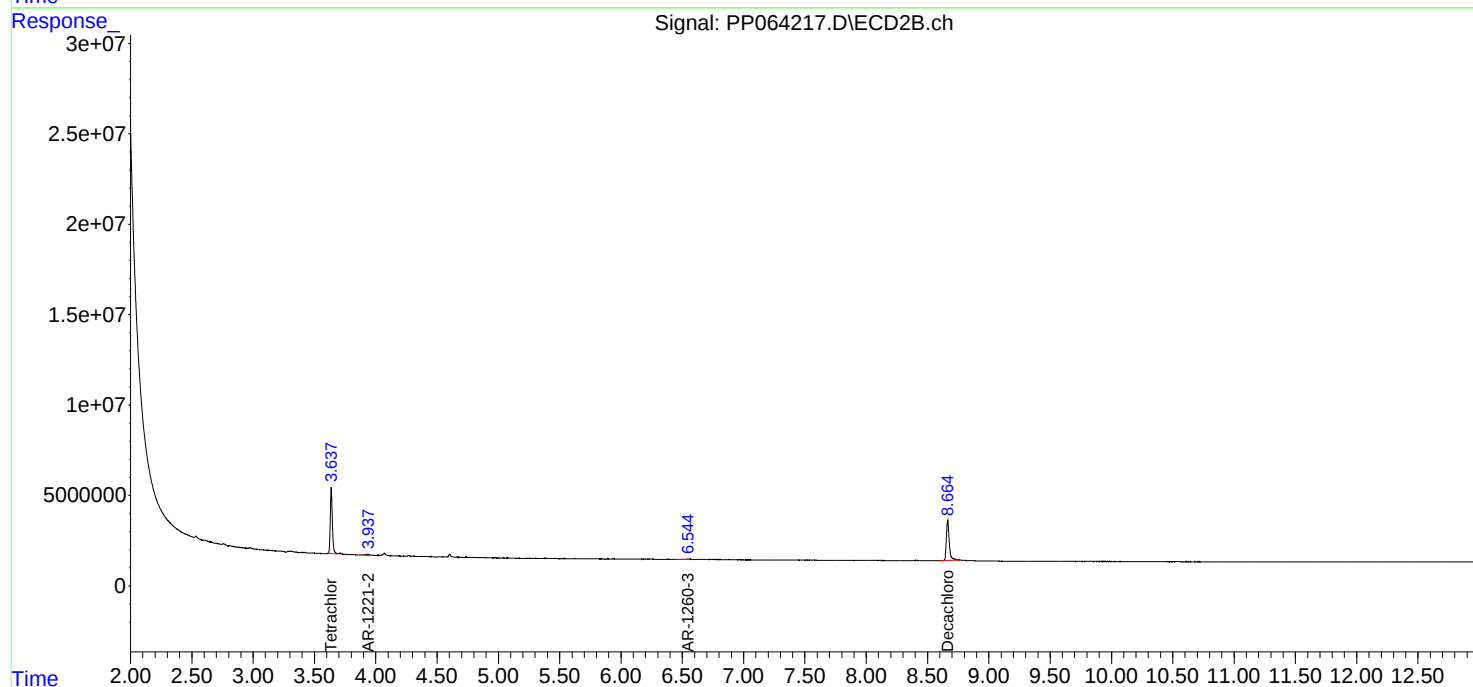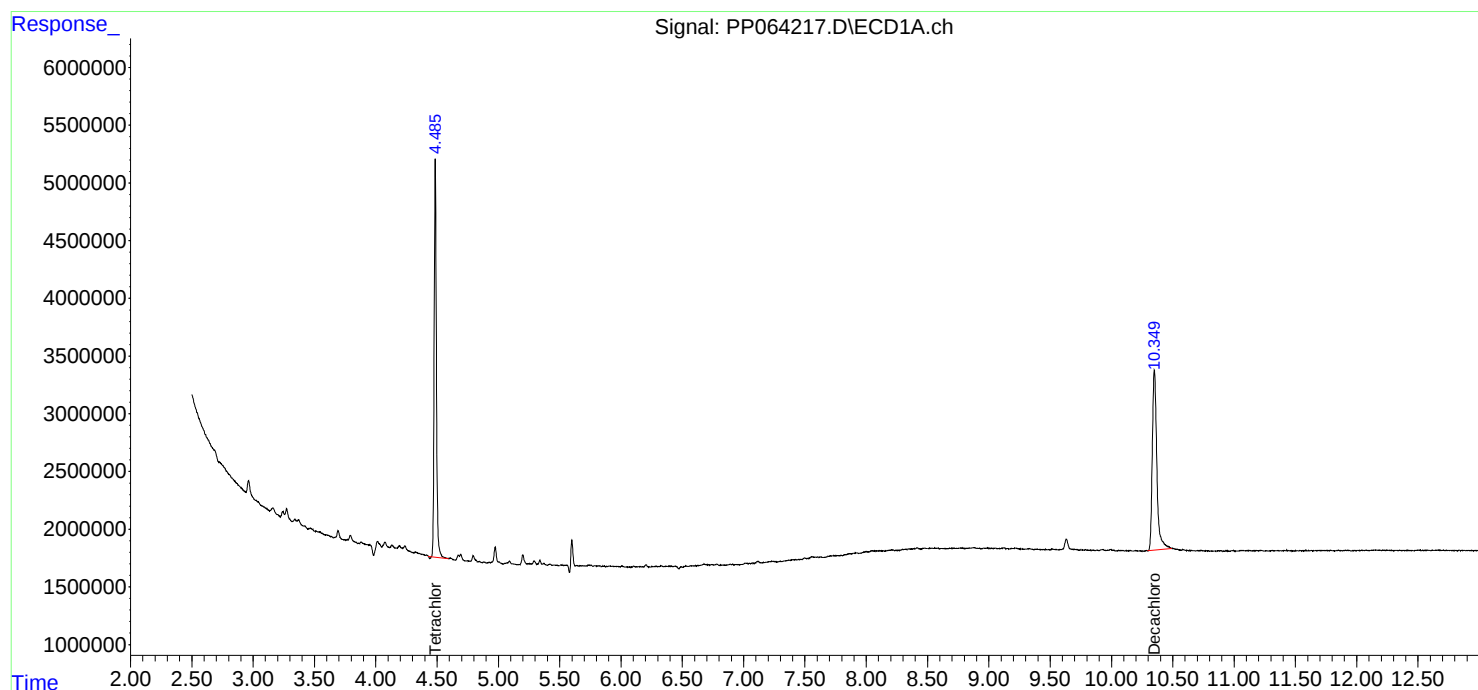


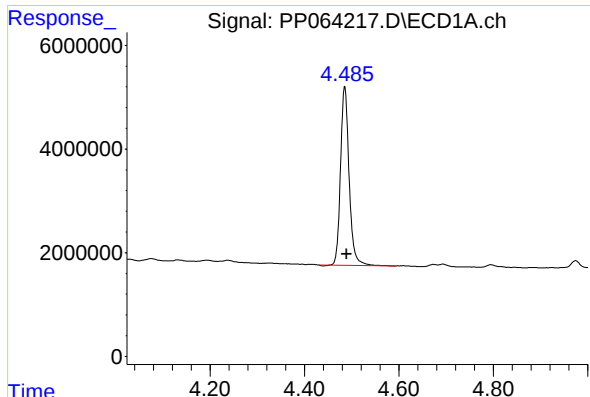

#1 Tetrachloro-m-xylene


R.T.: 4.485 min
Delta R.T.: -0.004 min
Response: 43572970
Conc: 18.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP

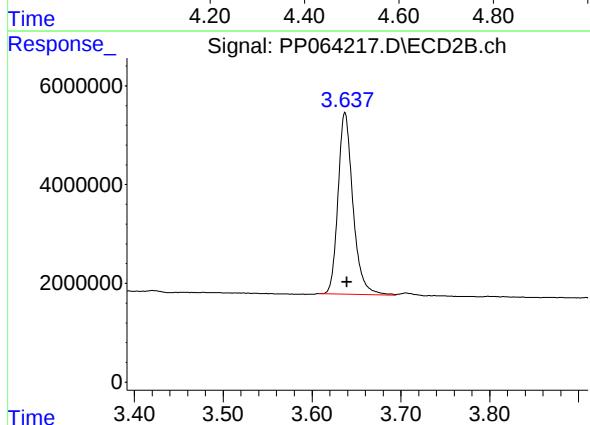


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 42969780
Conc: 18.00 ng/ml

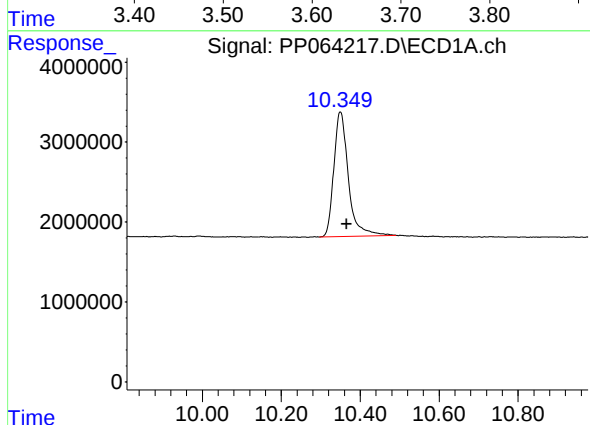


#2 Decachlorobiphenyl

R.T.: 10.350 min
Delta R.T.: -0.016 min
Response: 39996357
Conc: 15.75 ng/ml

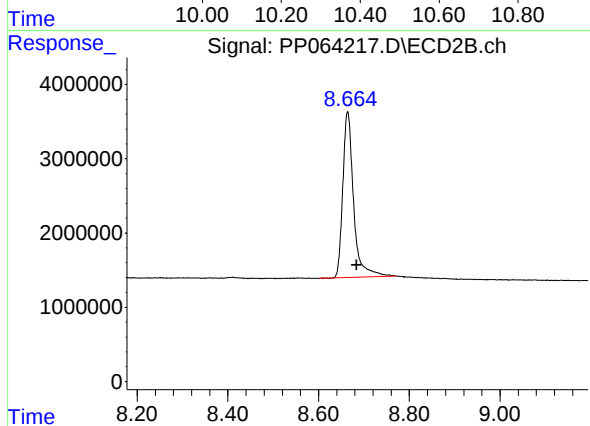

#2 Decachlorobiphenyl


R.T.: 8.664 min
Delta R.T.: -0.019 min
Response: 36716630
Conc: 13.59 ng/ml

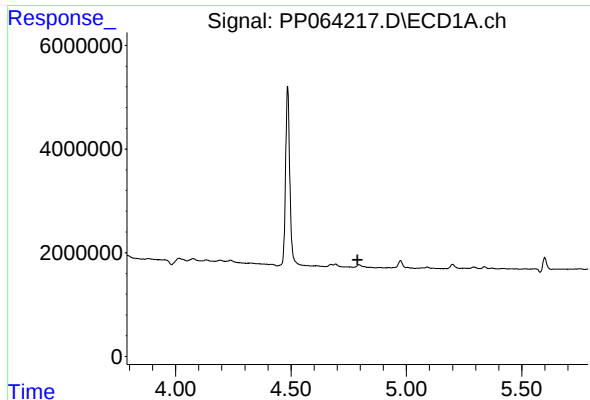

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP

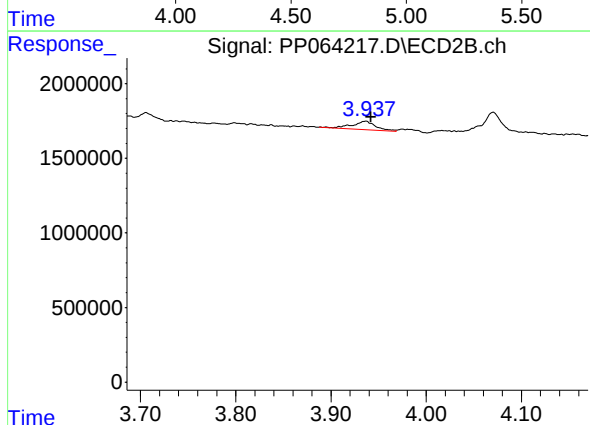


#9 AR-1221-2

R.T.: 3.936 min
Delta R.T.: -0.005 min
Response: 988690
Conc: 48.24 ng/ml

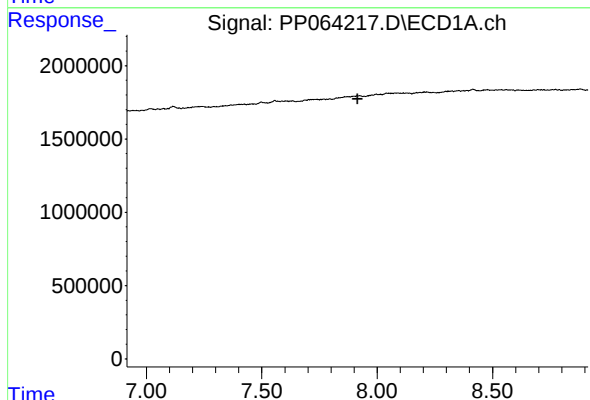

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.915 min
Response: 0
Conc: N.D.

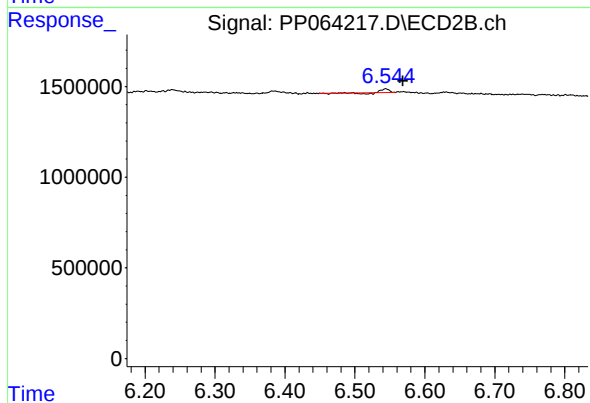

#33 AR-1260-3

R.T.: 6.544 min
Delta R.T.: -0.025 min
Response: 107729
Conc: 0.67 ng/ml