

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040925\
 Data File : PP071177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 13:31
 Operator : YP\AJ
 Sample : Q1748-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IB-1.5-WC

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2025
 Supervised By :mohammad ahmed 04/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 14:54:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.510	3.813	28326015	21448718	19.380m	20.691m
2) SA Decachlor...	10.232	8.851	17283469	10782885	16.420	13.680

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040925\
Data File : PP071177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 13:31
Operator : YP\AJ
Sample : Q1748-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
IB-1.5-WC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2025
Supervised By :mohammad ahmed 04/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 14:54:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

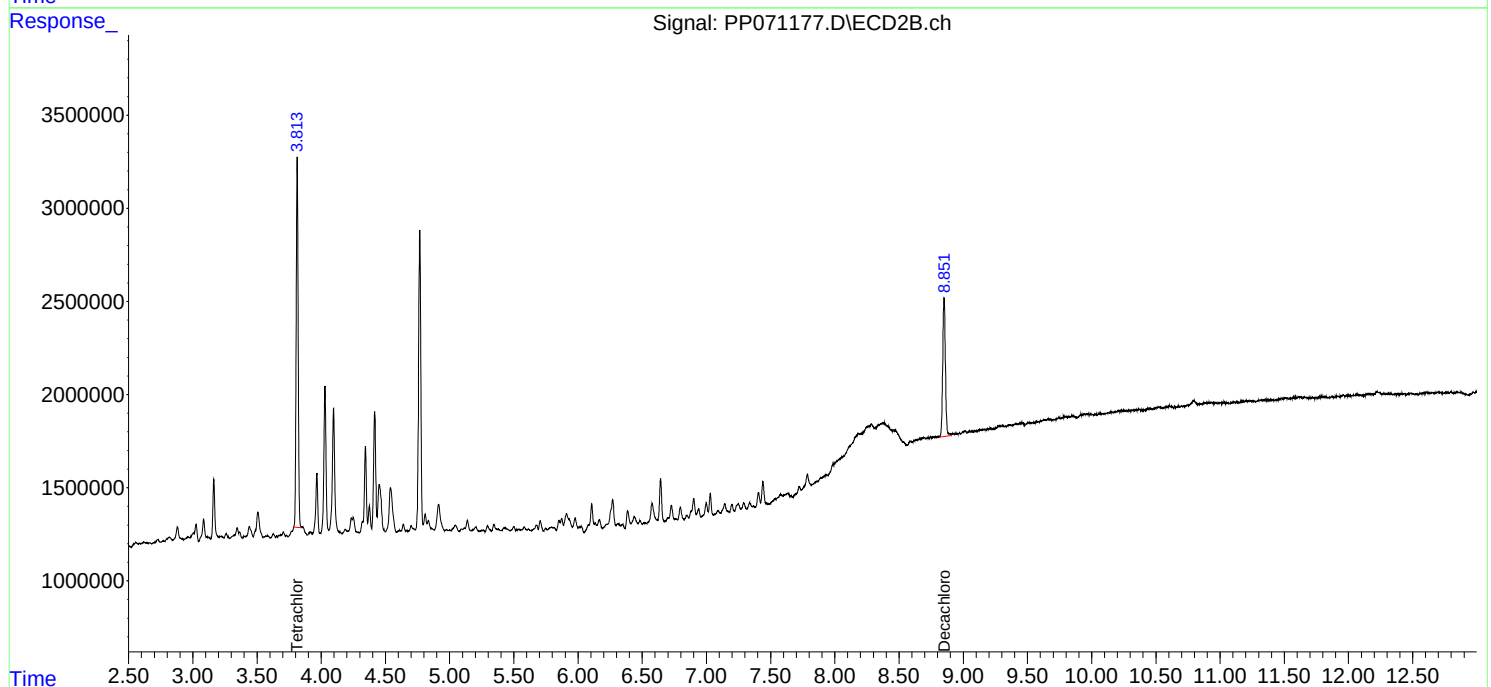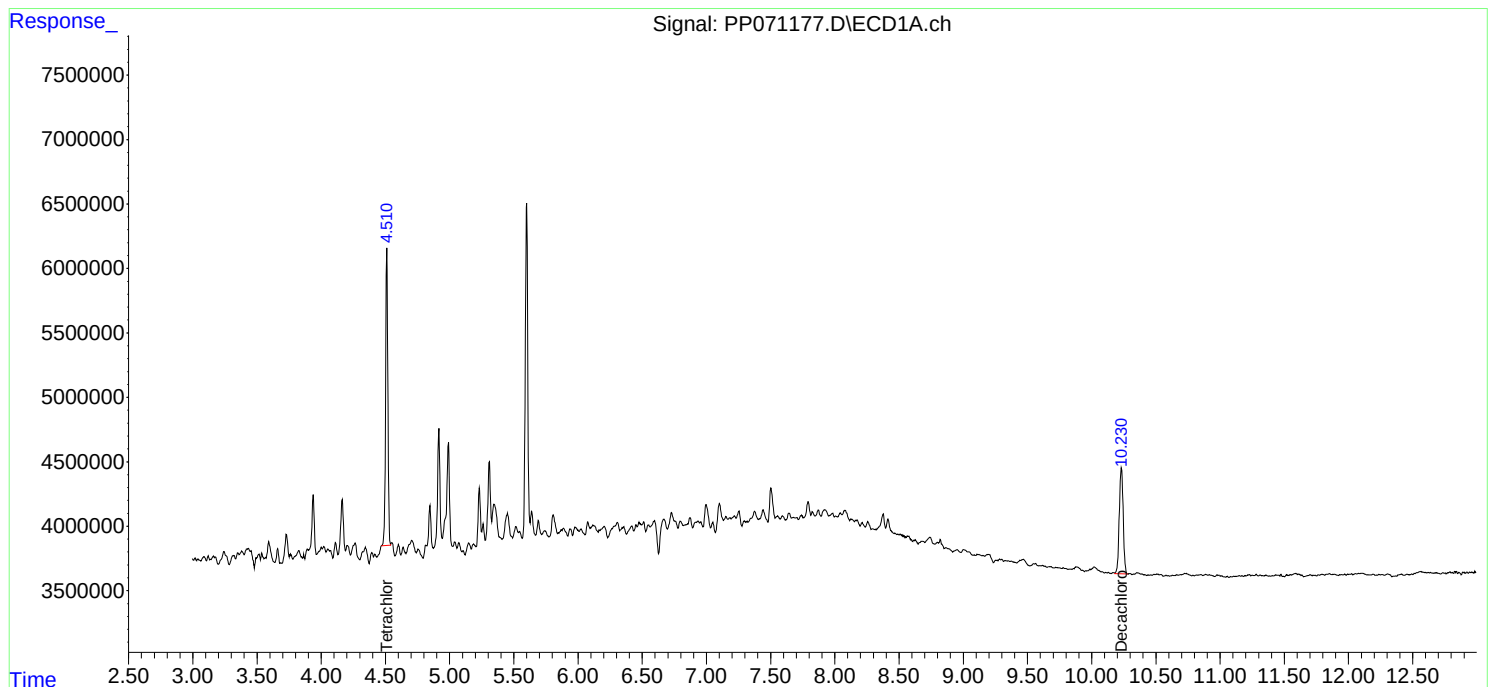

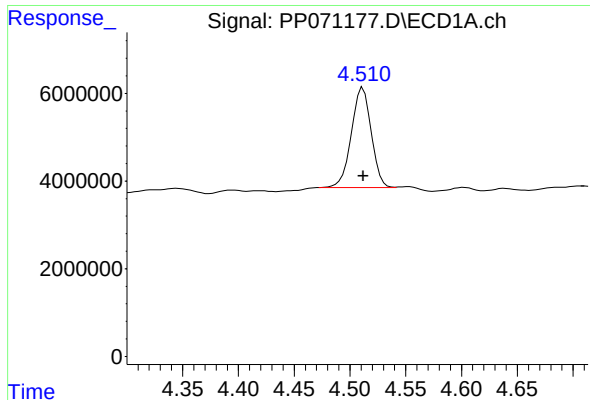


#1 Tetrachloro-m-xylene

R.T.: 4.510 min
Delta R.T.: -0.002 min
Response: 28326015
Conc: 19.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
IB-1.5-WC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2025
Supervised By :mohammad ahmed 04/11/2025

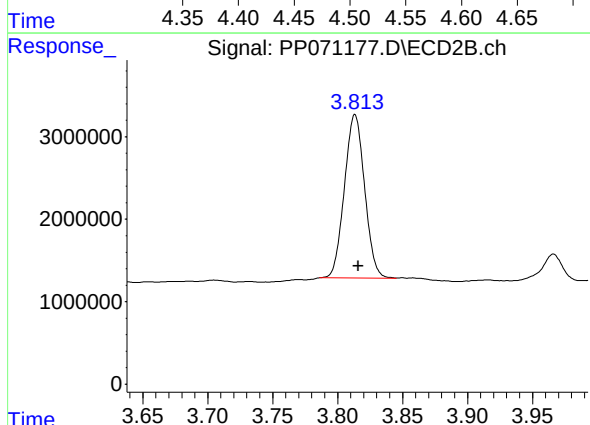


#1 Tetrachloro-m-xylene

R.T.: 3.813 min
Delta R.T.: -0.003 min
Response: 21448718
Conc: 20.69 ng/ml

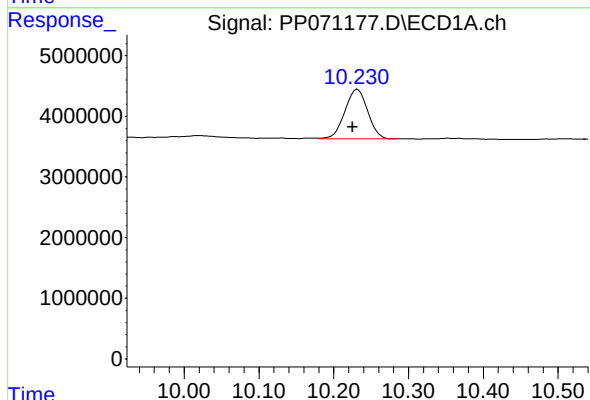

#2 Decachlorobiphenyl

R.T.: 10.232 min
Delta R.T.: 0.006 min
Response: 17283469
Conc: 16.42 ng/ml

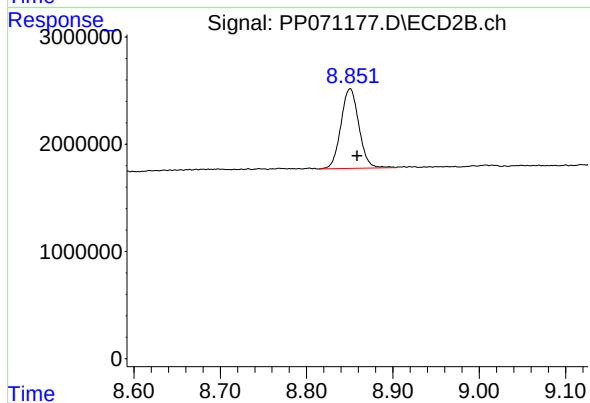

#2 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: -0.008 min
Response: 10782885
Conc: 13.68 ng/ml