

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041025\
 Data File : PP071215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2025 19:49
 Operator : YP\AJ
 Sample : Q1774-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TT-074-IDWGW-20250409

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/11/2025
 Supervised By :mohammad ahmed 04/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 01:39:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.515	3.814	37777800	24977202	25.847	24.094m
2) SA Decachlor...	10.233	8.851	8319859	5746962	7.904	7.291

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041025\
Data File : PP071215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2025 19:49
Operator : YP\AJ
Sample : Q1774-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TT-074-IDWGW-20250409


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2025
Supervised By :mohammad ahmed 04/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 01:39:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

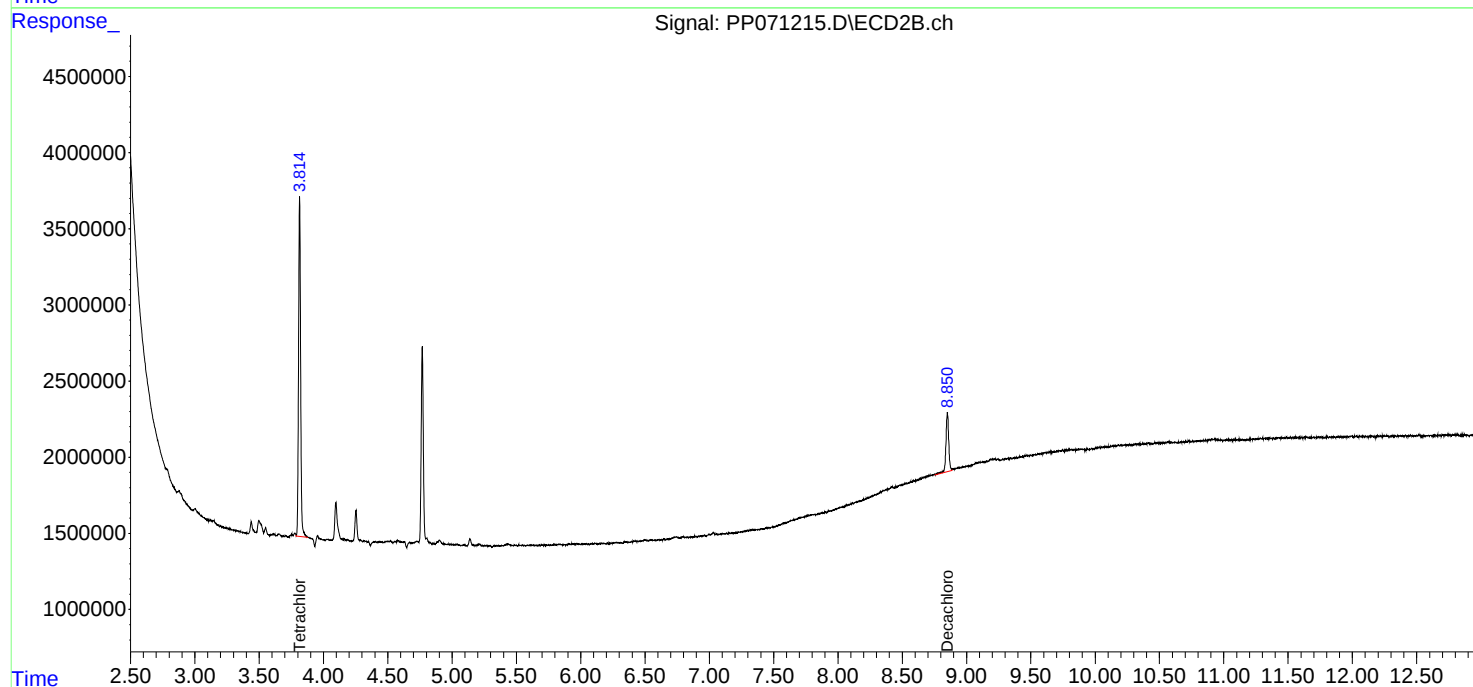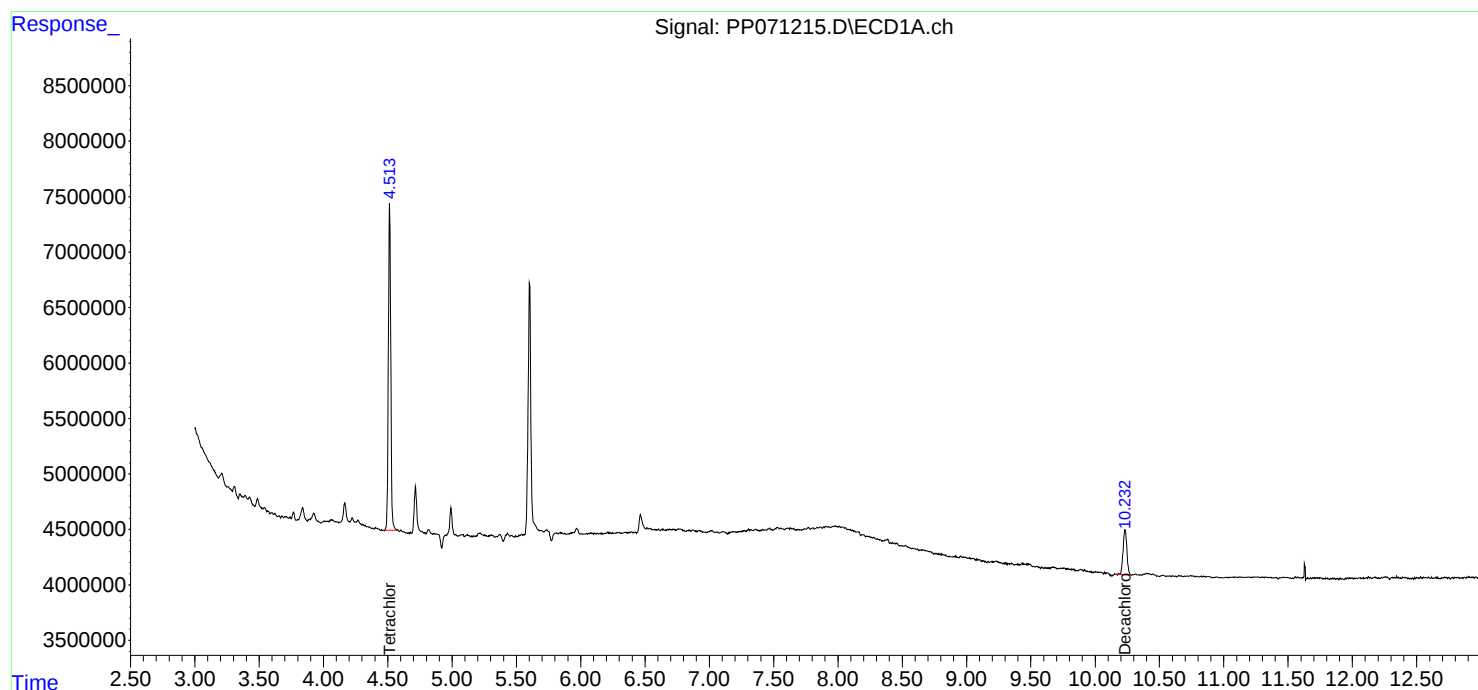

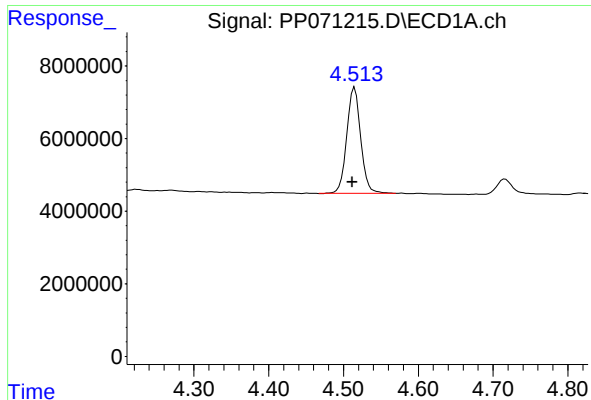


#1 Tetrachloro-m-xylene

R.T.: 4.515 min
Delta R.T.: 0.003 min
Response: 37777800
Conc: 25.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
TT-074-IDWGW-20250409


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2025
Supervised By :mohammad ahmed 04/14/2025

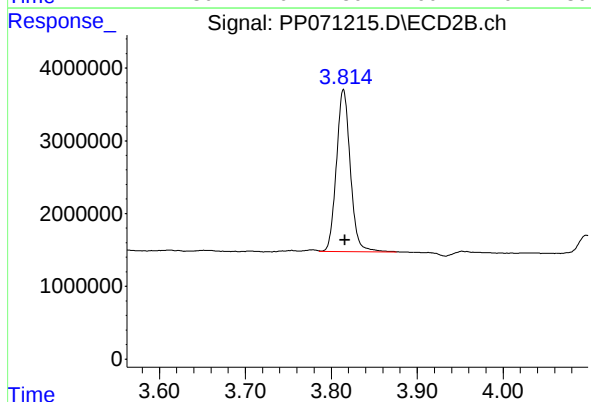


#1 Tetrachloro-m-xylene

R.T.: 3.814 min
Delta R.T.: -0.002 min
Response: 24977202
Conc: 24.09 ng/ml

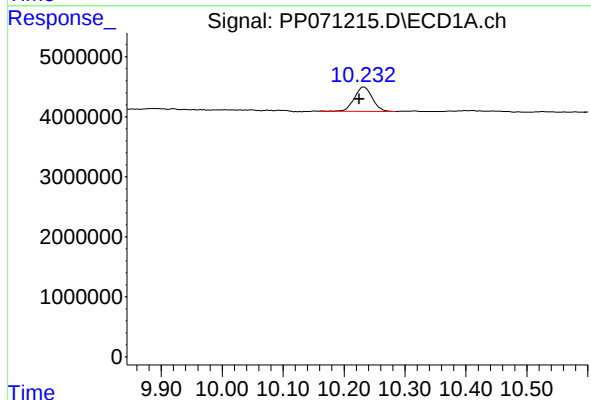

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: 0.008 min
Response: 8319859
Conc: 7.90 ng/ml

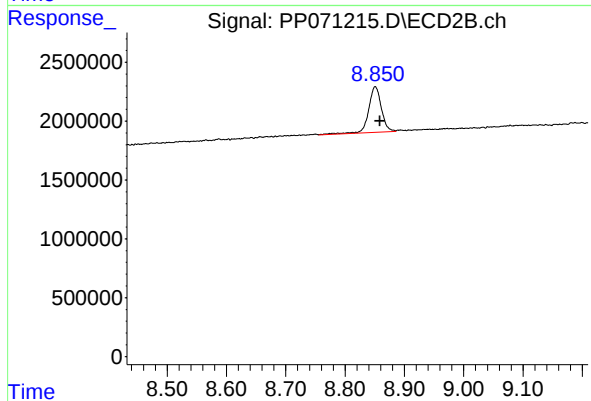

#2 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: -0.008 min
Response: 5746962
Conc: 7.29 ng/ml