

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041025\
 Data File : PP071216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2025 20:05
 Operator : YP\AJ
 Sample : Q1774-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TT-075-IDWGW-20250409

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/11/2025
 Supervised By :mohammad ahmed 04/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 01:39:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.512	3.814	37444227	25005440	25.619	24.122m
2) SA Decachlor...	10.231	8.851	9505881	6166112	9.031	7.823

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041025\
Data File : PP071216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2025 20:05
Operator : YP\AJ
Sample : Q1774-04
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TT-075-IDWGW-20250409


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2025
Supervised By :mohammad ahmed 04/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 01:39:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

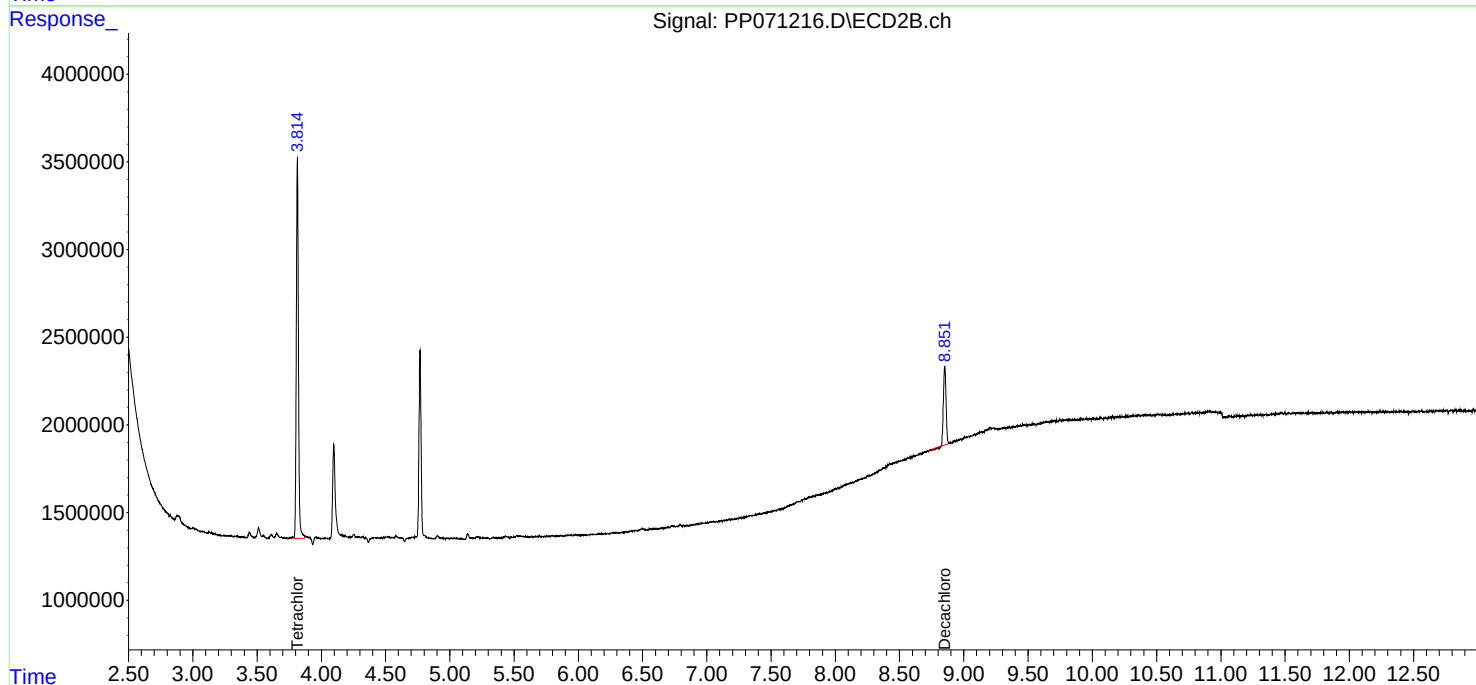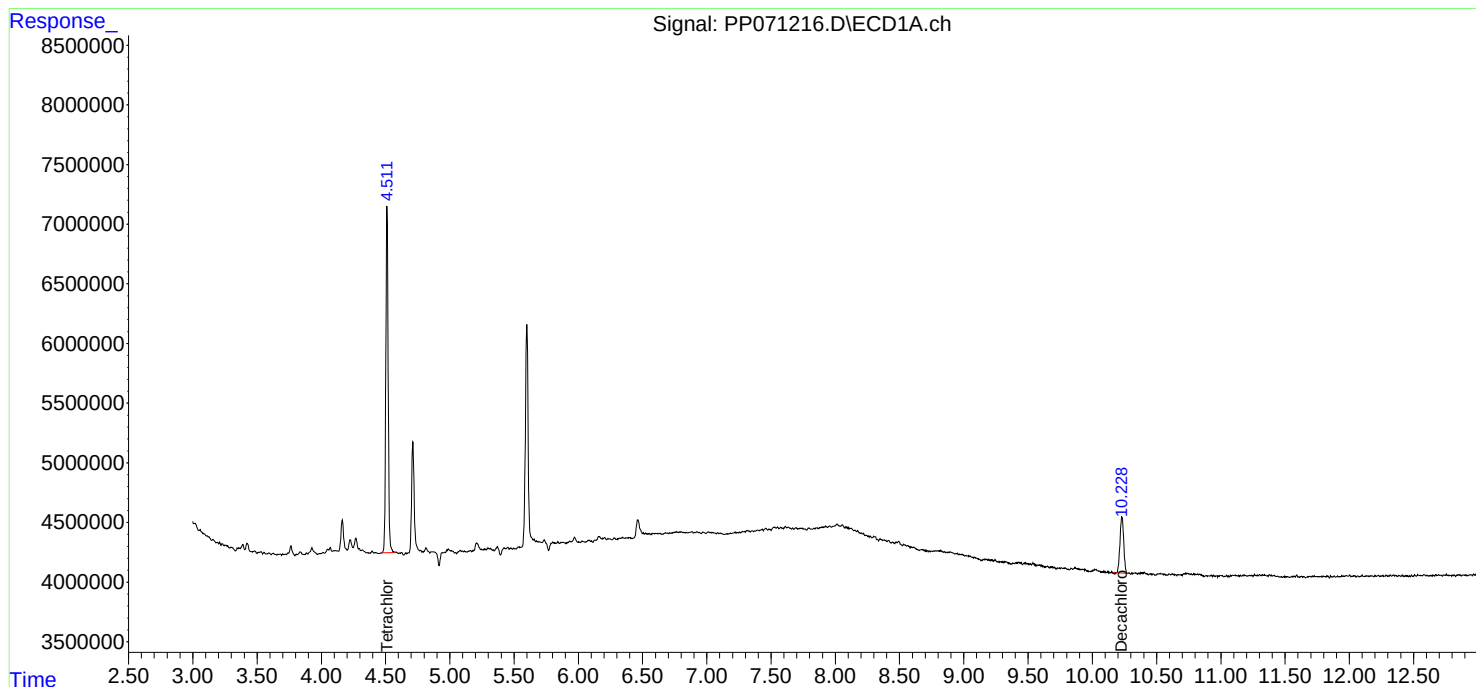

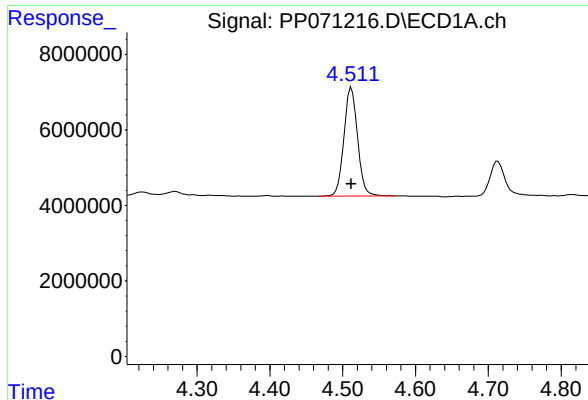


#1 Tetrachloro-m-xylene

R.T.: 4.512 min
Delta R.T.: 0.000 min
Response: 37444227
Conc: 25.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
TT-075-IDWGW-20250409


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2025
Supervised By :mohammad ahmed 04/14/2025

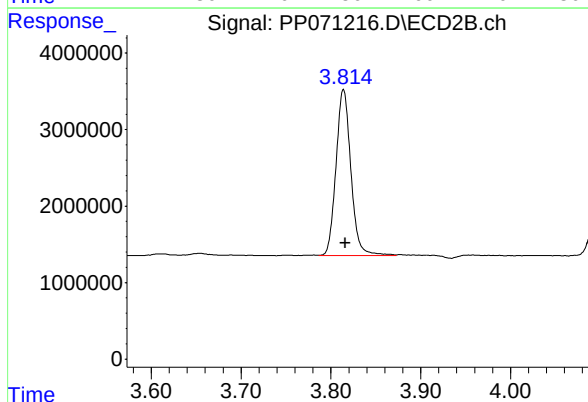


#1 Tetrachloro-m-xylene

R.T.: 3.814 min
Delta R.T.: -0.002 min
Response: 25005440
Conc: 24.12 ng/ml m

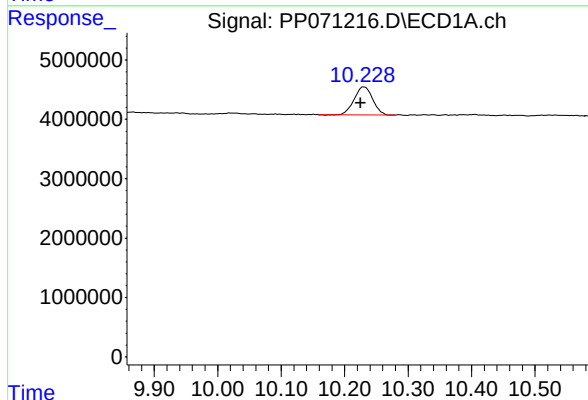

#2 Decachlorobiphenyl

R.T.: 10.231 min
Delta R.T.: 0.005 min
Response: 9505881
Conc: 9.03 ng/ml

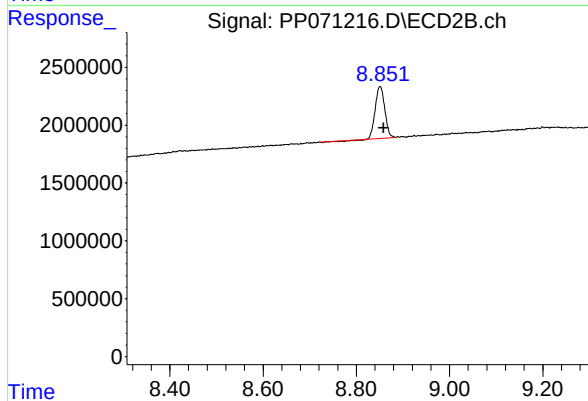

#2 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: -0.008 min
Response: 6166112
Conc: 7.82 ng/ml