

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041122\
 Data File : PP045810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 03:58
 Operator : YP\AJ
 Sample : N2334-12
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DUP040522

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/11/2022
 Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 06:29:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 09 07:55:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.882	3.143	21052869	15570840	8.725	9.840
2) SA Decachlor...	9.980	8.481	8360584	8092326	5.835m	5.336

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041122\
Data File : PP045810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 03:58
Operator : YP\AJ
Sample : N2334-12
Misc :
ALS Vial : 90 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DUP040522


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 06:29:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 09 07:55:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

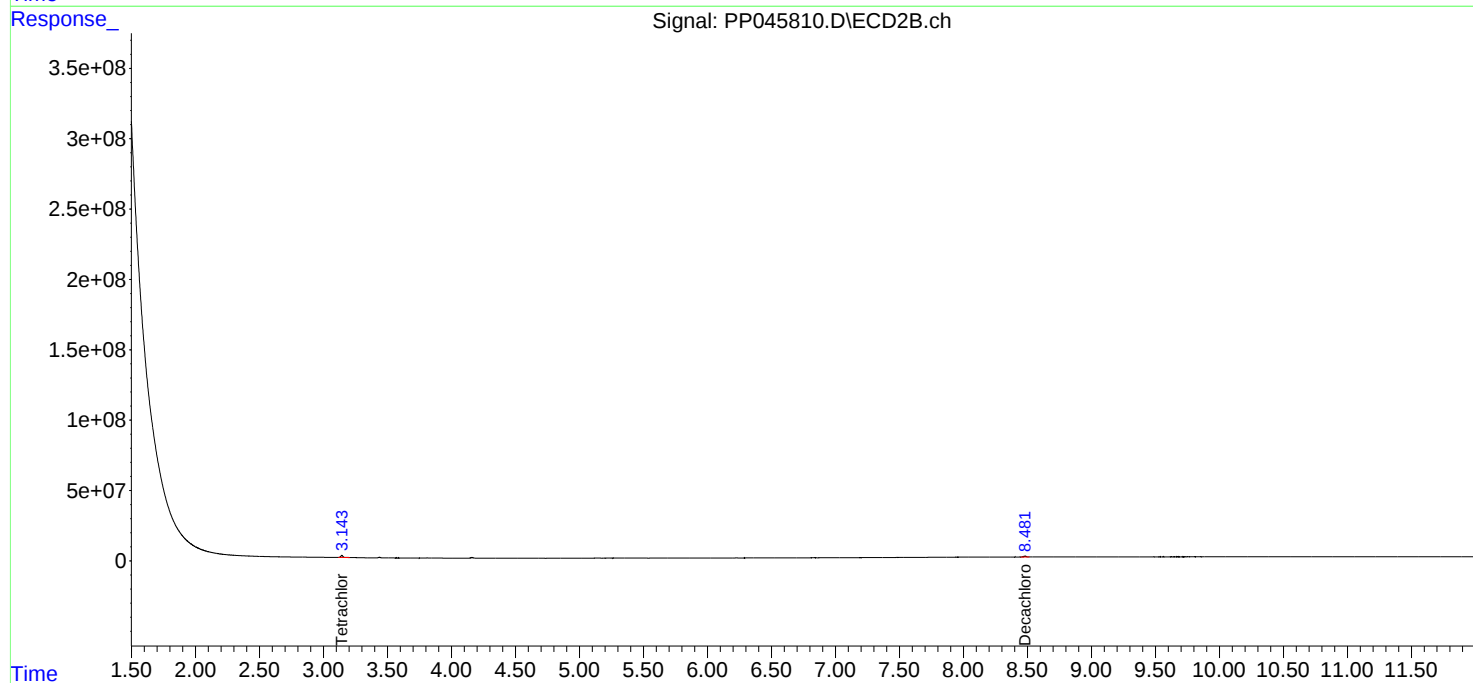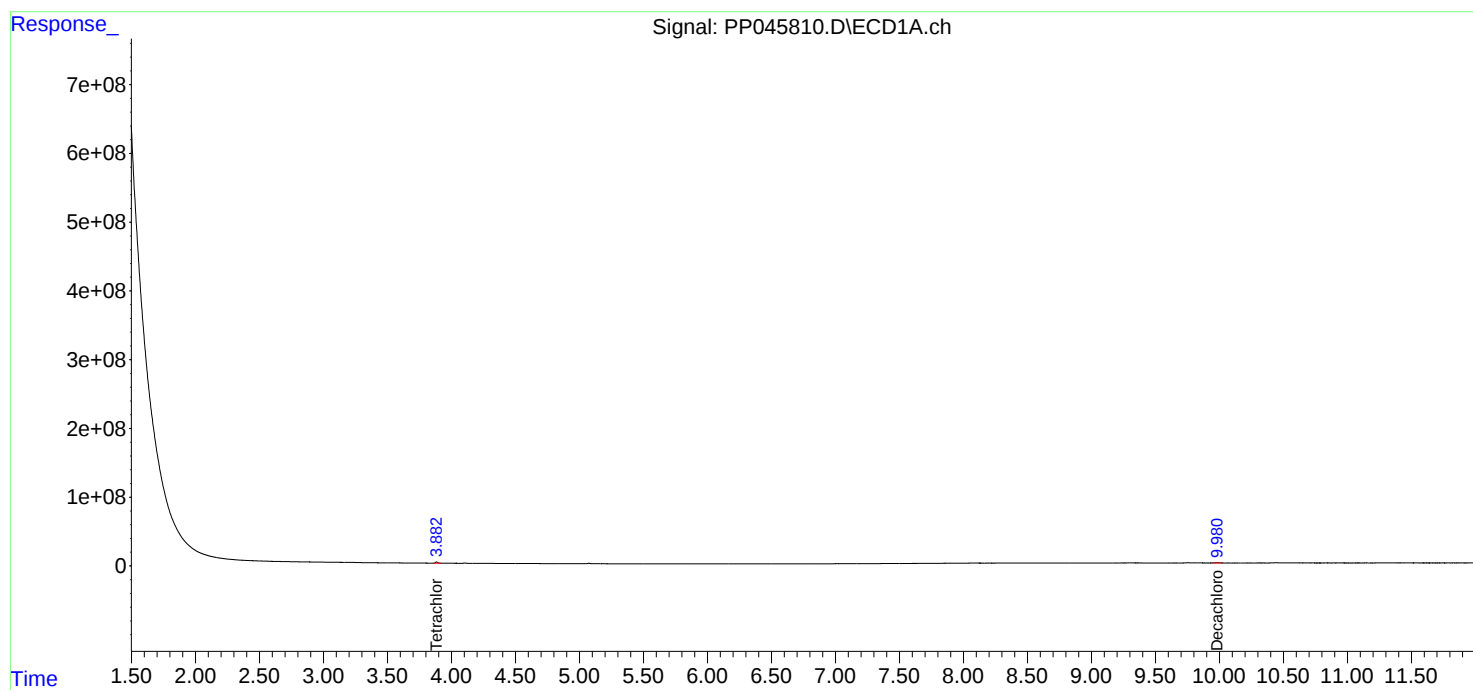

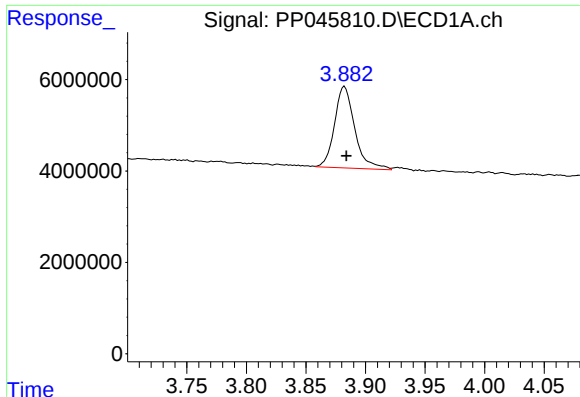


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: -0.002 min
Response: 21052869
Conc: 8.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
DUP040522


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

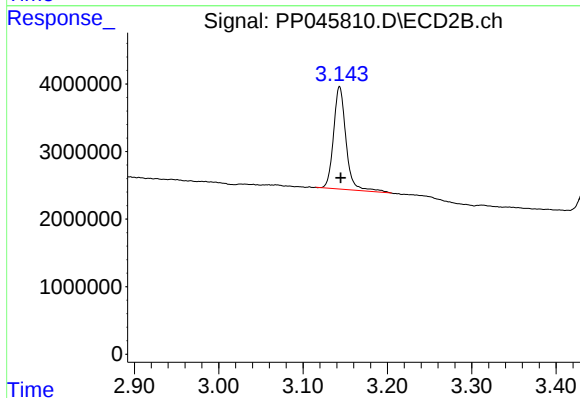


#1 Tetrachloro-m-xylene

R.T.: 3.143 min
Delta R.T.: -0.001 min
Response: 15570840
Conc: 9.84 ng/ml

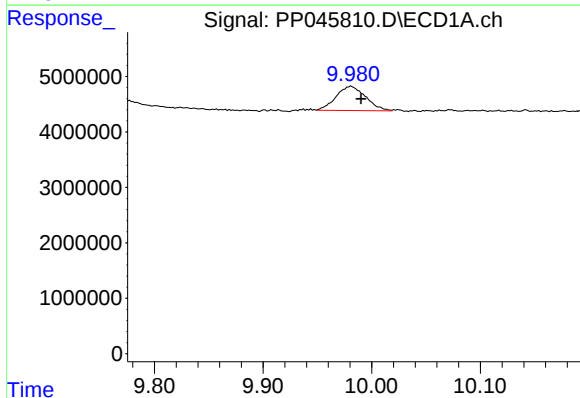

#2 Decachlorobiphenyl

R.T.: 9.980 min
Delta R.T.: -0.010 min
Response: 8360584
Conc: 5.84 ng/ml m

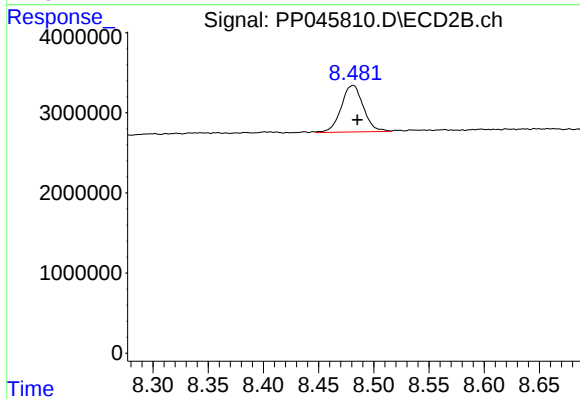

#2 Decachlorobiphenyl

R.T.: 8.481 min
Delta R.T.: -0.004 min
Response: 8092326
Conc: 5.34 ng/ml