

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041122\
 Data File : PP045814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 05:01
 Operator : YP\AJ
 Sample : PB143399BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB143399BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/11/2022
 Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 06:30:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 09 07:55:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.882	3.142	47571335	33207506	19.716	20.986
2) SA Decachlor...	9.982	8.481	34016545	30257309	23.741m	19.953

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041122\
Data File : PP045814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 05:01
Operator : YP\AJ
Sample : PB143399BL
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB143399BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 06:30:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 09 07:55:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

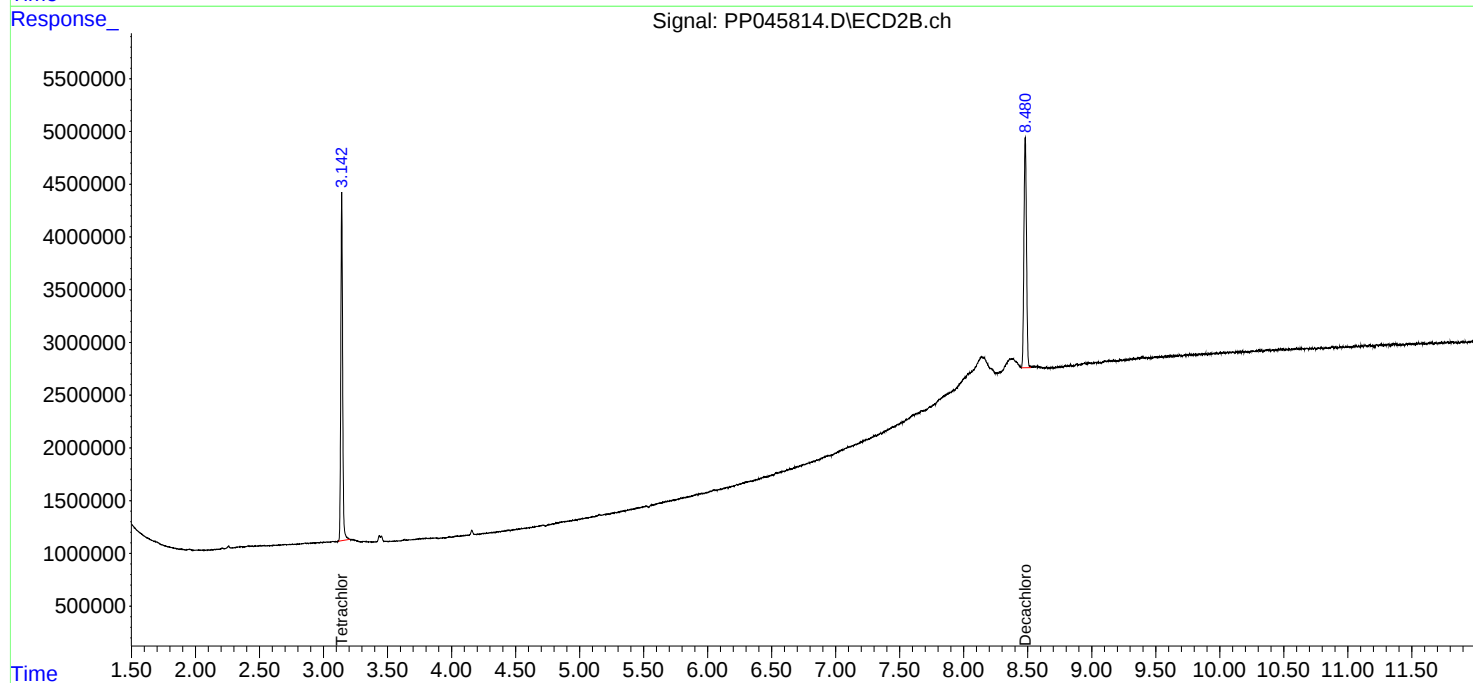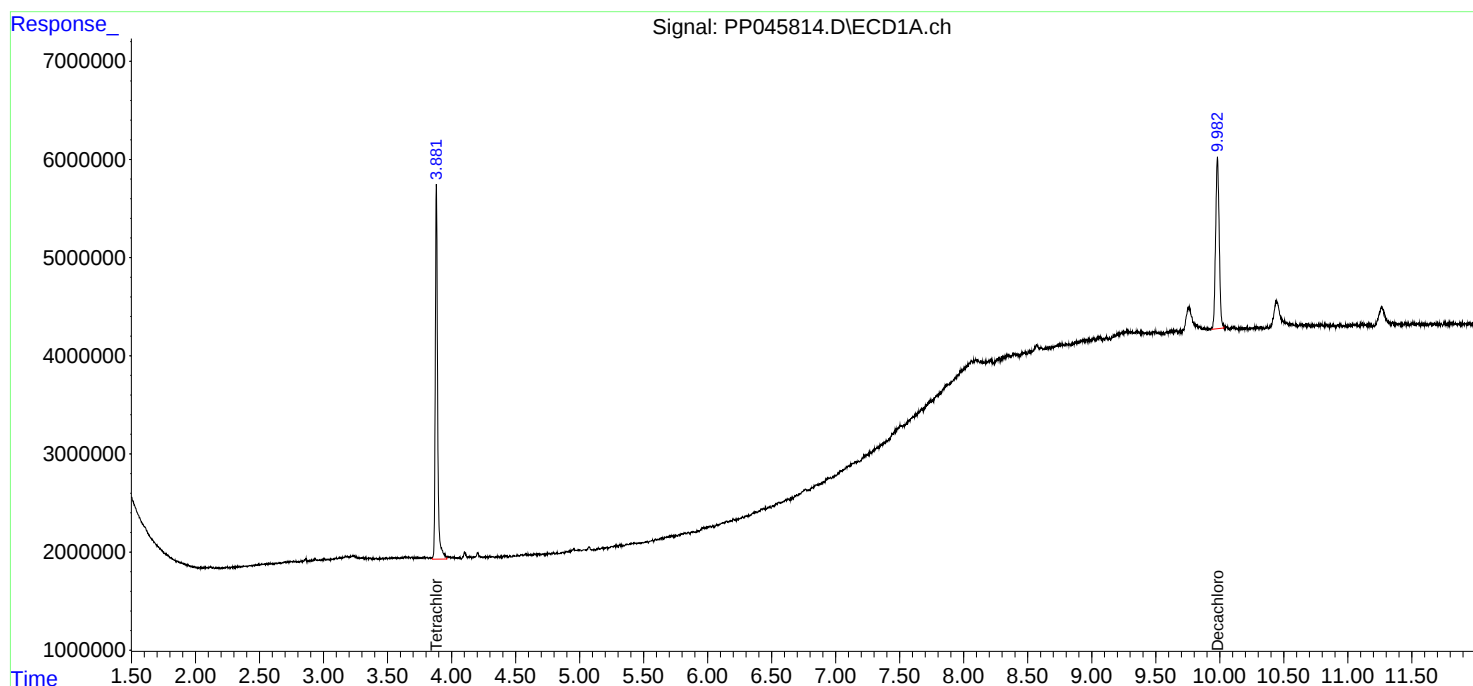

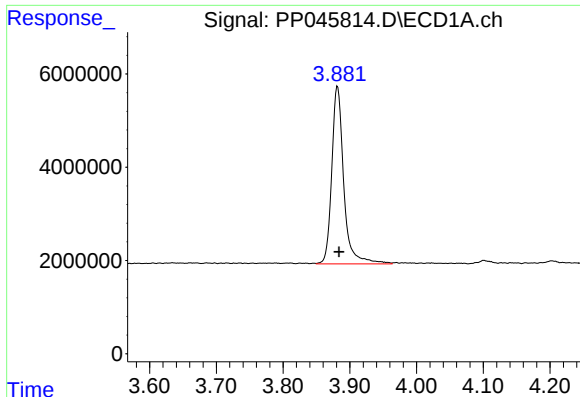


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: -0.002 min
Response: 47571335
Conc: 19.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB143399BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

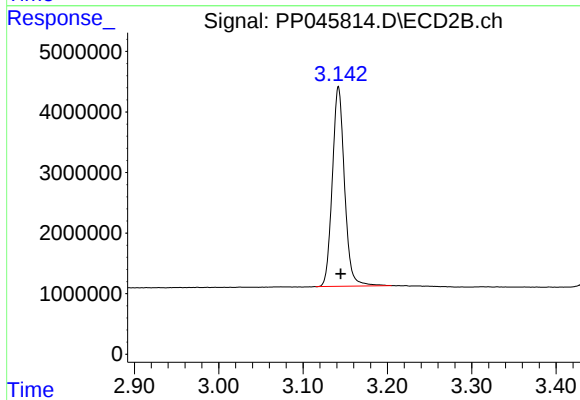


#1 Tetrachloro-m-xylene

R.T.: 3.142 min
Delta R.T.: -0.002 min
Response: 33207506
Conc: 20.99 ng/ml

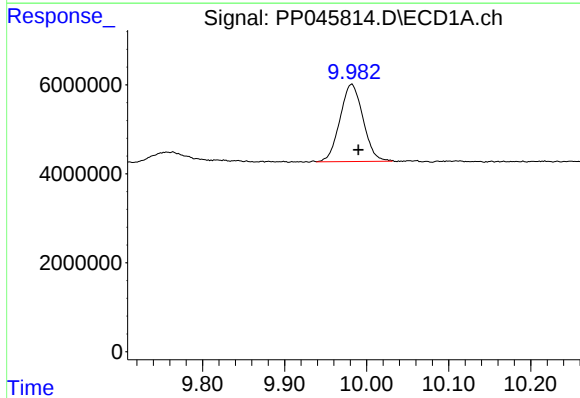

#2 Decachlorobiphenyl

R.T.: 9.982 min
Delta R.T.: -0.009 min
Response: 34016545
Conc: 23.74 ng/ml m

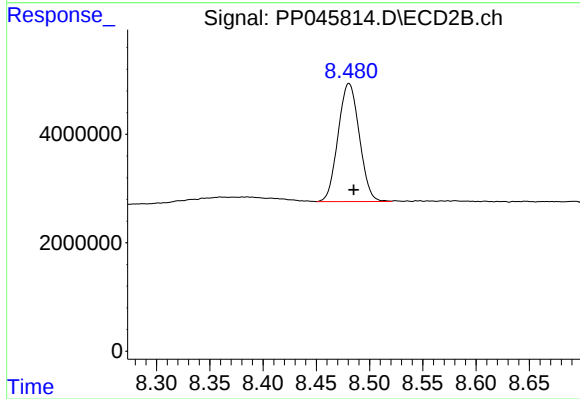

#2 Decachlorobiphenyl

R.T.: 8.481 min
Delta R.T.: -0.005 min
Response: 30257309
Conc: 19.95 ng/ml