

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041122\
 Data File : PP045825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 10:07
 Operator : YP\AJ
 Sample : N2348-24 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IRV-04-08-22-111-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/11/2022
 Supervised By :mohammad ahmed 04/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 14:42:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 11 14:34:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.881	3.141	3462464	2228664	1.435	1.408
2) SA Decachlor...	9.984	8.480	3483964	2490199	2.432m	1.642 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041122\
Data File : PP045825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 10:07
Operator : YP\AJ
Sample : N2348-24 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
IRV-04-08-22-111-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 14:42:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 11 14:34:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

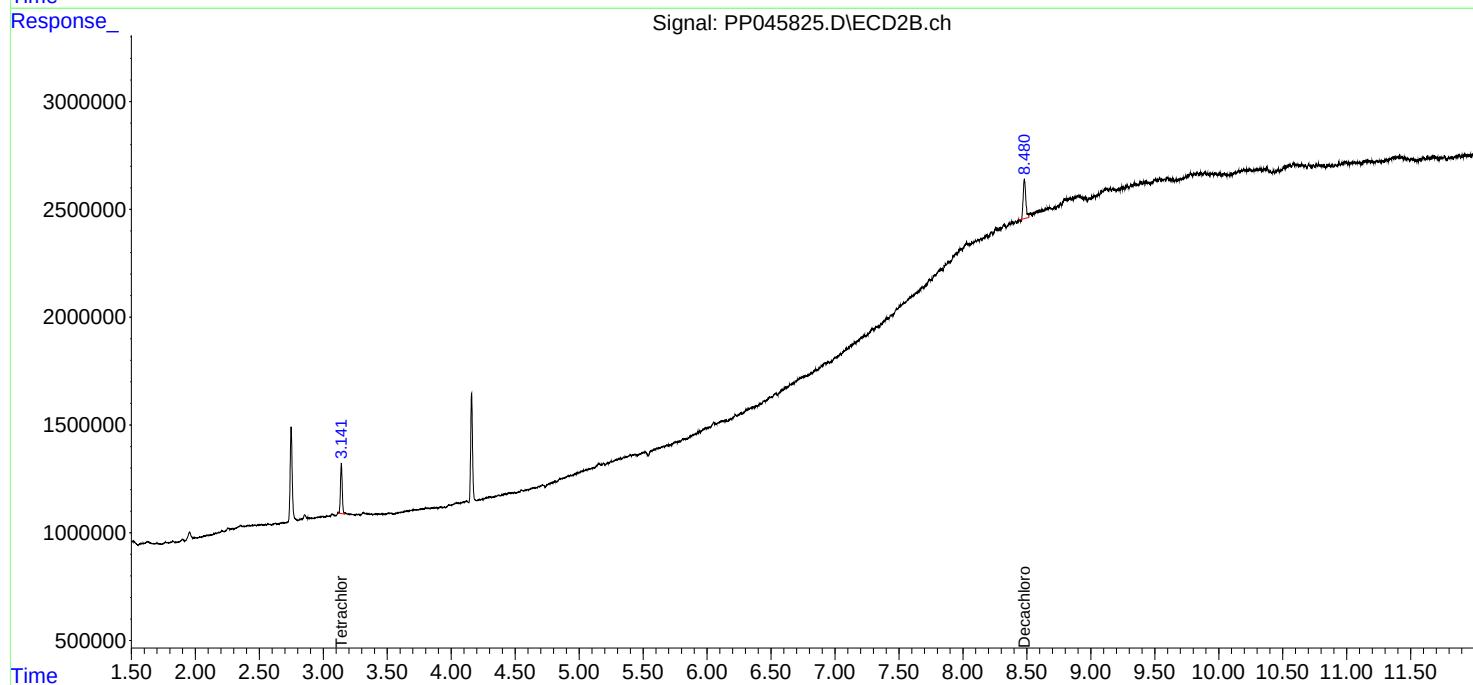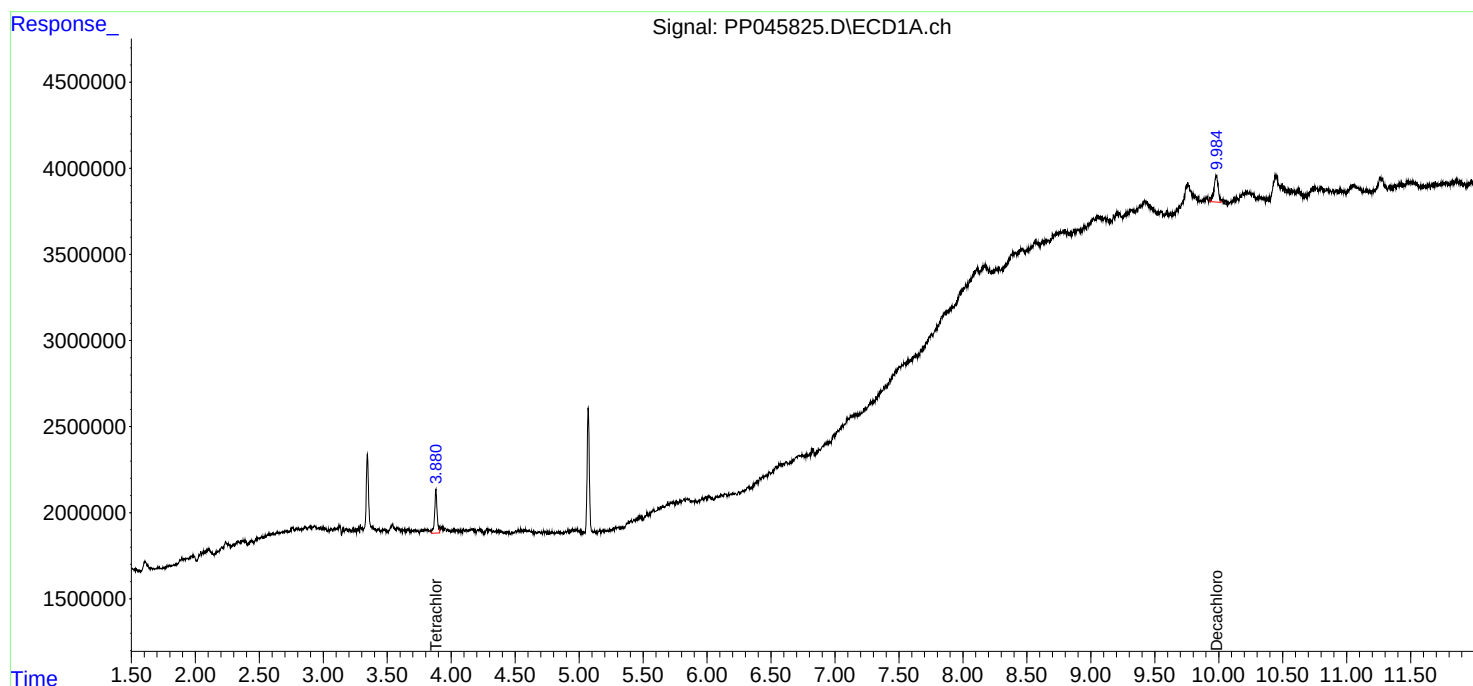

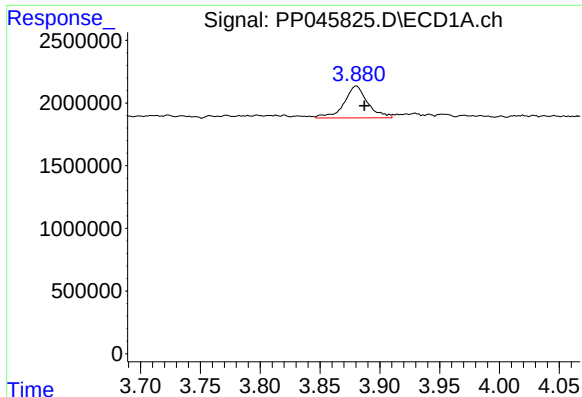


#1 Tetrachloro-m-xylene

R.T.: 3.881 min
Delta R.T.: -0.006 min
Response: 3462464
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-04-08-22-111-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/12/2022

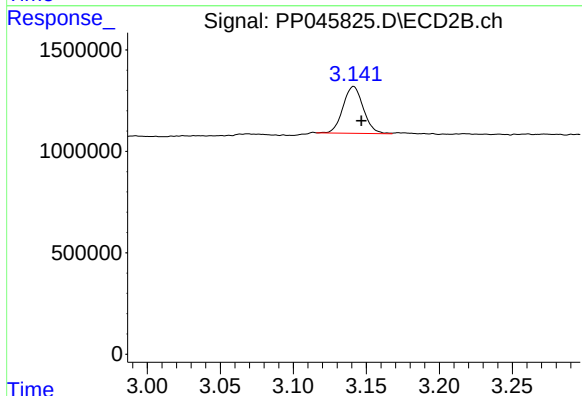


#1 Tetrachloro-m-xylene

R.T.: 3.141 min
Delta R.T.: -0.005 min
Response: 2228664
Conc: 1.41 ng/ml

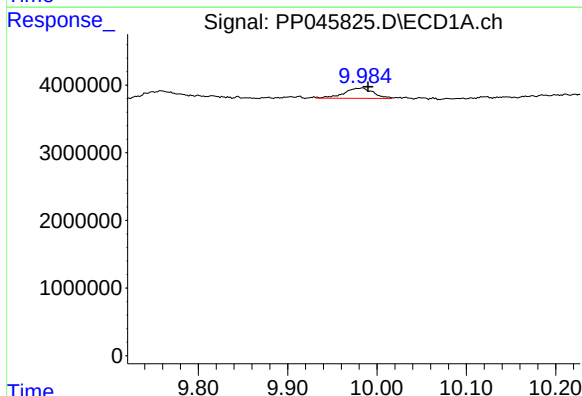

#2 Decachlorobiphenyl

R.T.: 9.984 min
Delta R.T.: -0.006 min
Response: 3483964
Conc: 2.43 ng/ml m

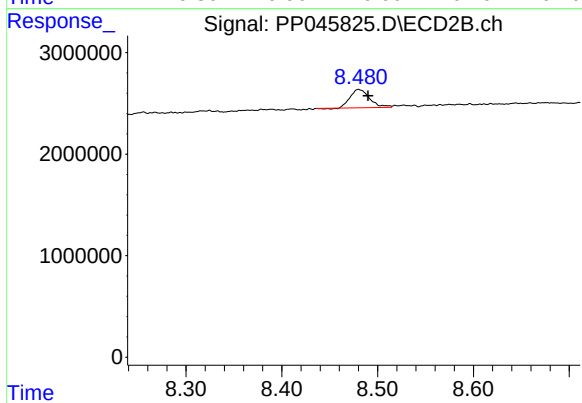

#2 Decachlorobiphenyl

R.T.: 8.480 min
Delta R.T.: -0.010 min
Response: 2490199
Conc: 1.64 ng/ml