

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041123\
 Data File : PP056847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2023 12:42
 Operator : YP\AJ
 Sample : 02257-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ELI-WATER-0407

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/12/2023
 Supervised By :Ankita Jodhani 04/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 13:20:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 04:14:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.435	3.663	3295242	2679508	1.534m	1.541
2) SA Decachlor...	10.276	8.745	3277570	3586604	2.504m	2.281

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041123\
Data File : PP056847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2023 12:42
Operator : YP\AJ
Sample : 02257-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ELI-WATER-0407


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/12/2023
Supervised By :Ankita Jodhani 04/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 13:20:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 04:14:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

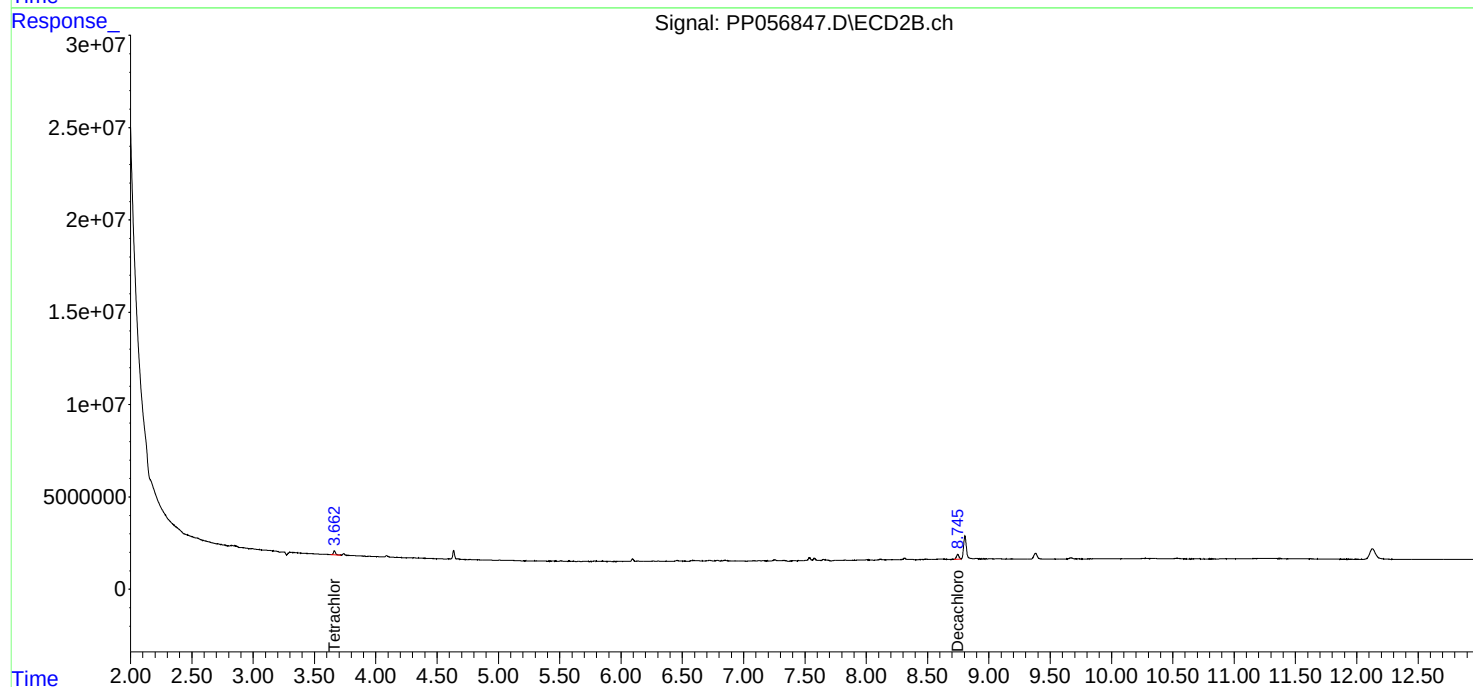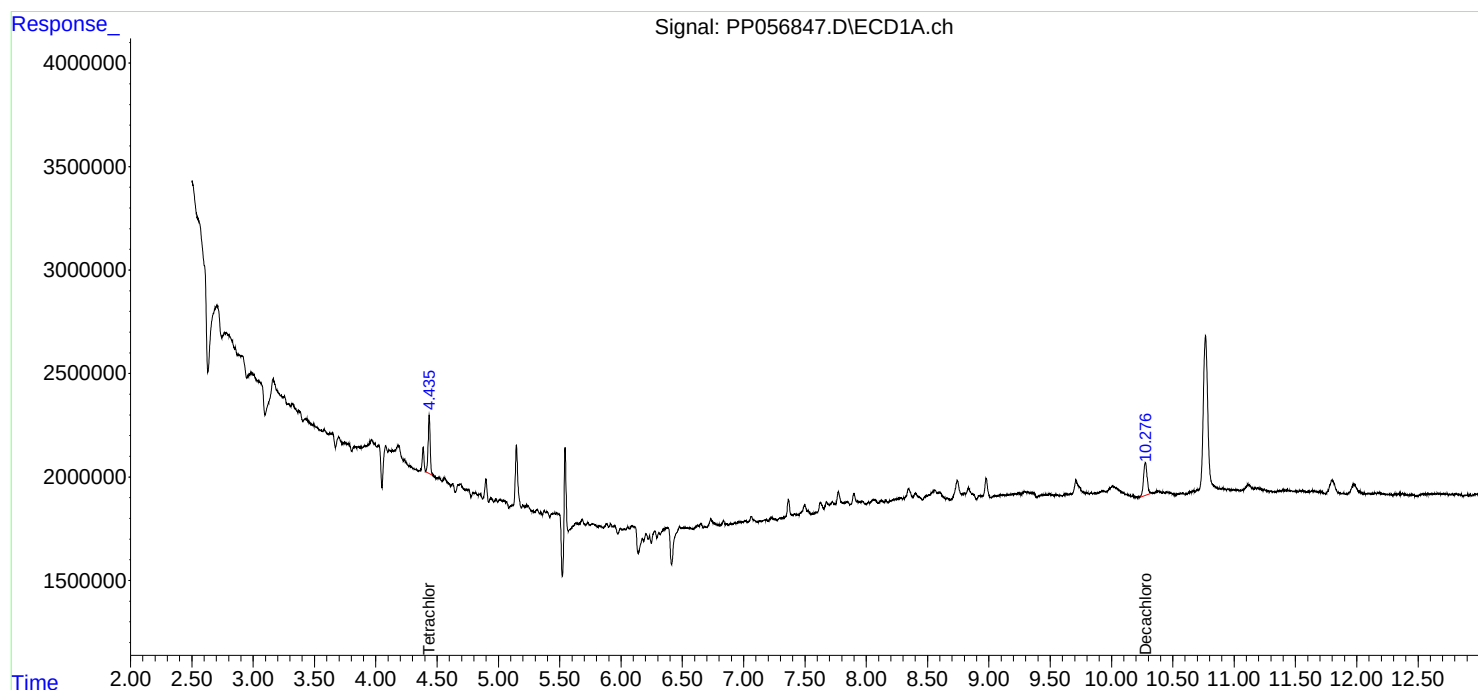

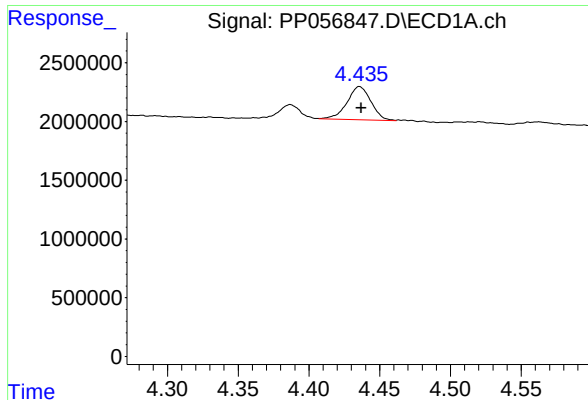


#1 Tetrachloro-m-xylene

R.T.: 4.435 min
Delta R.T.: -0.002 min
Response: 3295242
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
ELI-WATER-0407


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/12/2023
Supervised By :Ankita Jodhani 04/12/2023

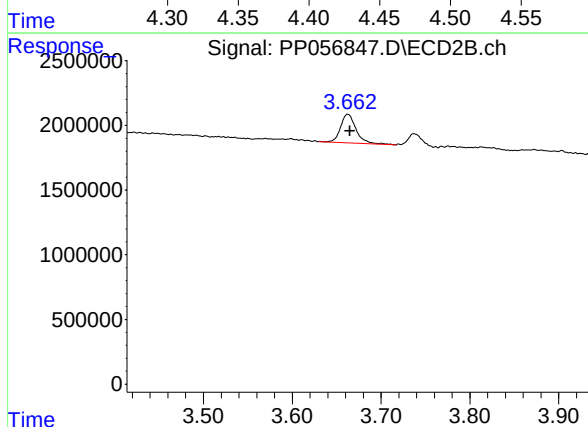


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.002 min
Response: 2679508
Conc: 1.54 ng/ml

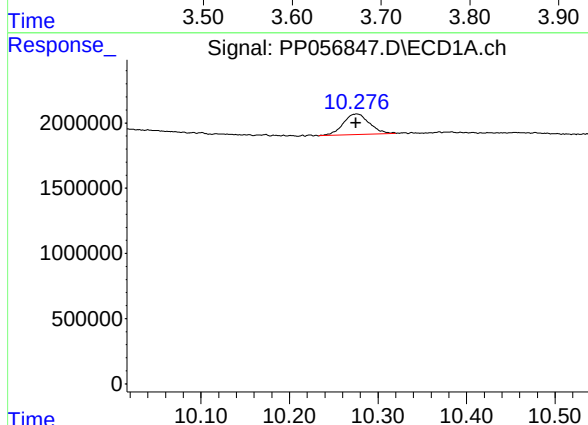

#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: 0.000 min
Response: 3277570
Conc: 2.50 ng/ml m

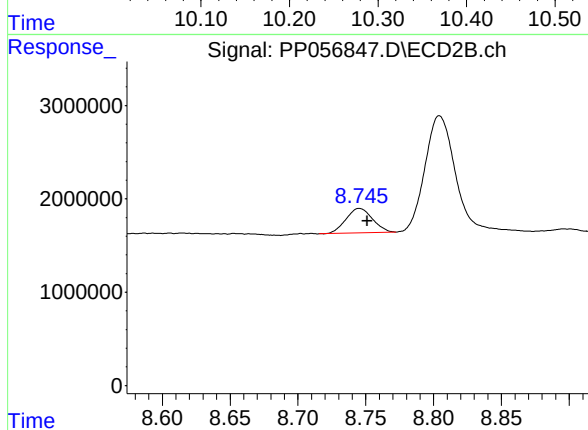

#2 Decachlorobiphenyl

R.T.: 8.745 min
Delta R.T.: -0.006 min
Response: 3586604
Conc: 2.28 ng/ml