

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041123\
 Data File : PP056855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2023 15:36
 Operator : YP\AJ
 Sample : 02257-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ELI-WATER-0407

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/12/2023
 Supervised By :Ankita Jodhani 04/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 15:56:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 04:14:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

 System Monitoring Compounds

1) SA Tetrachlo...	4.435	3.662	13654954	10617744	6.356m	6.105
2) SA Decachlor...	10.275	8.745	11803344	12459551	9.018	7.924

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041123\
Data File : PP056855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2023 15:36
Operator : YP\AJ
Sample : 02257-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ELI-WATER-0407


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/12/2023
Supervised By :Ankita Jodhani 04/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 15:56:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 04:14:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

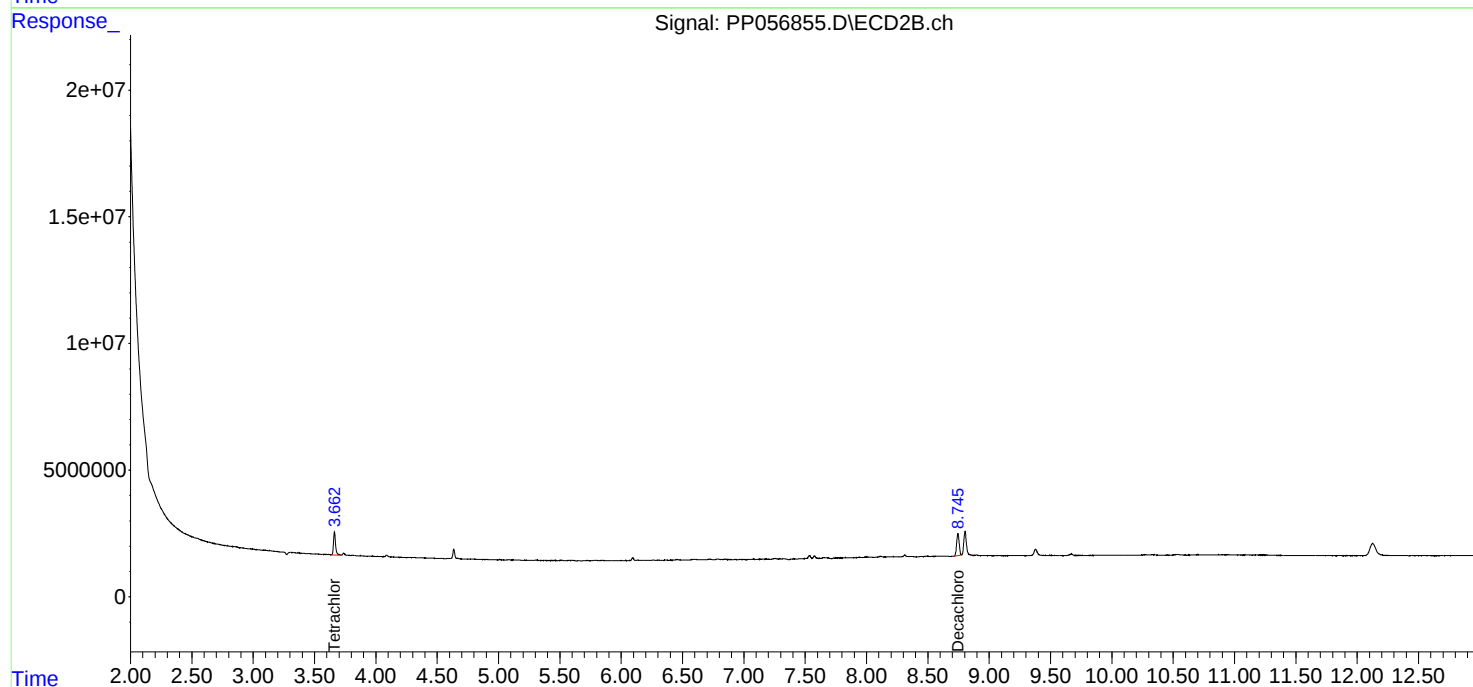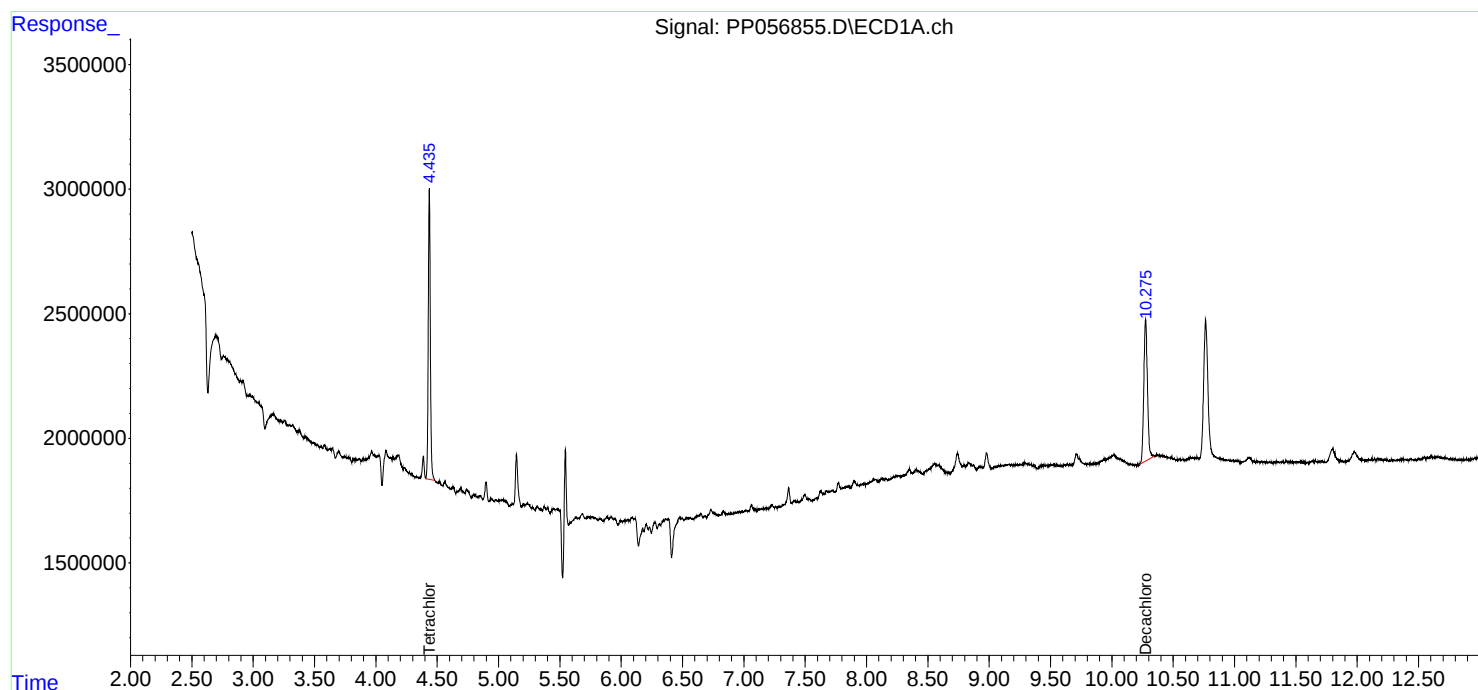

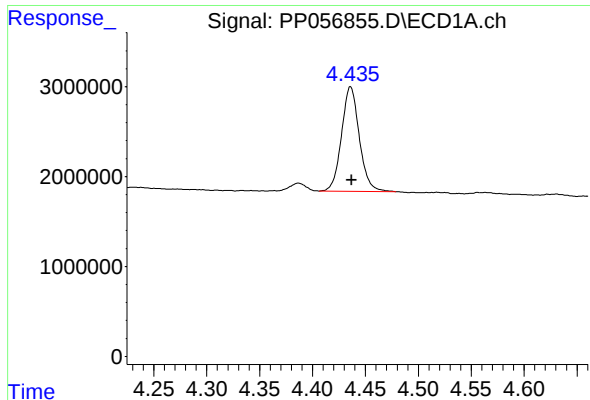


#1 Tetrachloro-m-xylene

R.T.: 4.435 min
Delta R.T.: -0.002 min
Response: 13654954
Conc: 6.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
ELI-WATER-0407


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/12/2023
Supervised By :Ankita Jodhani 04/12/2023

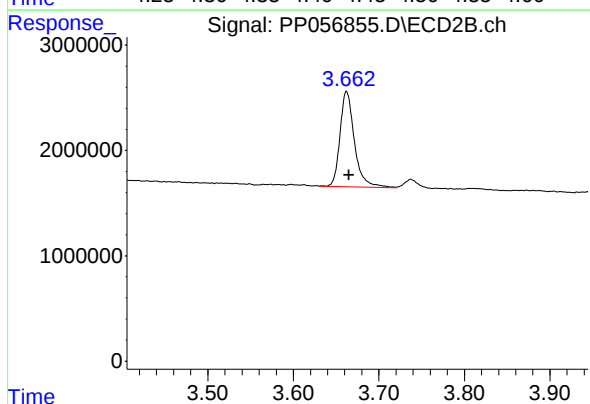


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.003 min
Response: 10617744
Conc: 6.10 ng/ml

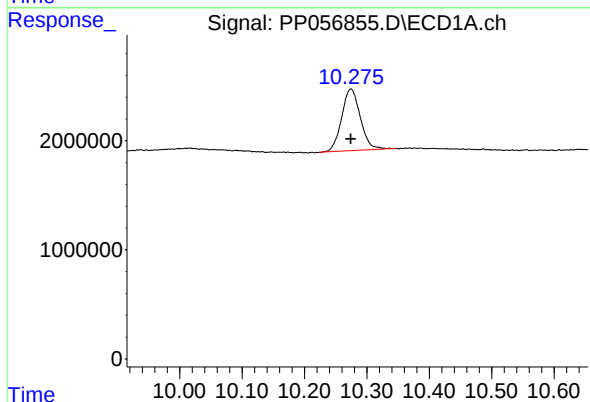

#2 Decachlorobiphenyl

R.T.: 10.275 min
Delta R.T.: 0.000 min
Response: 11803344
Conc: 9.02 ng/ml

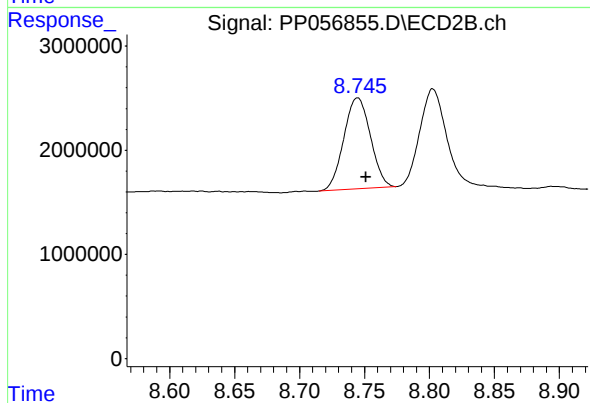

#2 Decachlorobiphenyl

R.T.: 8.745 min
Delta R.T.: -0.007 min
Response: 12459551
Conc: 7.92 ng/ml