

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041125\
Data File : PP071230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2025 13:30
Operator : YP\AJ
Sample : PB167563BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB167563BL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:16:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.516	3.812	36517423	25927837	24.985	25.011m
2) SA Decachlor...	10.234	8.850	27082125	17641113	25.728m	22.382

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041125\
Data File : PP071230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2025 13:30
Operator : YP\AJ
Sample : PB167563BL
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB167563BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:16:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

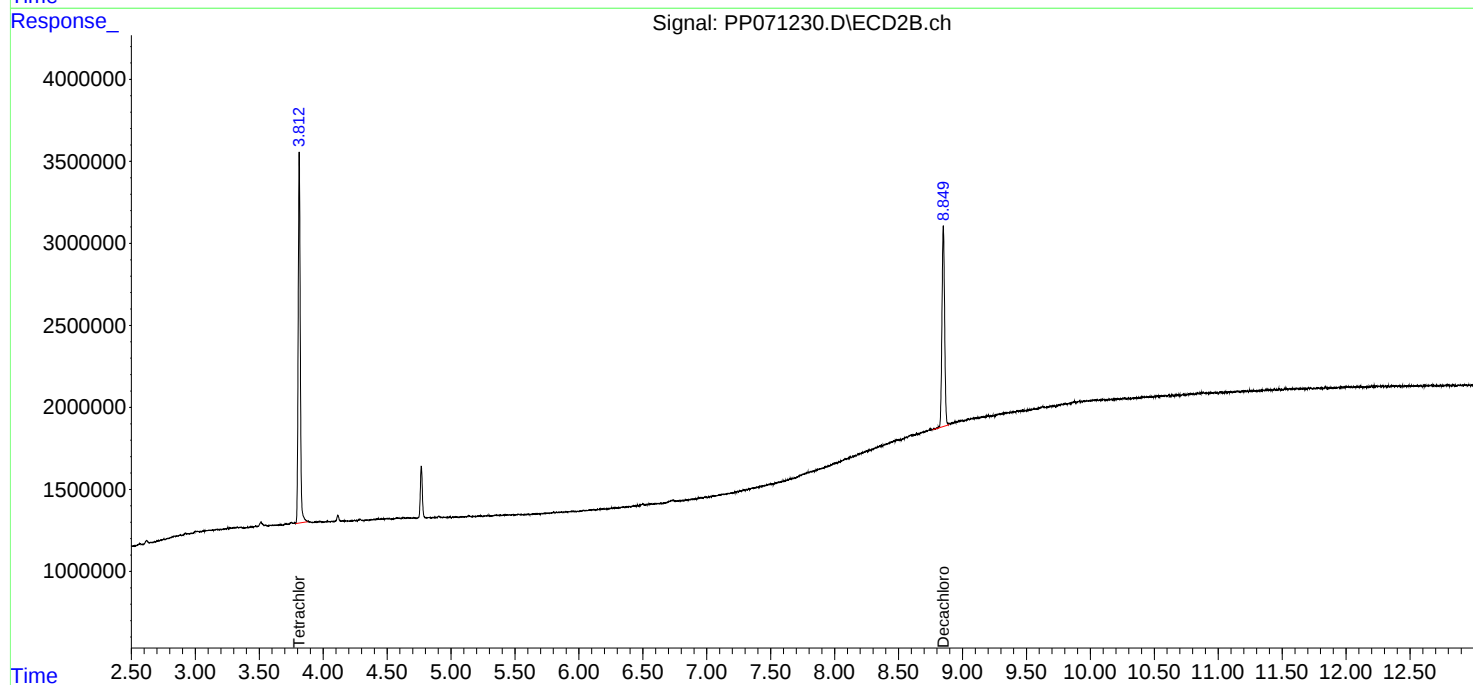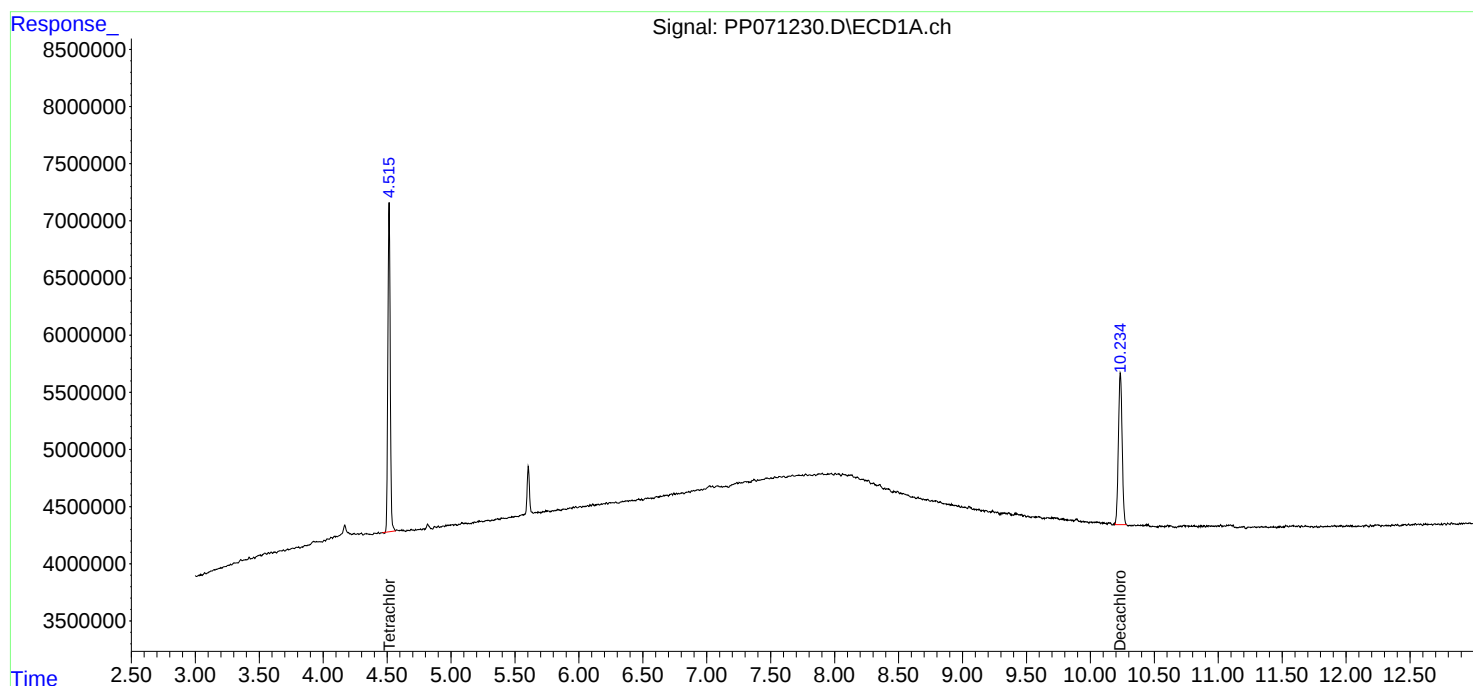

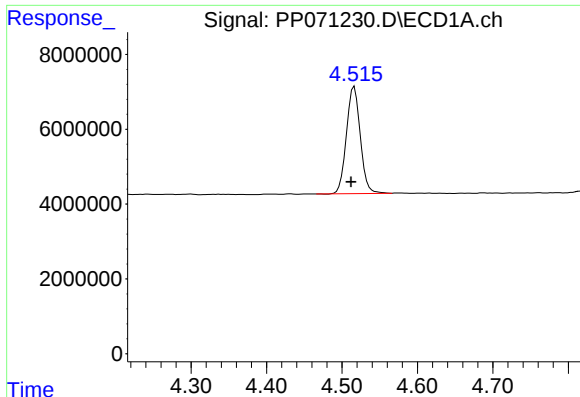


#1 Tetrachloro-m-xylene

R.T.: 4.516 min
Delta R.T.: 0.004 min
Response: 36517423
Conc: 24.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB167563BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

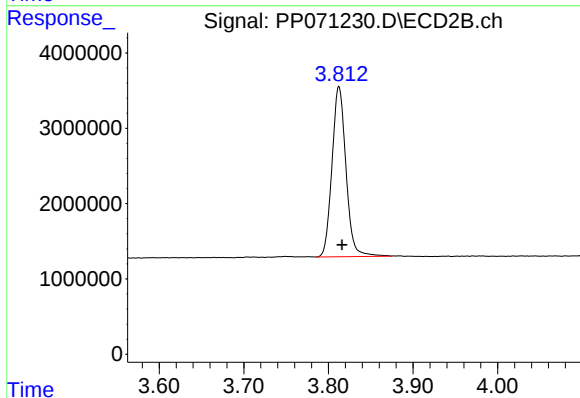


#1 Tetrachloro-m-xylene

R.T.: 3.812 min
Delta R.T.: -0.004 min
Response: 25927837
Conc: 25.01 ng/ml m

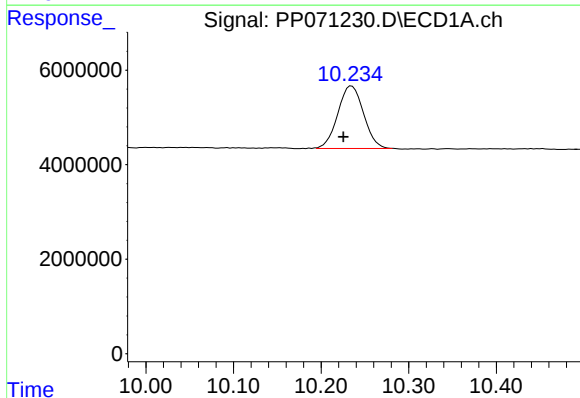

#2 Decachlorobiphenyl

R.T.: 10.234 min
Delta R.T.: 0.008 min
Response: 27082125
Conc: 25.73 ng/ml m

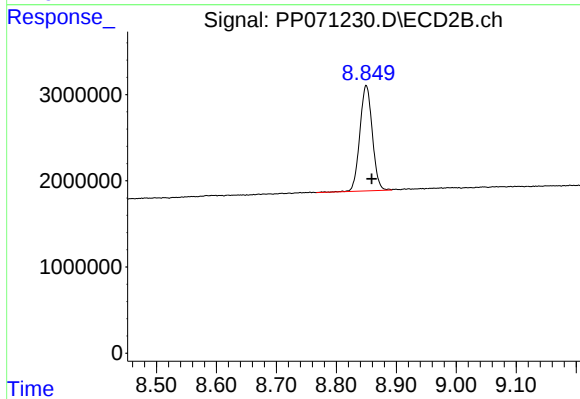

#2 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: -0.009 min
Response: 17641113
Conc: 22.38 ng/ml