

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041125\
 Data File : PP071235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2025 14:52
 Operator : YP\AJ
 Sample : Q1767-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NWB-2152

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/14/2025
 Supervised By :mohammad ahmed 04/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 00:17:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.513	3.814	27905827	25333497	19.093m	24.438 #
2) SA Decachlor...	10.233	8.850	13976569	9442958	13.278	11.980

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041125\
Data File : PP071235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2025 14:52
Operator : YP\AJ
Sample : Q1767-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NWB-2152


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:17:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

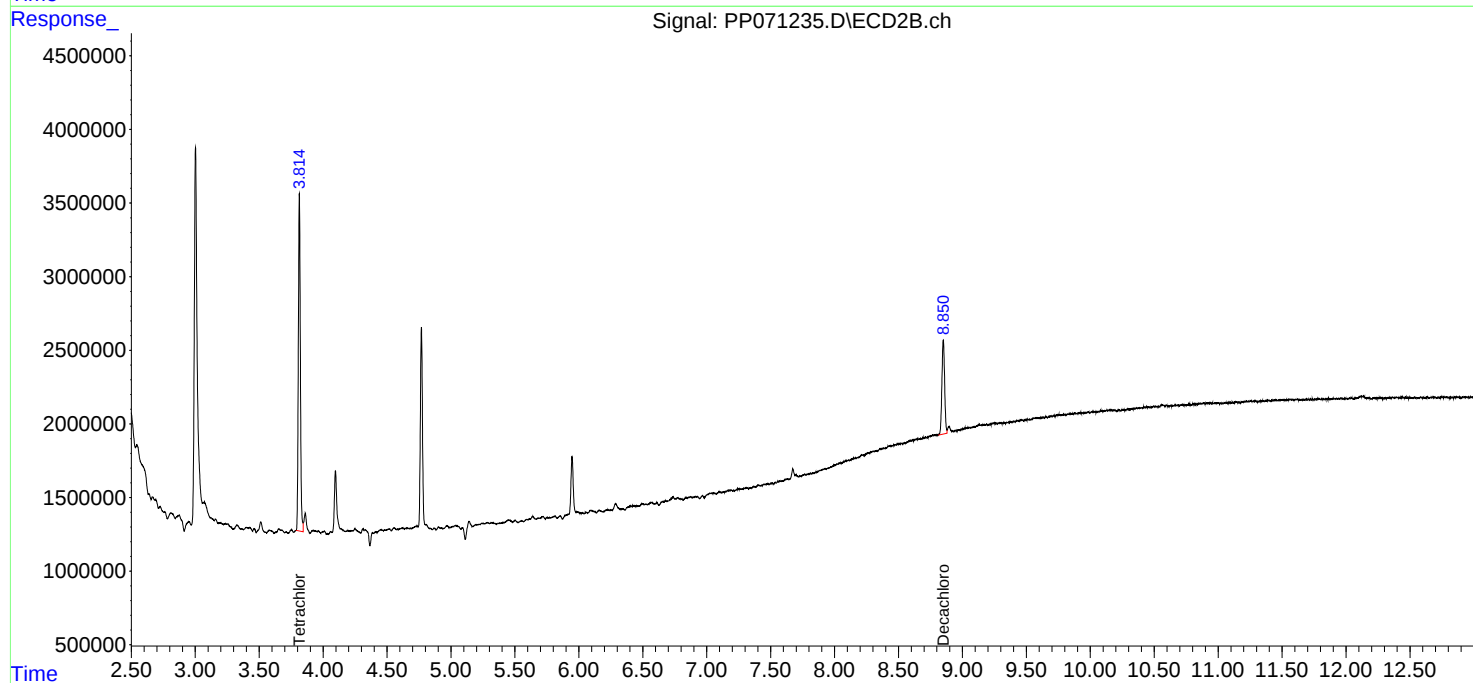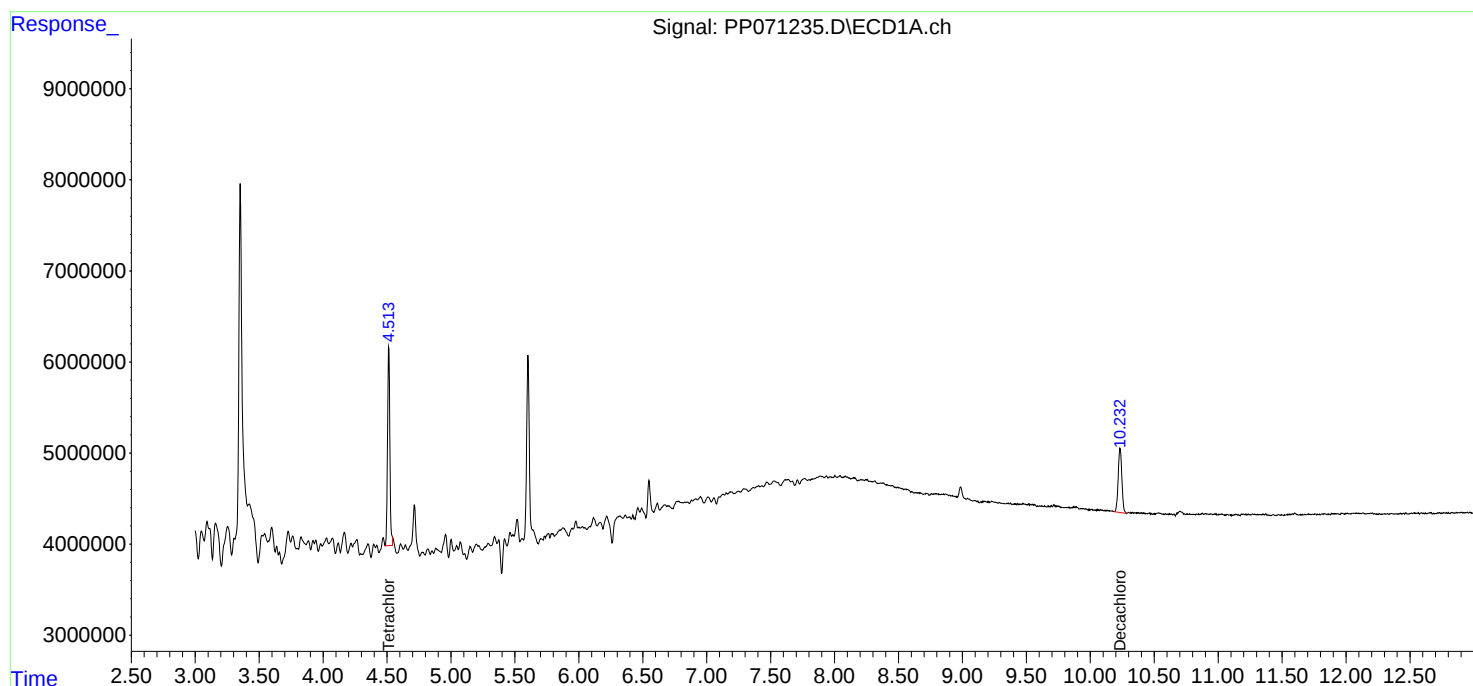

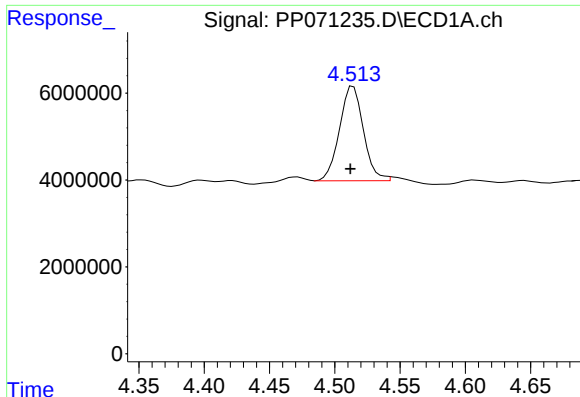


#1 Tetrachloro-m-xylene

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 27905827
Conc: 19.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
NWB-2152


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

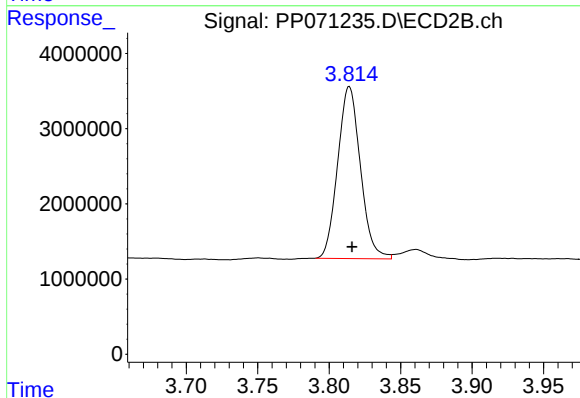


#1 Tetrachloro-m-xylene

R.T.: 3.814 min
Delta R.T.: -0.002 min
Response: 25333497
Conc: 24.44 ng/ml

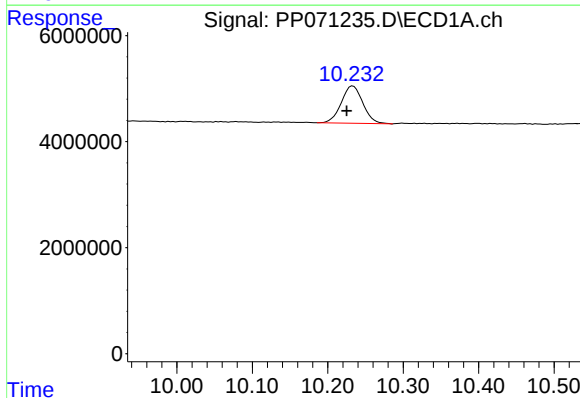

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: 0.008 min
Response: 13976569
Conc: 13.28 ng/ml

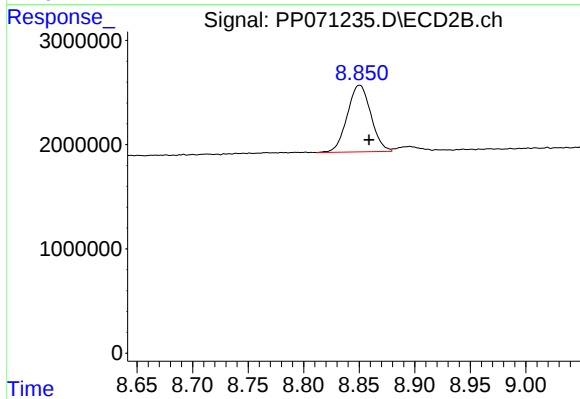

#2 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: -0.008 min
Response: 9442958
Conc: 11.98 ng/ml