

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041125\
 Data File : PP071236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2025 15:08
 Operator : YP\AJ
 Sample : Q1767-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NWB-2106

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/14/2025
 Supervised By :mohammad ahmed 04/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 00:17:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.511	3.816	26577929	15457260	18.184m	14.911m
2) SA Decachlor...	10.254	8.870	20618115	14337759	19.587m	18.191

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041125\
Data File : PP071236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2025 15:08
Operator : YP\AJ
Sample : Q1767-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NWB-2106


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:17:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

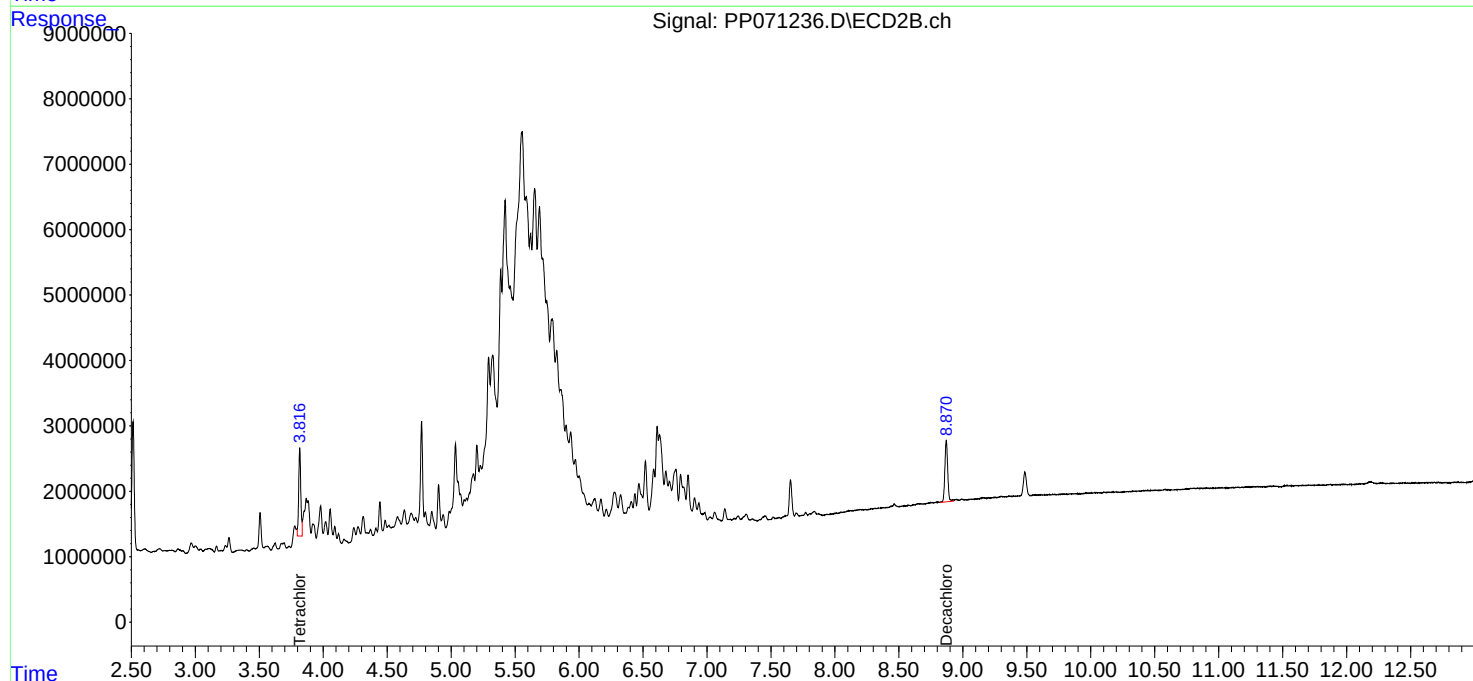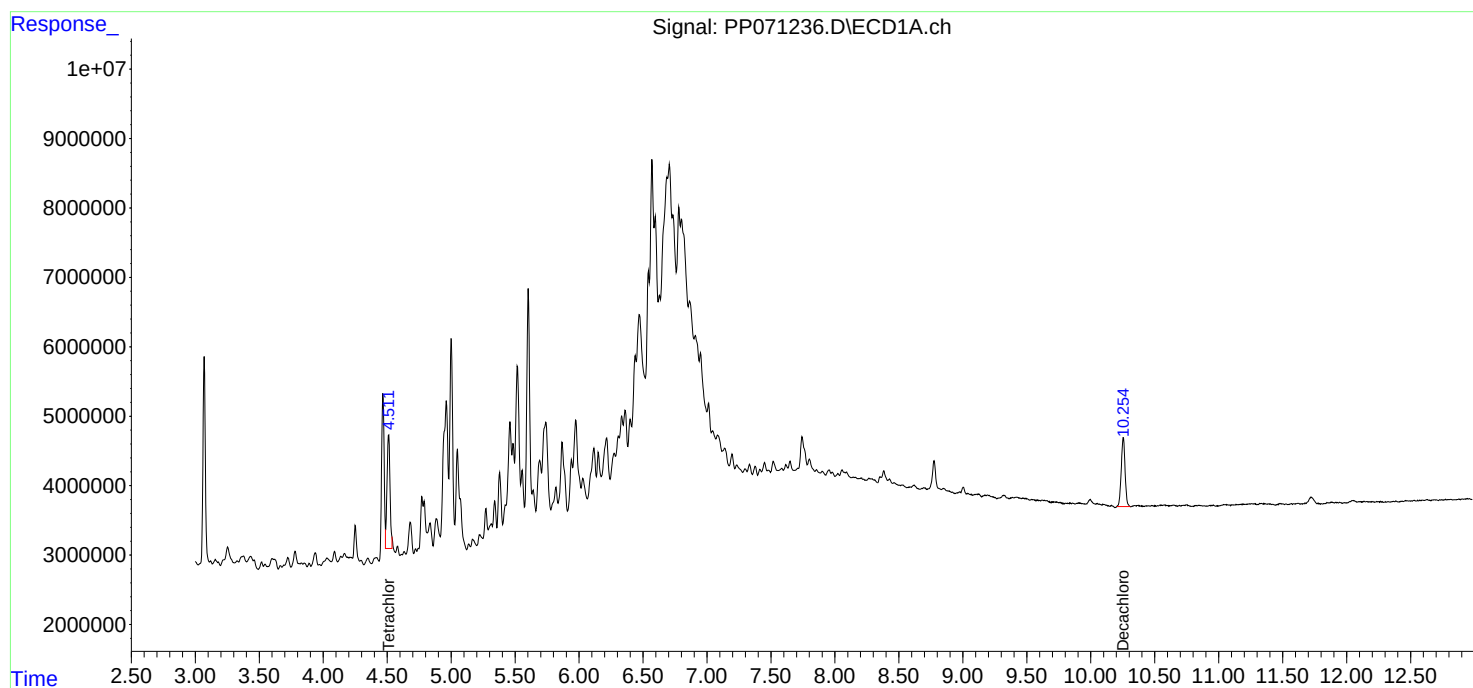

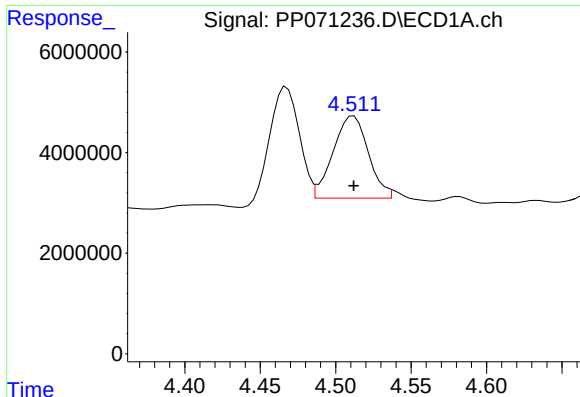


#1 Tetrachloro-m-xylene

R.T.: 4.511 min
Delta R.T.: -0.001 min
Response: 26577929
Conc: 18.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
NWB-2106


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

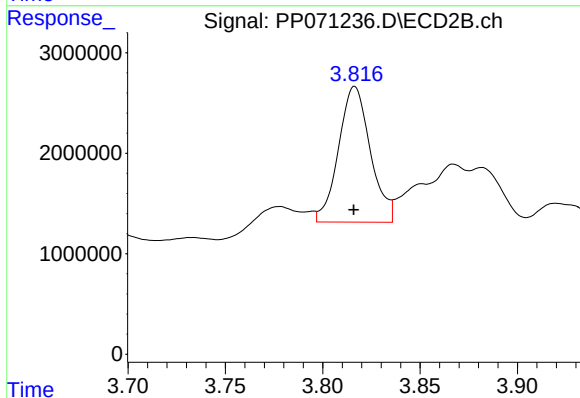


#1 Tetrachloro-m-xylene

R.T.: 3.816 min
Delta R.T.: 0.000 min
Response: 15457260
Conc: 14.91 ng/ml m

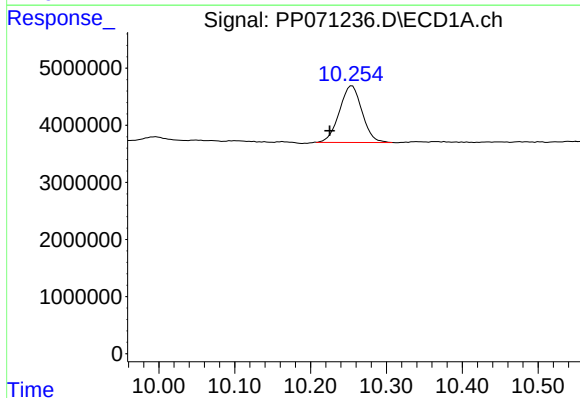

#2 Decachlorobiphenyl

R.T.: 10.254 min
Delta R.T.: 0.028 min
Response: 20618115
Conc: 19.59 ng/ml m

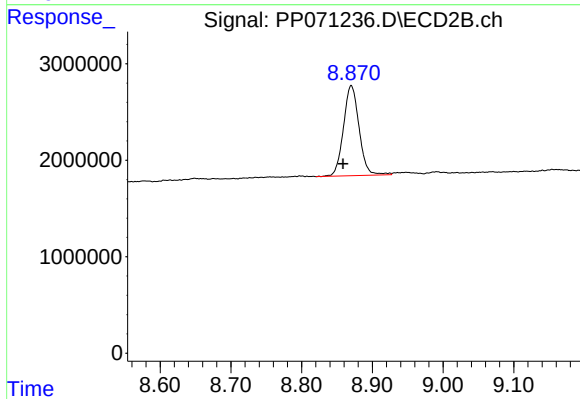

#2 Decachlorobiphenyl

R.T.: 8.870 min
Delta R.T.: 0.011 min
Response: 14337759
Conc: 18.19 ng/ml