

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041221\
 Data File : PP034811.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2021 14:50
 Operator : DD\AJ
 Sample : M1998-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-3A

Manual Integrations
 APPROVED

Ankita
 4/13/2021 1:15:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 08:54:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.843	4.256	1646738	890746	21.587	19.829m
2) SA Decachlor...	10.760	9.553	1821656	711061	23.664	25.183m
Target Compounds						
21) L5 AR-1248-1	6.154	5.505	486698	270916	342.159	371.361
22) L5 AR-1248-2	6.447	5.767	628591	316949	317.647	308.765
23) L5 AR-1248-3	6.663	5.811	668217	373079	281.107	340.403
24) L5 AR-1248-4	7.089	5.998	694314	369207	272.078	292.528
25) L5 AR-1248-5	7.130	6.417	1155976	406246	453.645	359.465

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041221\
Data File : PP034811.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2021 14:50
Operator : DD\AJ
Sample : M1998-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-3A


Manual Integrations
APPROVED

Ankita
4/13/2021 1:15:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 08:54:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

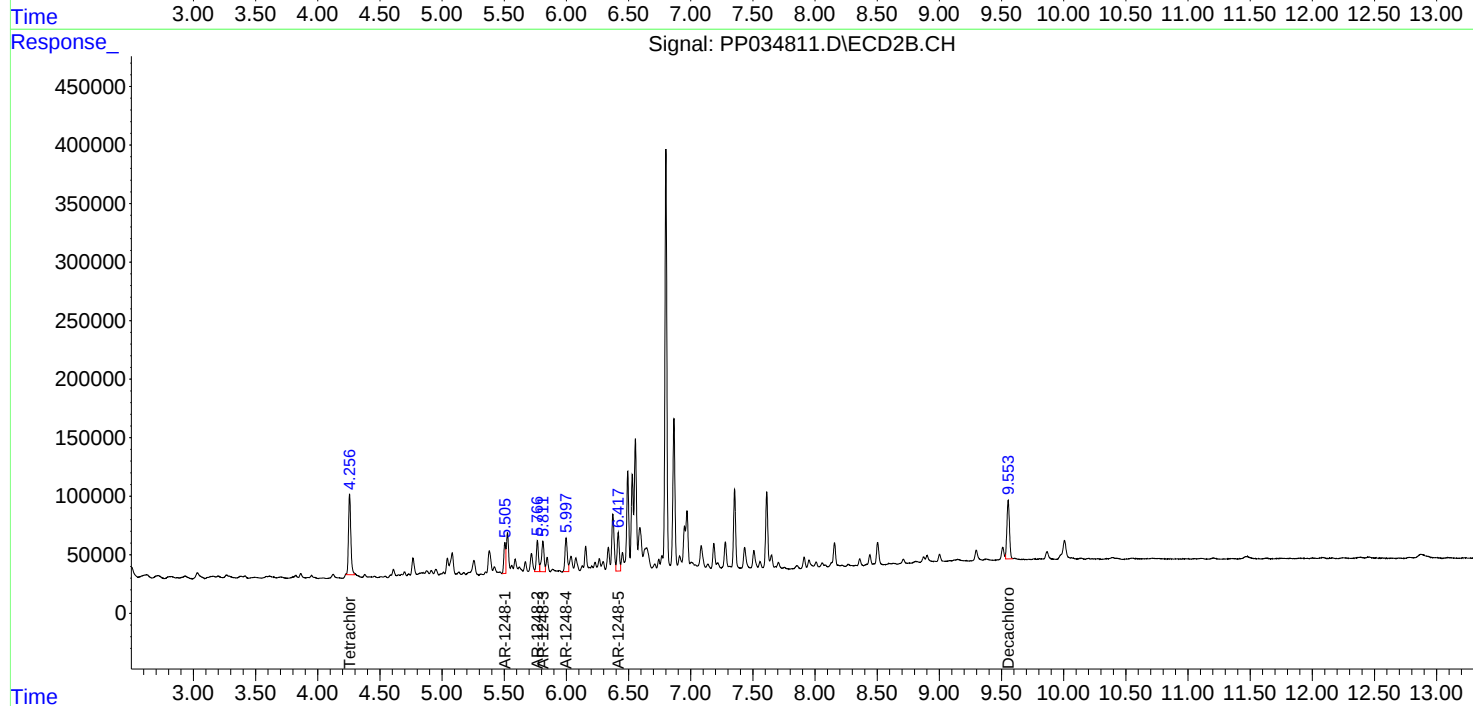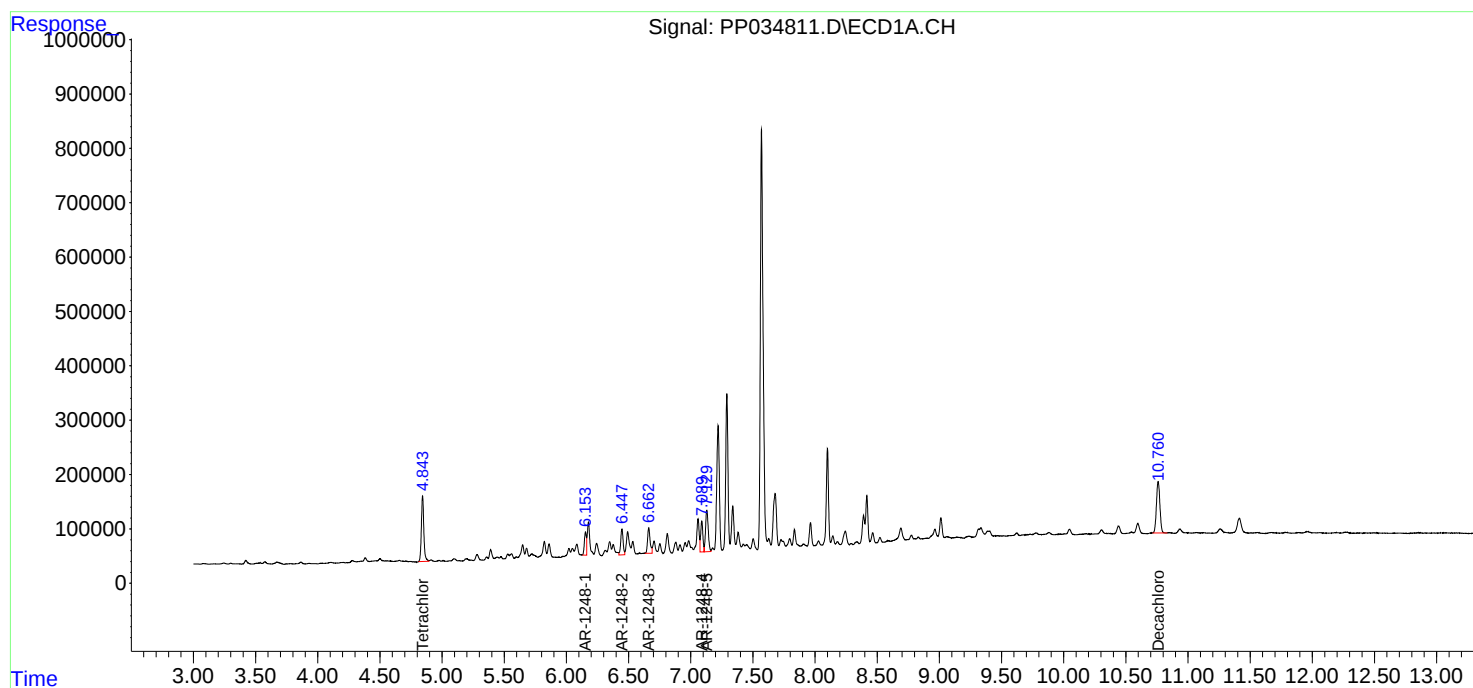

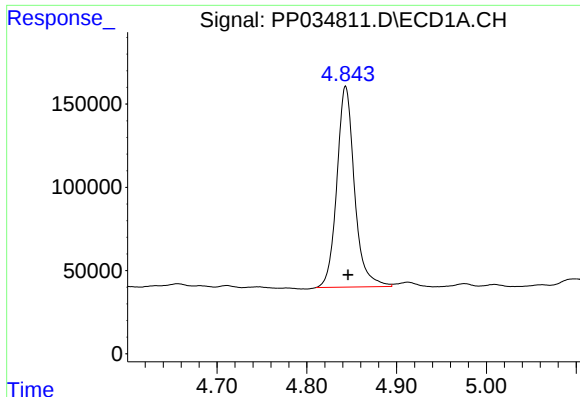


#1 Tetrachloro-m-xylene

R.T.: 4.843 min
Delta R.T.: -0.003 min
Response: 1646738
Conc: 21.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-3A


Manual Integrations
APPROVED

Ankita
4/13/2021 1:15:33 PM

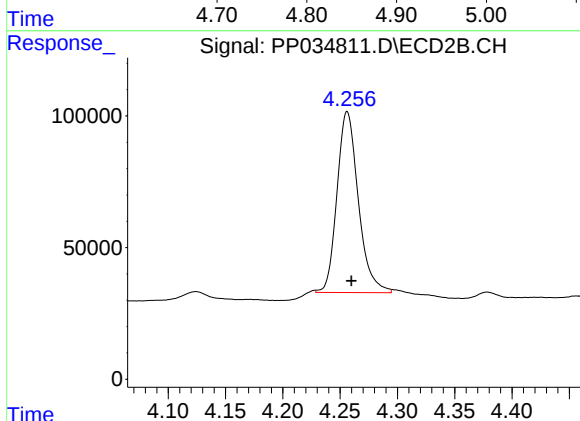


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.004 min
Response: 890746
Conc: 19.83 ng/ml m

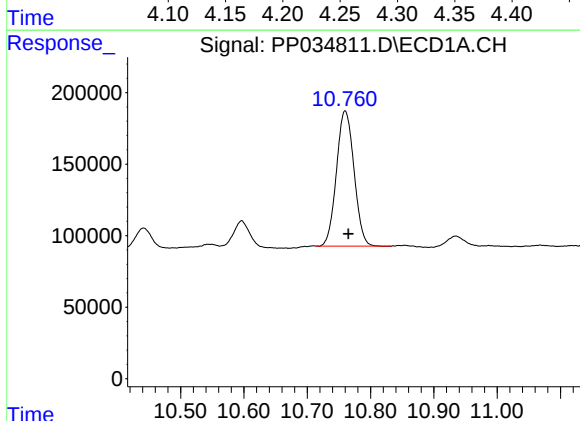


#2 Decachlorobiphenyl

R.T.: 10.760 min
Delta R.T.: -0.005 min
Response: 1821656
Conc: 23.66 ng/ml

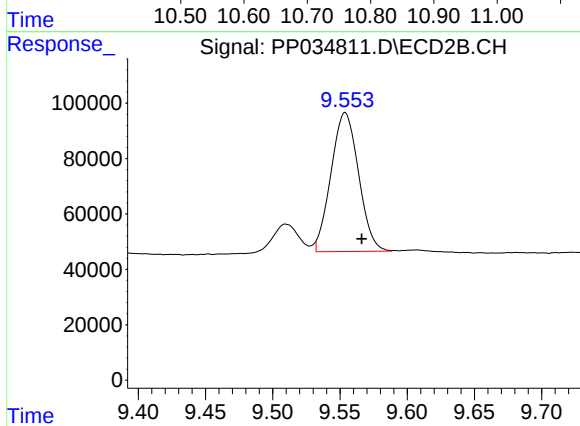

#2 Decachlorobiphenyl

R.T.: 9.553 min
Delta R.T.: -0.013 min
Response: 711061
Conc: 25.18 ng/ml m

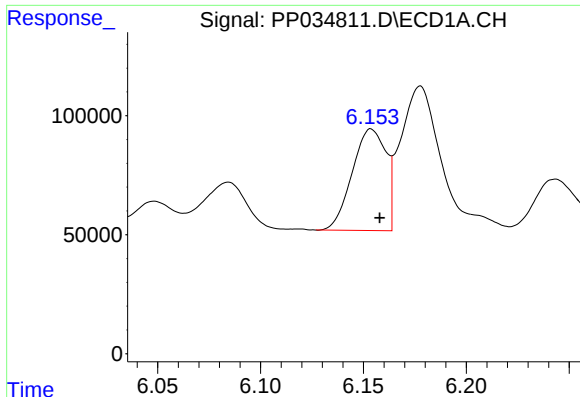


#21 AR-1248-1

R.T.: 6.154 min
Delta R.T.: -0.004 min
Response: 486698
Conc: 342.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-3A


Manual Integrations
APPROVED

Ankita
4/13/2021 1:15:33 PM

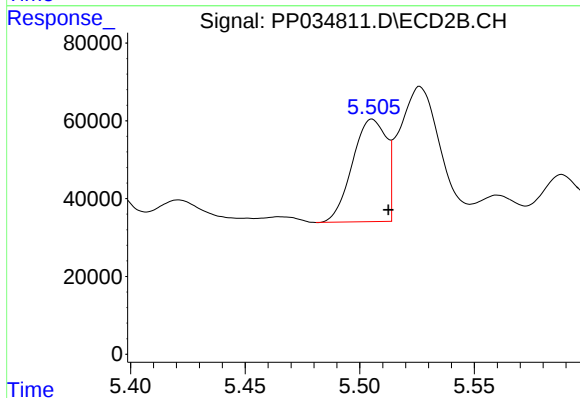


#21 AR-1248-1

R.T.: 5.505 min
Delta R.T.: -0.007 min
Response: 270916
Conc: 371.36 ng/ml

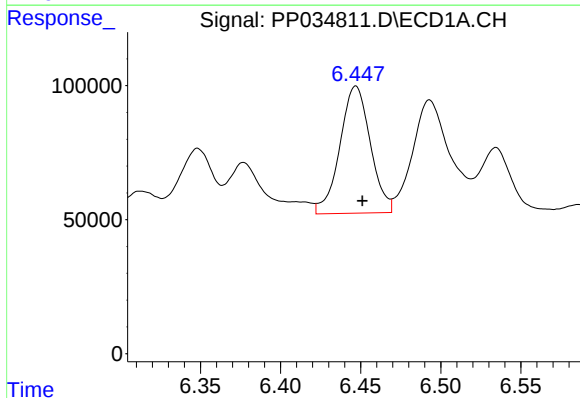


#22 AR-1248-2

R.T.: 6.447 min
Delta R.T.: -0.004 min
Response: 628591
Conc: 317.65 ng/ml

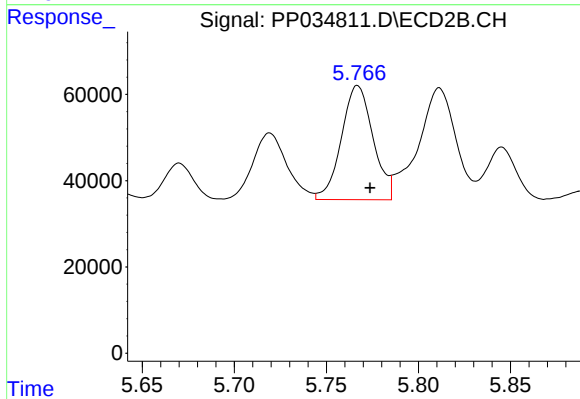

#22 AR-1248-2

R.T.: 5.767 min
Delta R.T.: -0.007 min
Response: 316949
Conc: 308.77 ng/ml

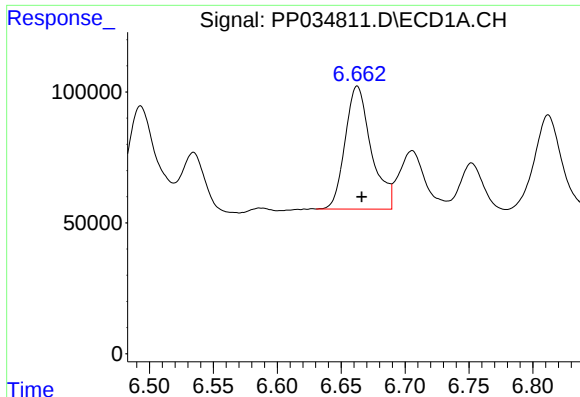


#23 AR-1248-3

R.T.: 6.663 min
Delta R.T.: -0.004 min
Response: 668217
Conc: 281.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-3A


Manual Integrations
APPROVED

Ankita
4/13/2021 1:15:33 PM

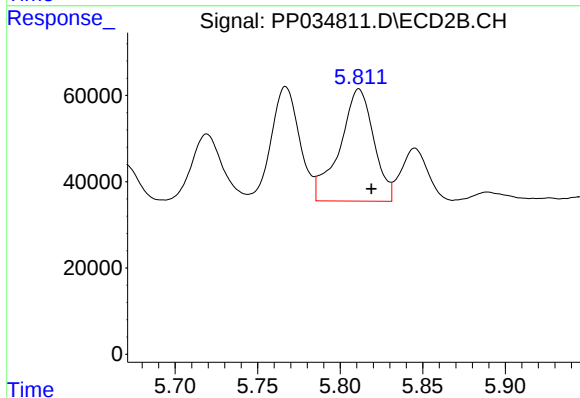


#23 AR-1248-3

R.T.: 5.811 min
Delta R.T.: -0.008 min
Response: 373079
Conc: 340.40 ng/ml

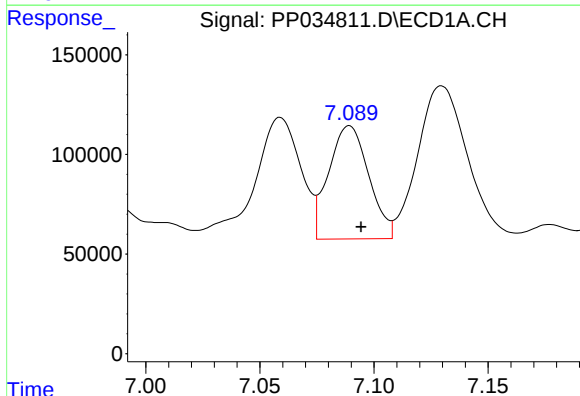


#24 AR-1248-4

R.T.: 7.089 min
Delta R.T.: -0.005 min
Response: 694314
Conc: 272.08 ng/ml

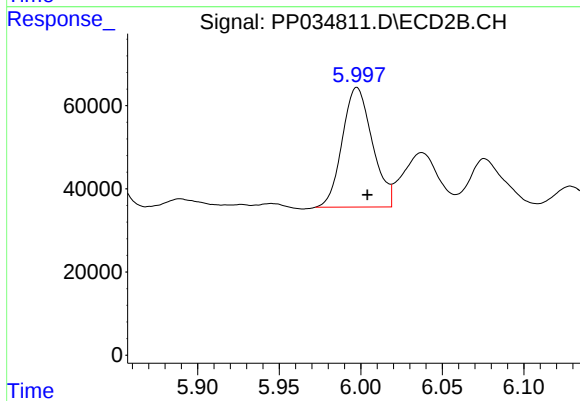

#24 AR-1248-4

R.T.: 5.998 min
Delta R.T.: -0.006 min
Response: 369207
Conc: 292.53 ng/ml

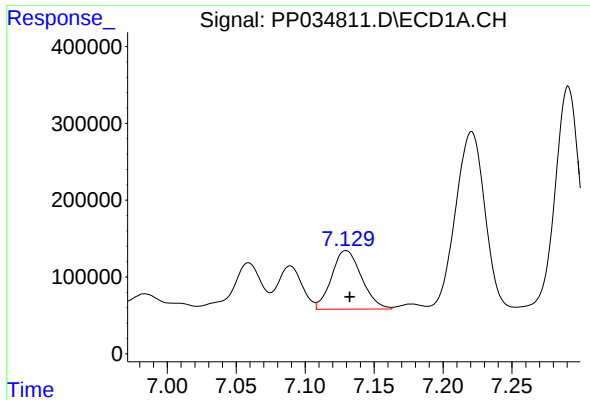


#25 AR-1248-5

R.T.: 7.130 min
Delta R.T.: -0.003 min
Response: 1155976
Conc: 453.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-3A

Manual Integrations
APPROVED

Ankita
4/13/2021 1:15:33 PM

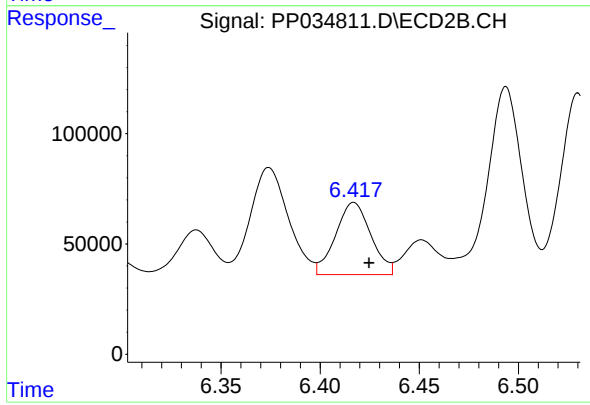

#25 AR-1248-5

R.T.: 6.417 min
Delta R.T.: -0.008 min
Response: 406246
Conc: 359.47 ng/ml