

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041221\
 Data File : PP034832.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2021 21:02
 Operator : DD\AJ
 Sample : M1997-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RBR-58-56

Manual Integrations
 APPROVED

Ankita
 4/13/2021 1:19:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 02:10:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.843	4.257	1286436	801385	16.864	17.839
2) SA Decachlor...	10.757	9.553	1127278	396414	14.644m	14.039

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041221\
Data File : PP034832.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2021 21:02
Operator : DD\AJ
Sample : M1997-02
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RBR-58-56


Manual Integrations
APPROVED

Ankita
4/13/2021 1:19:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 02:10:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

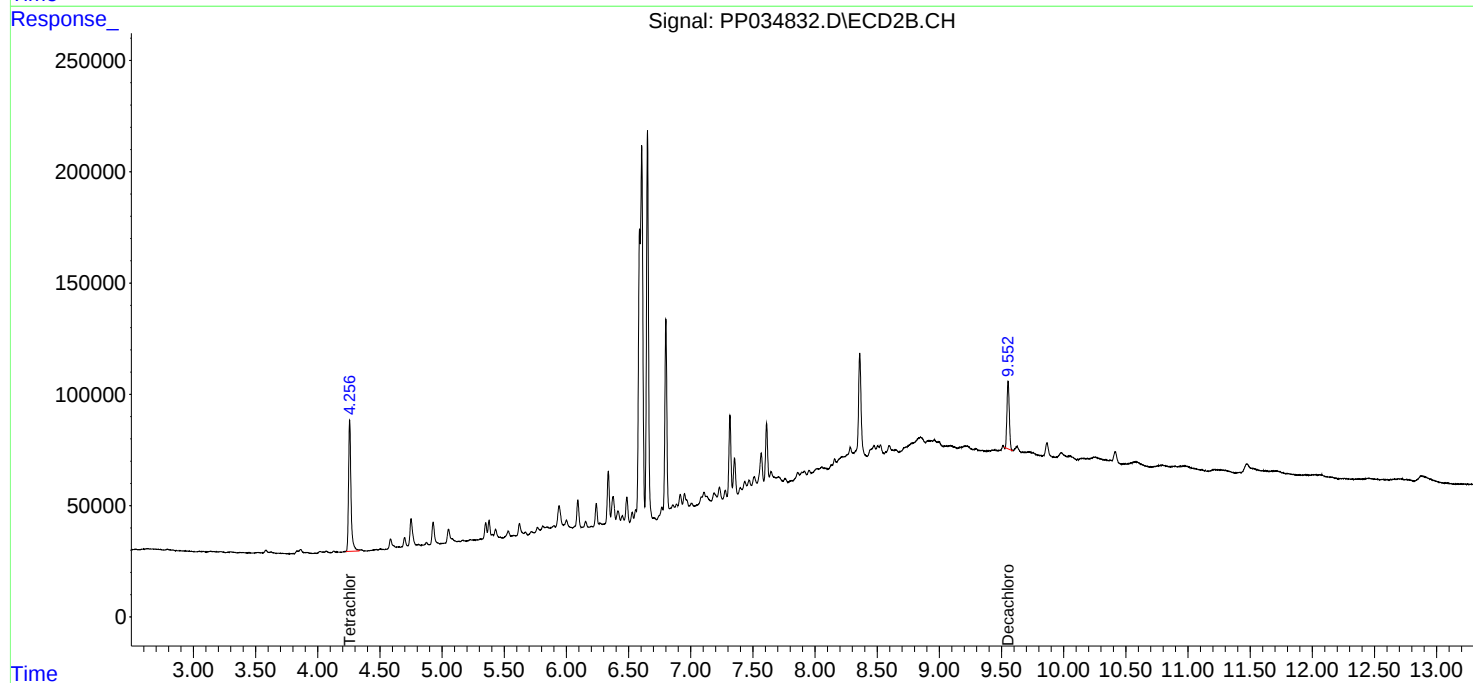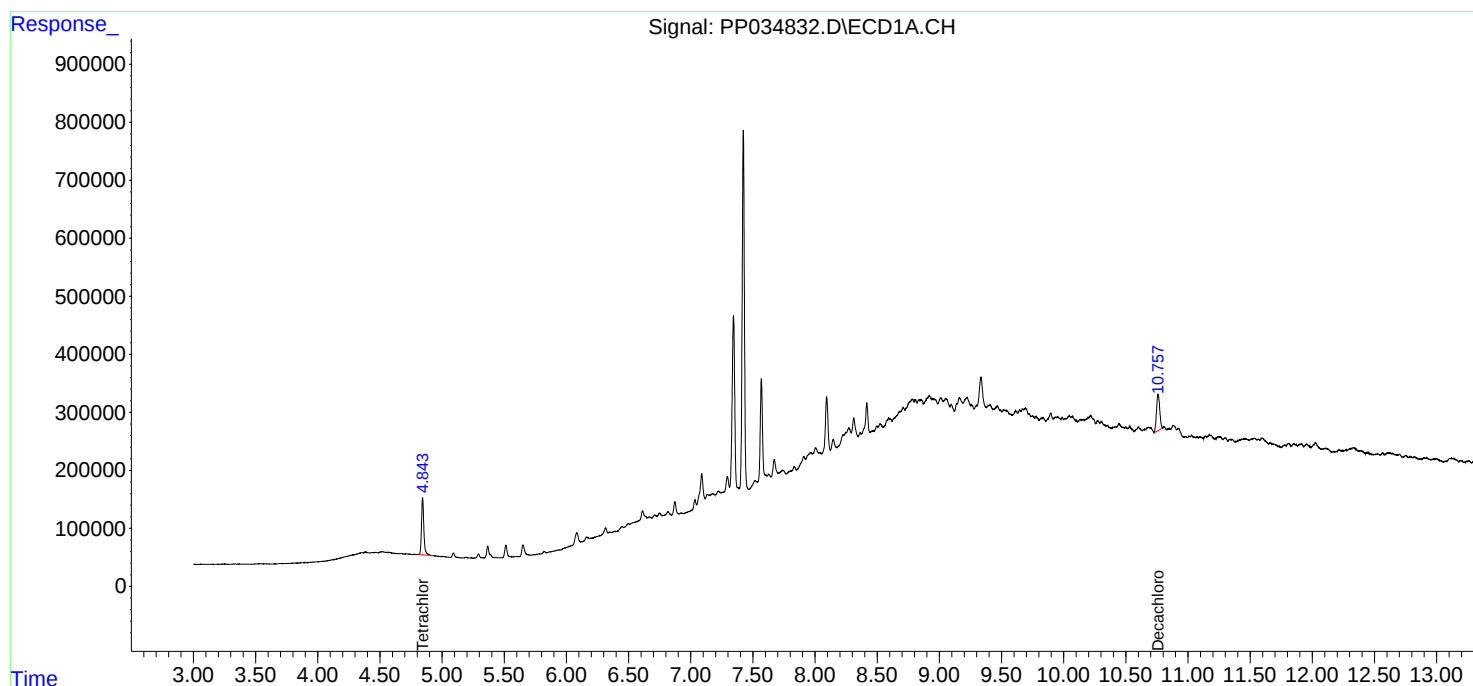

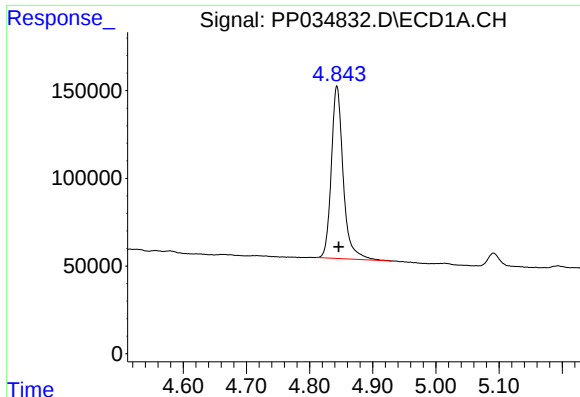


#1 Tetrachloro-m-xylene

R.T.: 4.843 min
Delta R.T.: -0.003 min
Response: 1286436
Conc: 16.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
RBR-58-56


Manual Integrations
APPROVED

Ankita
4/13/2021 1:19:25 PM

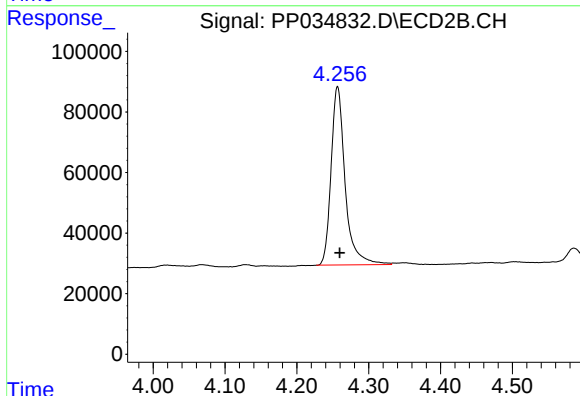


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: -0.003 min
Response: 801385
Conc: 17.84 ng/ml

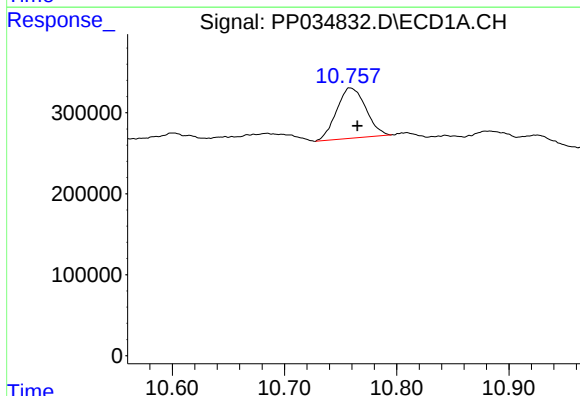

#2 Decachlorobiphenyl

R.T.: 10.757 min
Delta R.T.: -0.008 min
Response: 1127278
Conc: 14.64 ng/ml m

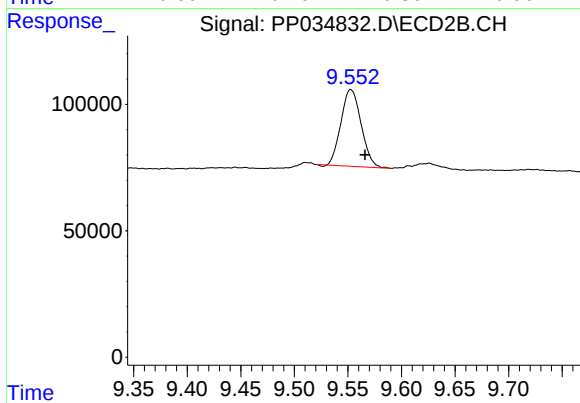

#2 Decachlorobiphenyl

R.T.: 9.553 min
Delta R.T.: -0.013 min
Response: 396414
Conc: 14.04 ng/ml