

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041224\
 Data File : PP064293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2024 15:52
 Operator : YP\AJ
 Sample : P2087-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 60186

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/15/2024
 Supervised By :Ankita Jodhani 04/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 01:27:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.486	3.637	34470556	32958276	14.446m	13.804m
2) SA Decachlor...	10.361	8.669	20663446	20871920	8.138	7.723

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041224\
Data File : PP064293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2024 15:52
Operator : YP\AJ
Sample : P2087-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
60186


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2024
Supervised By :Ankita Jodhani 04/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 01:27:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

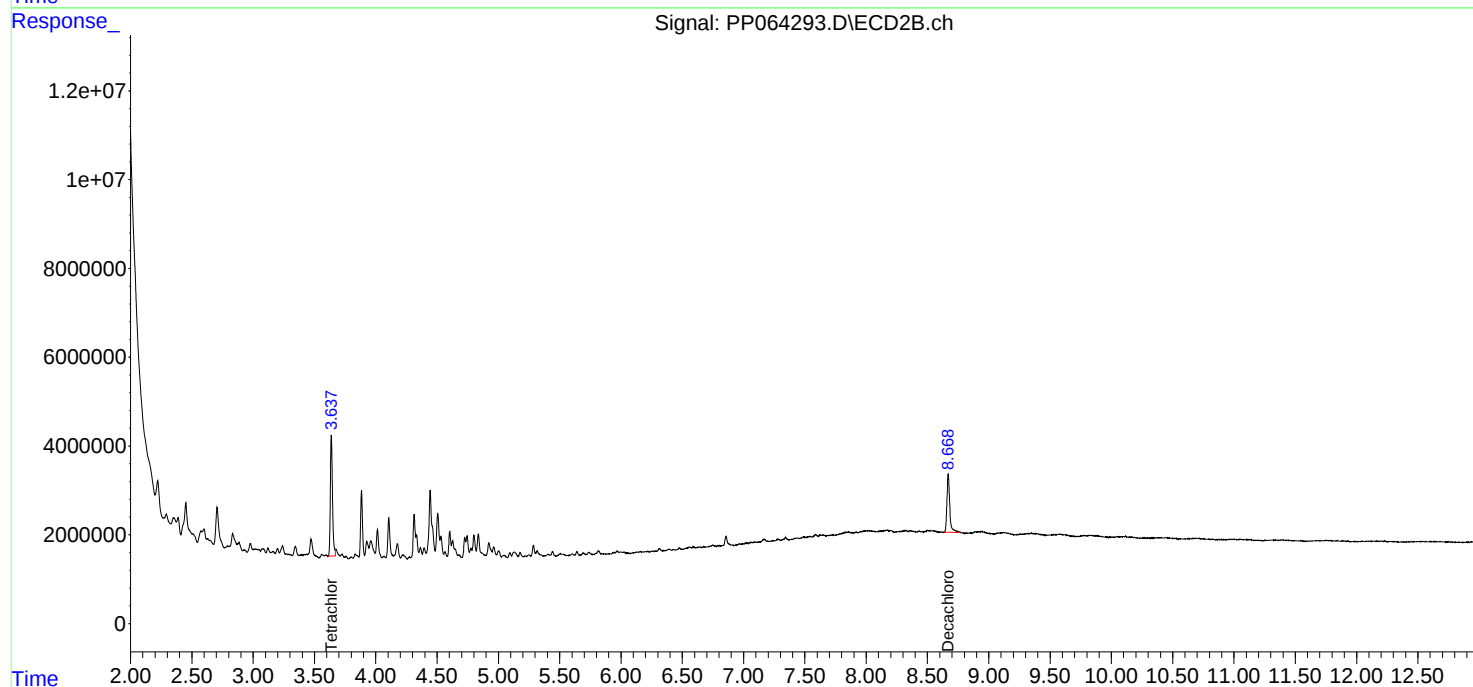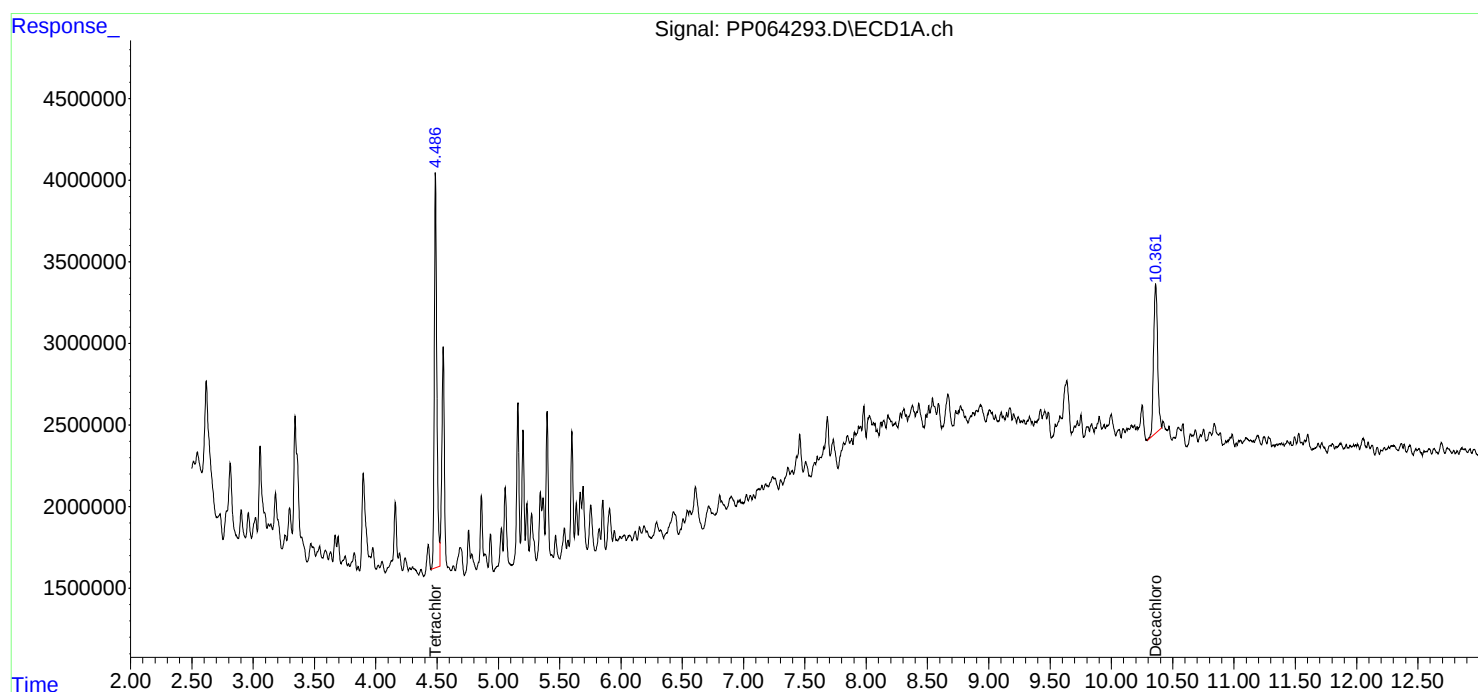

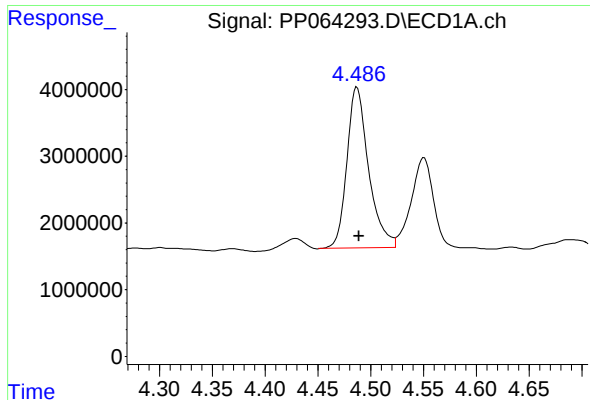


#1 Tetrachloro-m-xylene

R.T.: 4.486 min
Delta R.T.: -0.003 min
Response: 34470556
Conc: 14.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
60186


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2024
Supervised By :Ankita Jodhani 04/15/2024

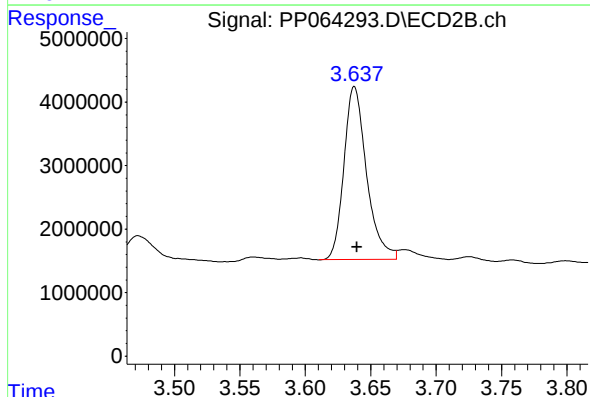


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 32958276
Conc: 13.80 ng/ml

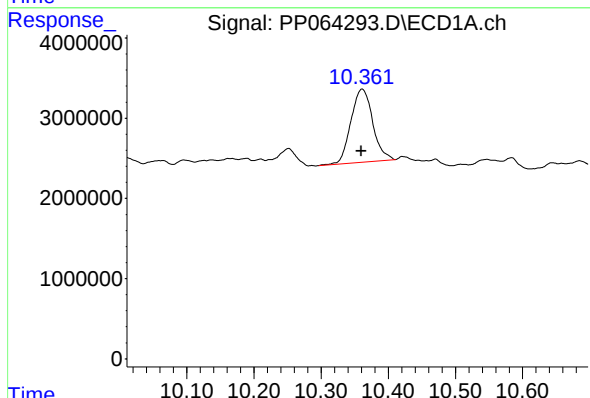

#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: 0.001 min
Response: 20663446
Conc: 8.14 ng/ml

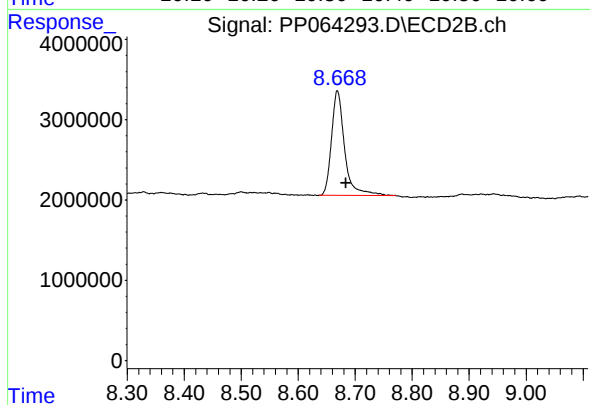

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: -0.015 min
Response: 20871920
Conc: 7.72 ng/ml