

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041321\
 Data File : PP034840.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2021 10:11
 Operator : DD\AJ
 Sample : M1993-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 T-2

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 15:38:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.843	4.258	1456385	858916	19.092	19.120
2) SA Decachlor...	10.757	9.550	2202201	679064	28.607	24.050
Target Compounds						
26) L6 AR-1254-1	7.064	6.378	450170	191787	163.726	103.955 #
27) L6 AR-1254-2	7.292	6.532	472966	129515	111.230	80.953 #
28) L6 AR-1254-3	7.668	6.950	443706	328911	97.215m	131.788m#
29) L6 AR-1254-4	7.964	7.184	540221	147430	174.724m	112.153m#
30) L6 AR-1254-5	8.388	7.609	800462	337829	225.239m	166.219m#

Ankita

4/14/2021
 1:49:29 PM

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041321\
Data File : PP034840.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2021 10:11
Operator : DD\AJ
Sample : M1993-03
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampled :
T-2

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 15:38:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

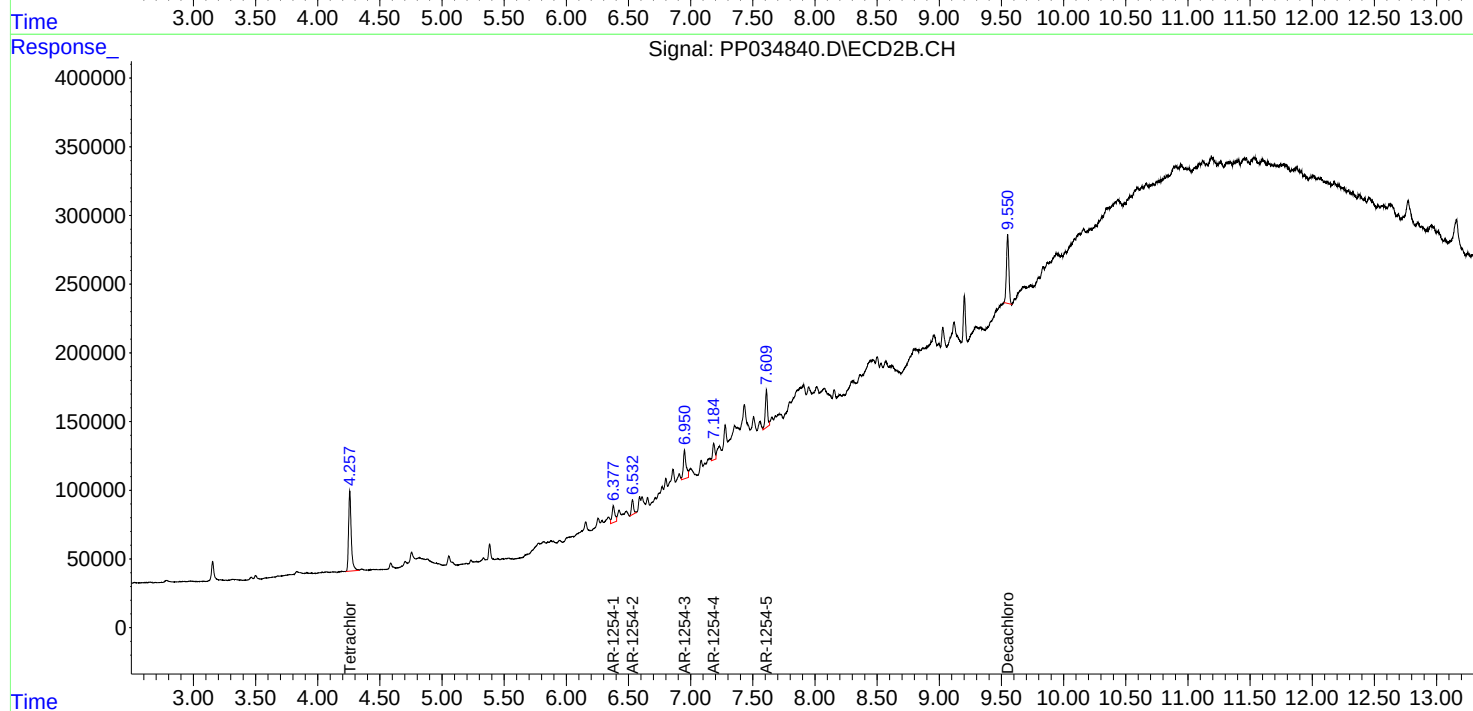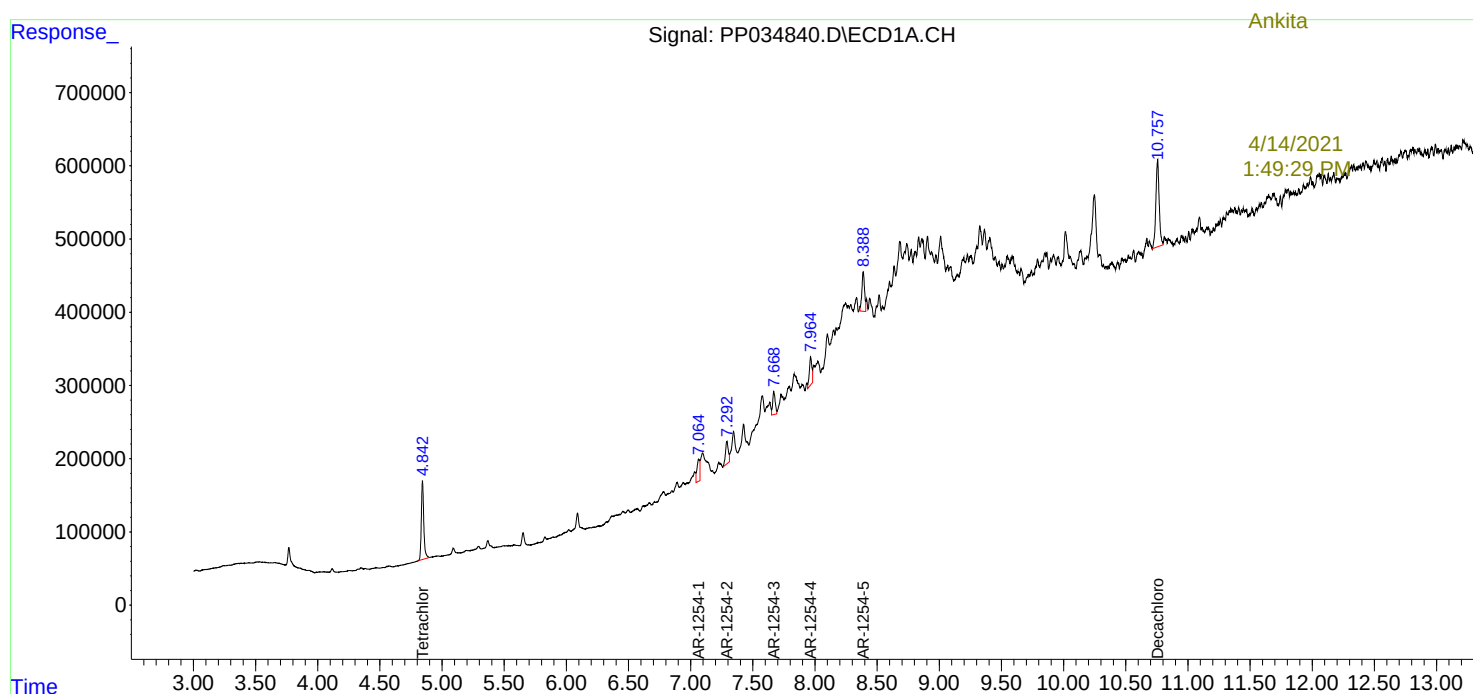

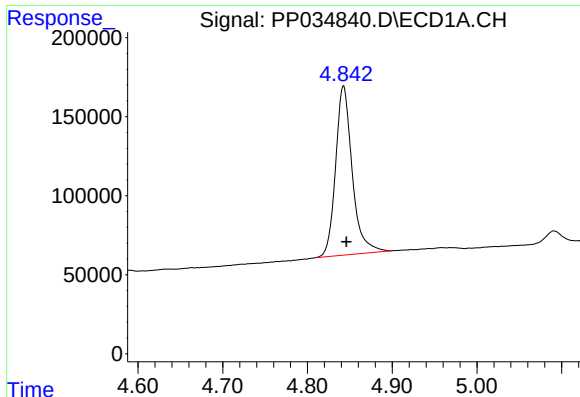


#1 Tetrachloro-m-xylene

R.T.: 4.843 min
Delta R.T.: -0.003 min
Response: 1456385
Conc: 19.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
T-2

Manual Integrations
APPROVED

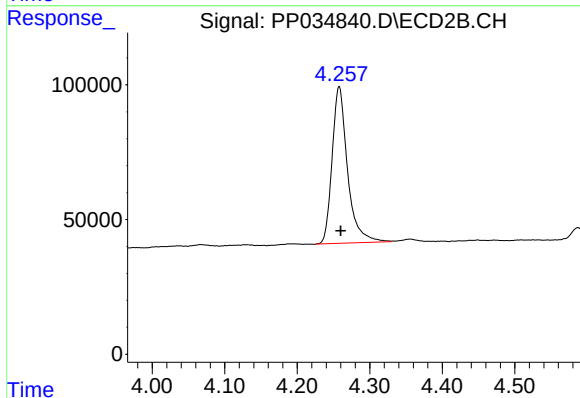


#1 Tetrachloro-m-xylene

R.T.: 4.258 min
Delta R.T.: -0.002 min
Response: 858916
Conc: 19.12 ng/ml


Ankita

4/14/2021
1:49:29 PM

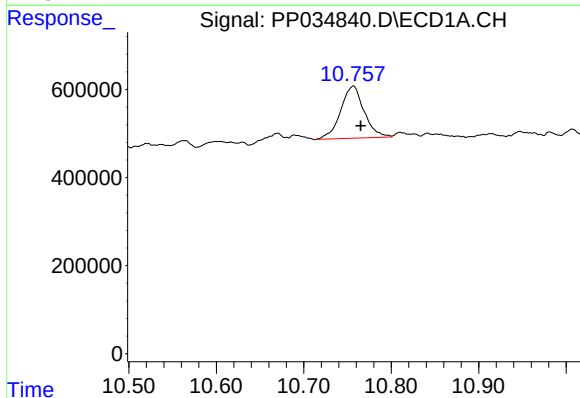


#2 Decachlorobiphenyl

R.T.: 10.757 min
Delta R.T.: -0.008 min
Response: 2202201
Conc: 28.61 ng/ml

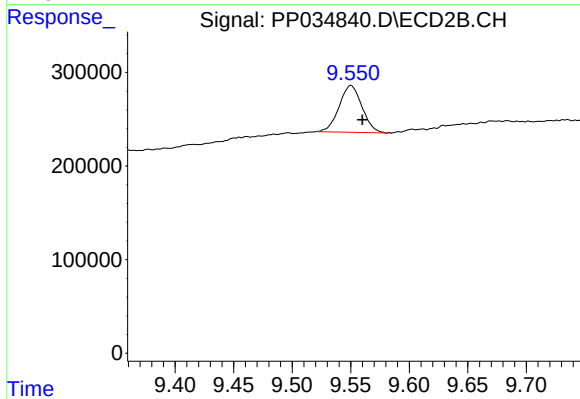

#2 Decachlorobiphenyl

R.T.: 9.550 min
Delta R.T.: -0.010 min
Response: 679064
Conc: 24.05 ng/ml

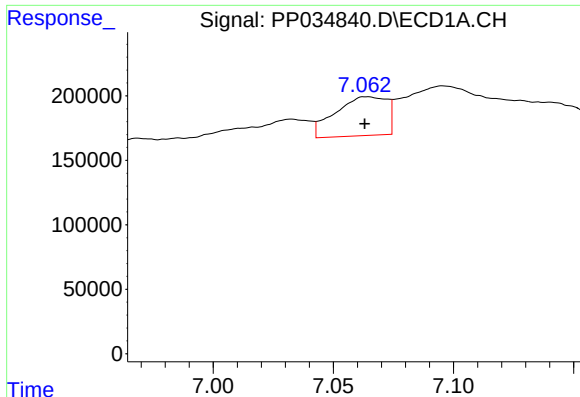


#26 AR-1254-1

R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 450170
Conc: 163.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
T-2

Manual Integrations
APPROVED

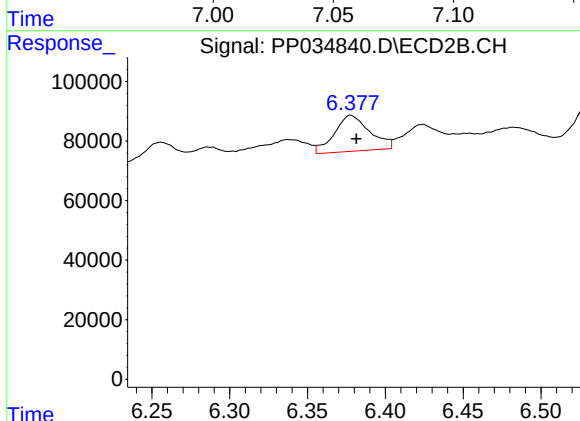


#26 AR-1254-1

R.T.: 6.378 min
Delta R.T.: -0.004 min
Response: 191787
Conc: 103.95 ng/ml


Ankita

4/14/2021
1:49:29 PM

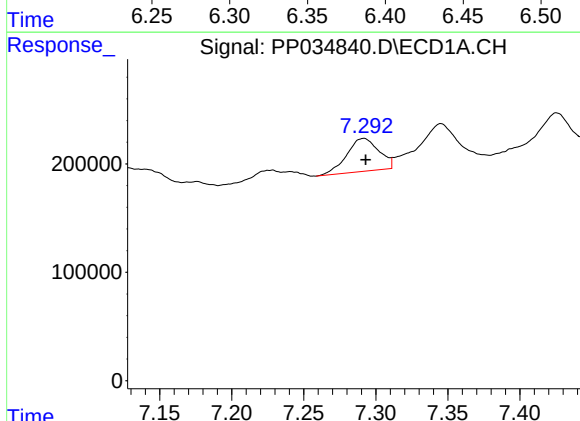


#27 AR-1254-2

R.T.: 7.292 min
Delta R.T.: -0.001 min
Response: 472966
Conc: 111.23 ng/ml

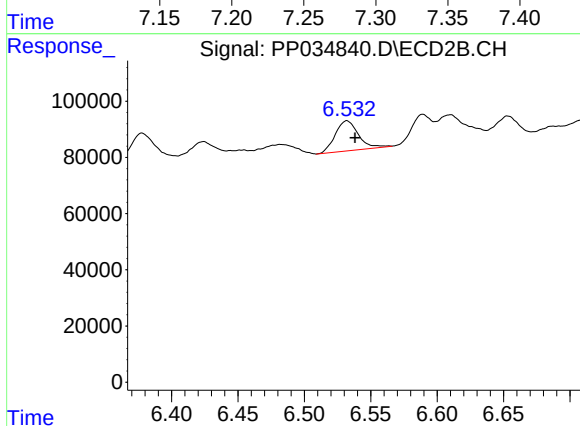

#27 AR-1254-2

R.T.: 6.532 min
Delta R.T.: -0.006 min
Response: 129515
Conc: 80.95 ng/ml

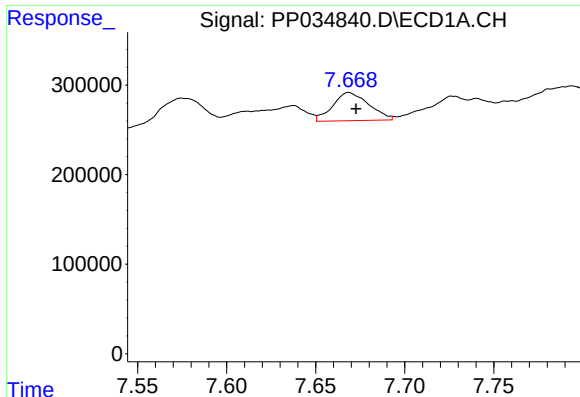


#28 AR-1254-3

R.T.: 7.668 min
Delta R.T.: -0.005 min
Response: 443706
Conc: 97.21 ng/ml m

Instrument :
ECD_P
ClientSampleId :
T-2

Manual Integrations
APPROVED

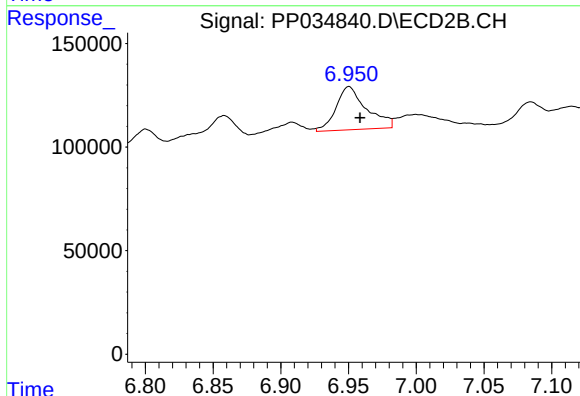


#28 AR-1254-3

R.T.: 6.950 min
Delta R.T.: -0.008 min
Response: 328911
Conc: 131.79 ng/ml m


Ankita

4/14/2021
1:49:29 PM

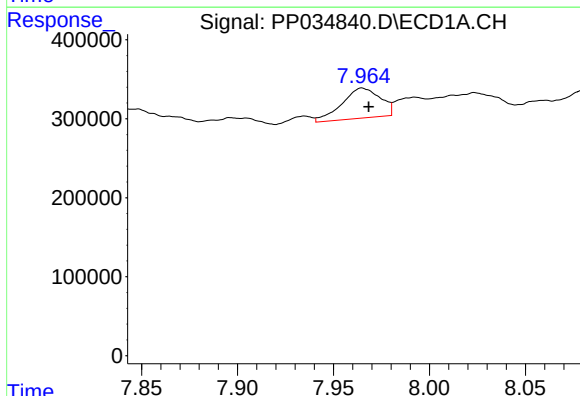


#29 AR-1254-4

R.T.: 7.964 min
Delta R.T.: -0.004 min
Response: 540221
Conc: 174.72 ng/ml m

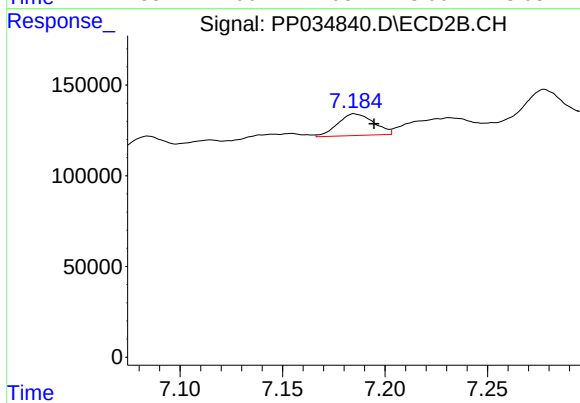

#29 AR-1254-4

R.T.: 7.184 min
Delta R.T.: -0.010 min
Response: 147430
Conc: 112.15 ng/ml m

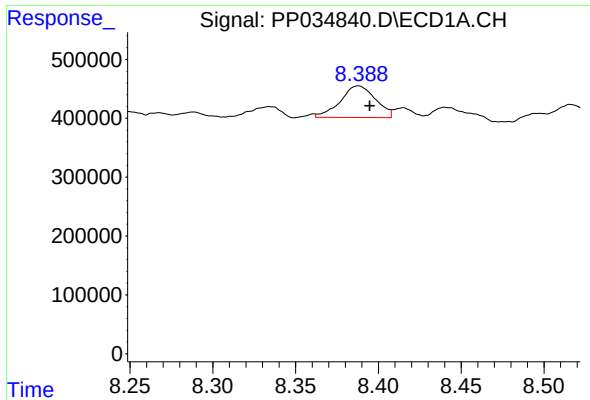


#30 AR-1254-5

R.T.: 8.388 min
Delta R.T.: -0.007 min
Response: 800462
Conc: 225.24 ng/ml m

Instrument :
ECD_P
ClientSampleId :
T-2

Manual Integrations
APPROVED

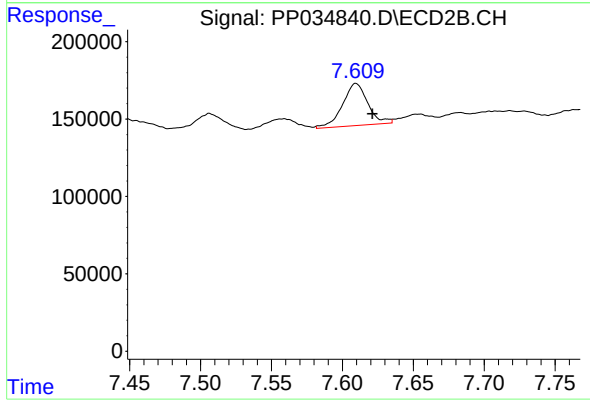

#30 AR-1254-5

R.T.: 7.609 min
Delta R.T.: -0.012 min
Response: 337829
Conc: 166.22 ng/ml m

Ankita

4/14/2021
1:49:29 PM