

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041321\
 Data File : PP034851.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2021 13:52
 Operator : DD\AJ
 Sample : M2012-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MS-PC

Manual Integrations
 APPROVED

Ankita
 4/14/2021 1:50:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 16:08:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.841	4.258	1896712	1185543	24.864	26.391
2) SA Decachlor...	10.753	9.551	1835214	749048	23.840	26.528

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041321\
Data File : PP034851.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2021 13:52
Operator : DD\AJ
Sample : M2012-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MS-PC


Manual Integrations
APPROVED

Ankita
4/14/2021 1:50:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 16:08:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

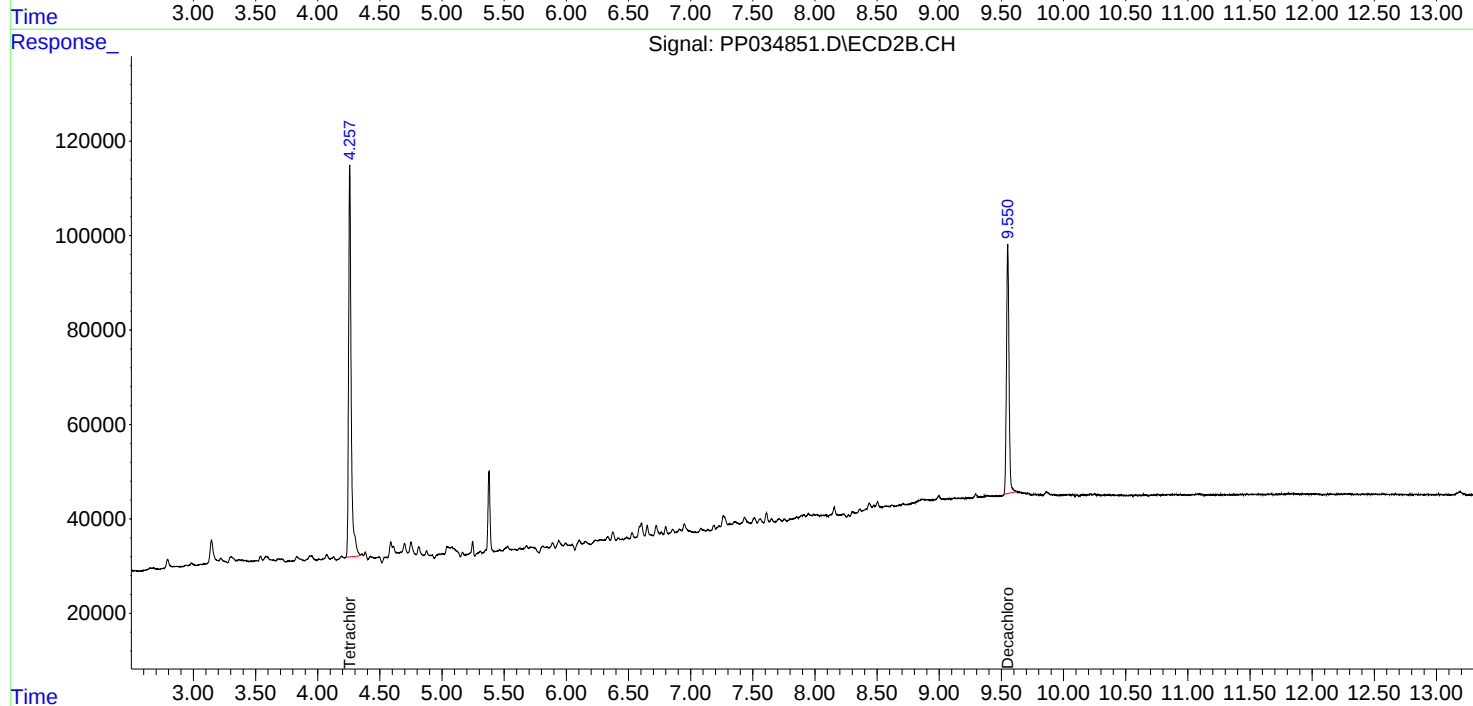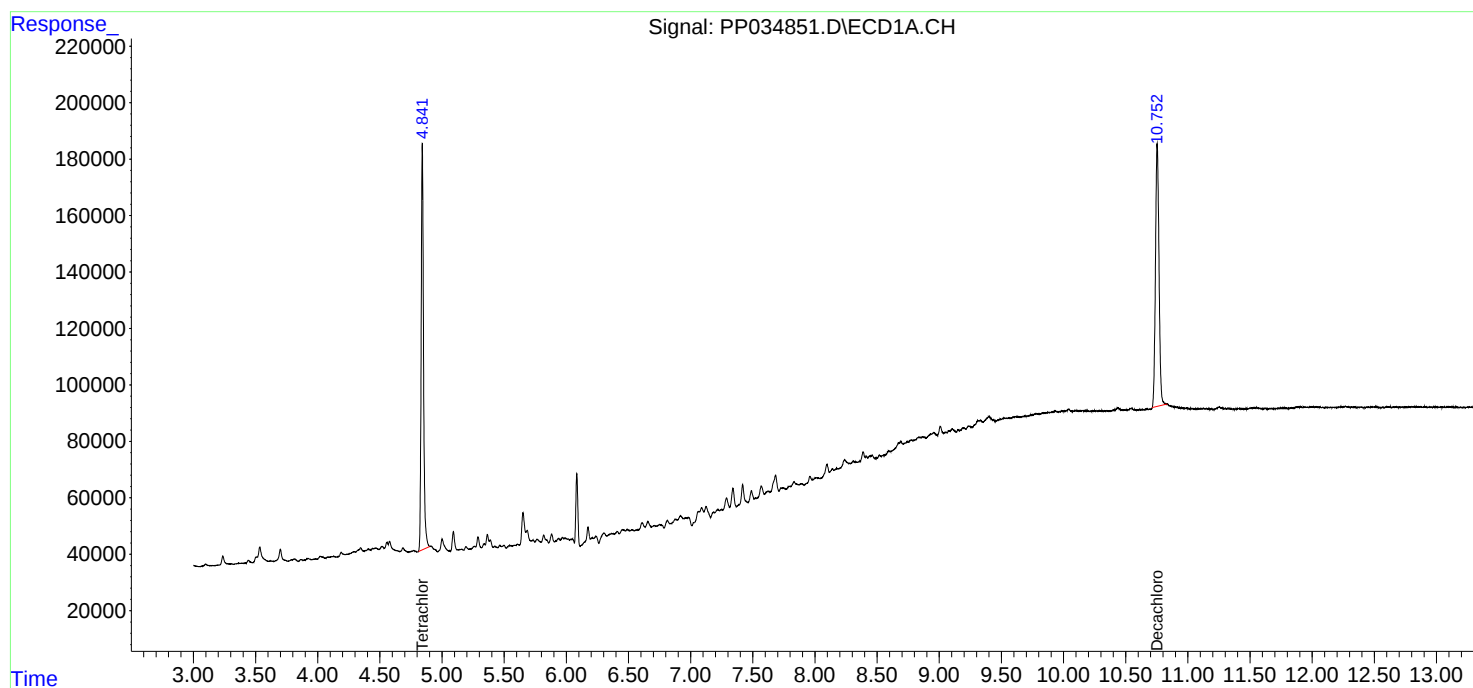

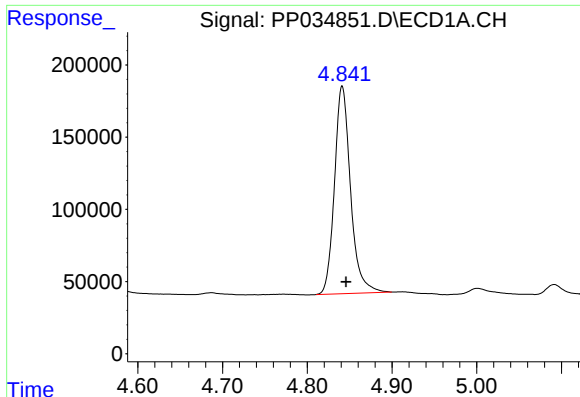


#1 Tetrachloro-m-xylene

R.T.: 4.841 min
Delta R.T.: -0.005 min
Response: 1896712
Conc: 24.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-PC


Manual Integrations
APPROVED

Ankita
4/14/2021 1:50:01 PM

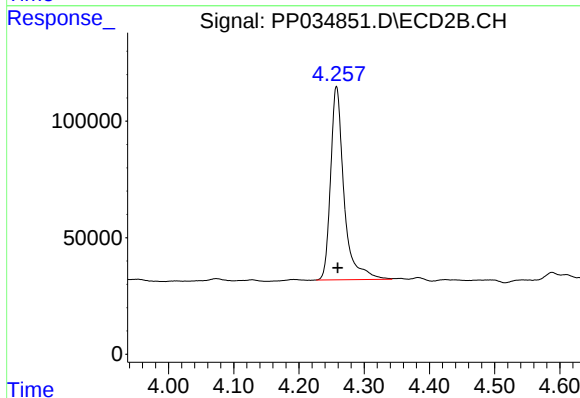


#1 Tetrachloro-m-xylene

R.T.: 4.258 min
Delta R.T.: -0.002 min
Response: 1185543
Conc: 26.39 ng/ml

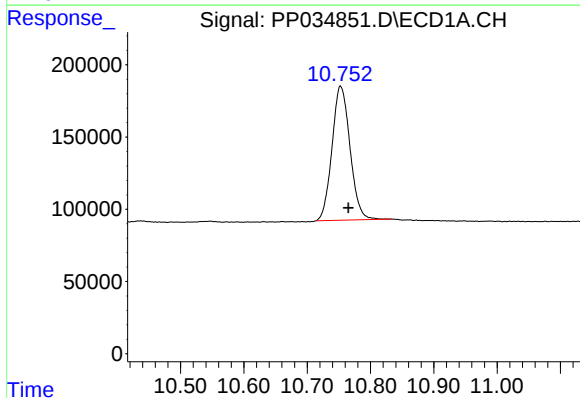

#2 Decachlorobiphenyl

R.T.: 10.753 min
Delta R.T.: -0.012 min
Response: 1835214
Conc: 23.84 ng/ml

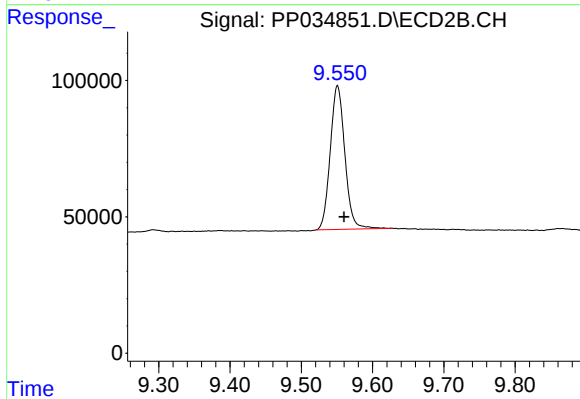

#2 Decachlorobiphenyl

R.T.: 9.551 min
Delta R.T.: -0.009 min
Response: 749048
Conc: 26.53 ng/ml