

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041323\
 Data File : PP056911.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 14:51
 Operator : YP\AJ
 Sample : 02293-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IDW-LIQ-FRAC-041123

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 17:40:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 04:14:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.436	3.662	47915923	33316250	22.302	19.156
2) SA Decachlor...	10.276	8.745	23614758	24616355	18.042	15.656

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041323\
Data File : PP056911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 14:51
Operator : YP\AJ
Sample : 02293-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
IDW-LIQ-FRAC-041123

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 17:40:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 04:14:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

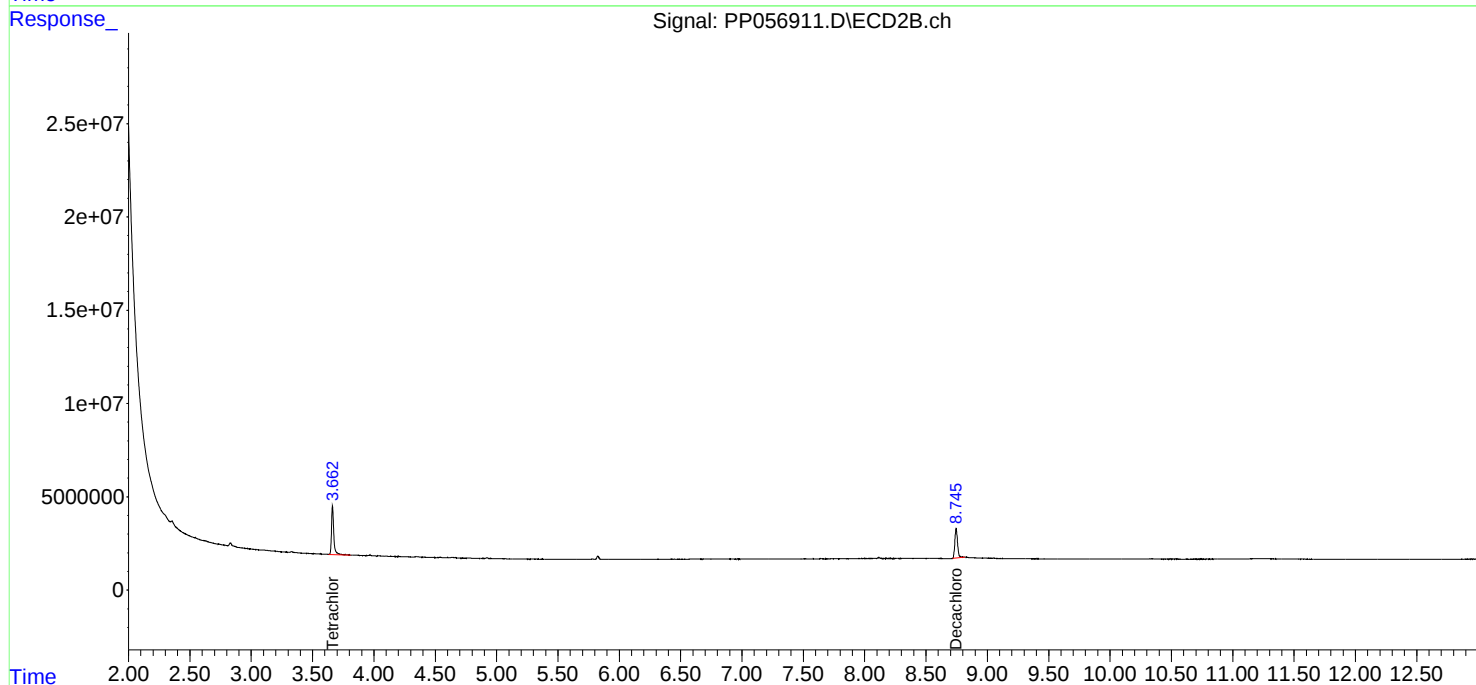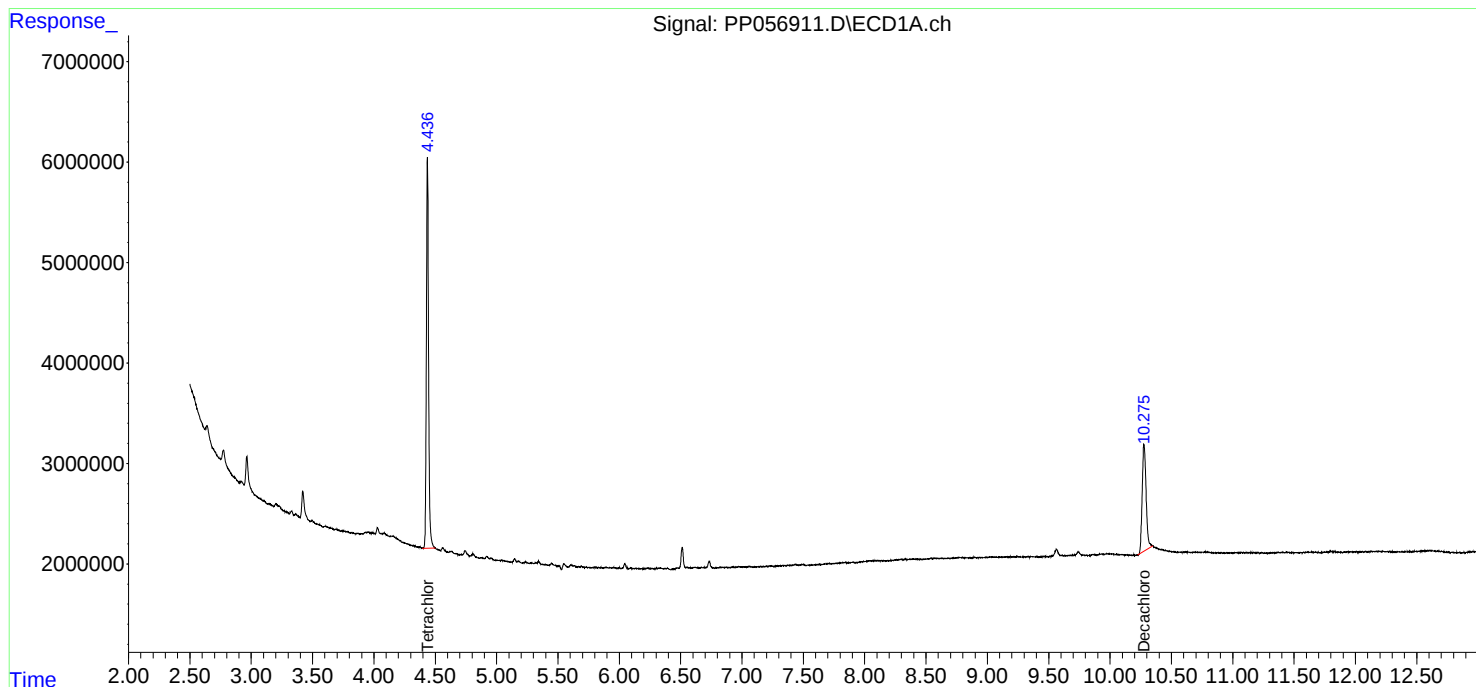


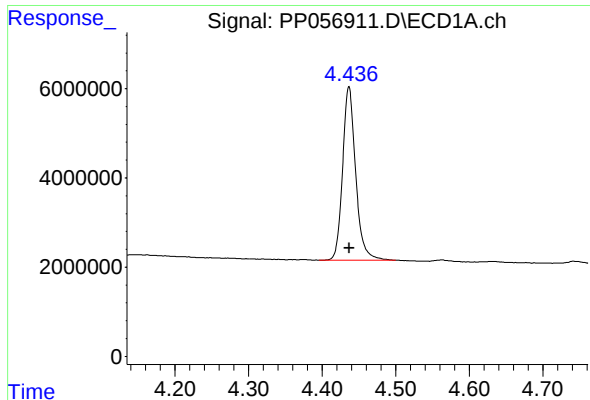

#1 Tetrachloro-m-xylene


R.T.: 4.436 min
Delta R.T.: 0.000 min
Response: 47915923
Conc: 22.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
IDW-LIQ-FRAC-041123

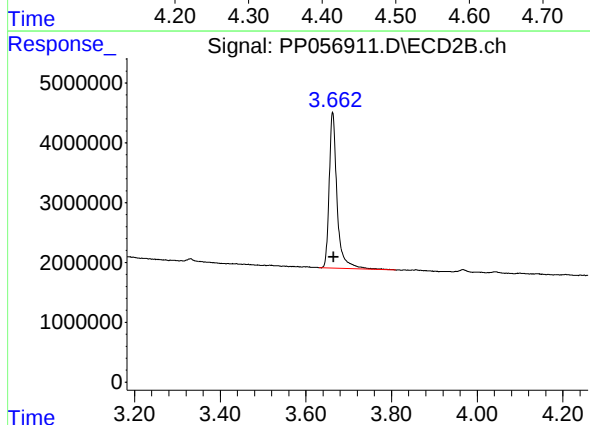


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.003 min
Response: 33316250
Conc: 19.16 ng/ml

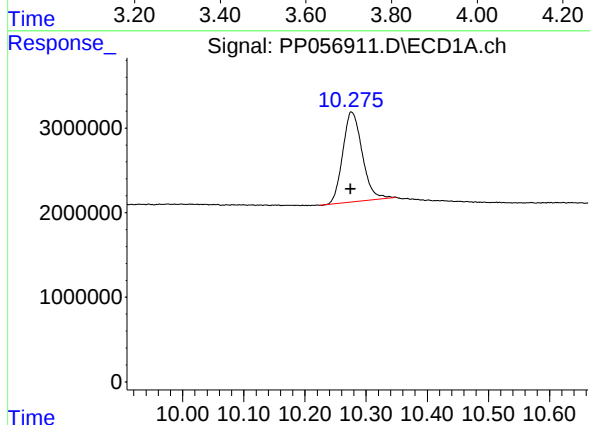

#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: 0.000 min
Response: 23614758
Conc: 18.04 ng/ml

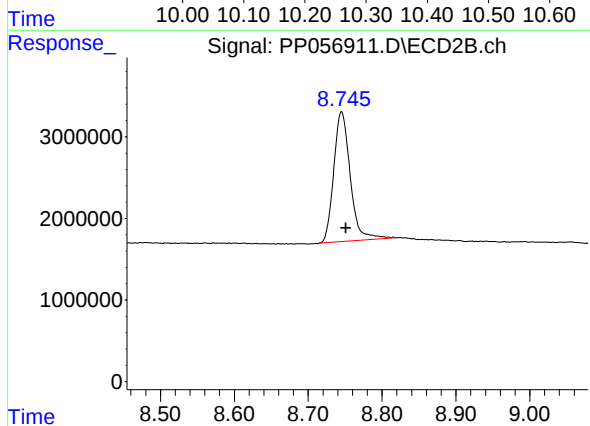

#2 Decachlorobiphenyl

R.T.: 8.745 min
Delta R.T.: -0.006 min
Response: 24616355
Conc: 15.66 ng/ml