

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041323\
 Data File : PP056913.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 16:20
 Operator : YP\AJ
 Sample : 02295-01RE 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEW-30994RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/14/2023
 Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 17:41:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 04:14:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.436	3.663	4904926	3552379	2.283m	2.043
2) SA Decachlor...	10.280	8.739	606876	8222986	0.464m	5.230m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041323\
Data File : PP056913.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 16:20
Operator : YP\AJ
Sample : 02295-01RE 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SEW-30994RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 17:41:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 04:14:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

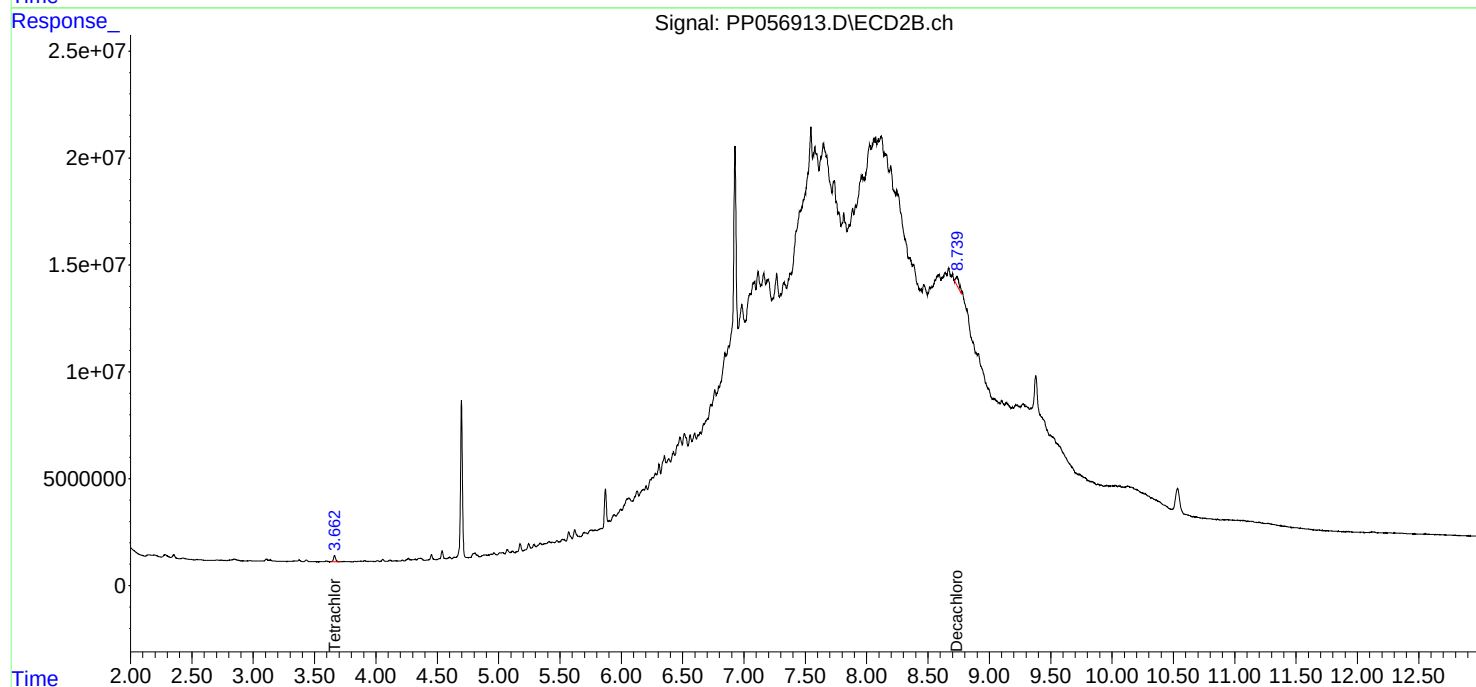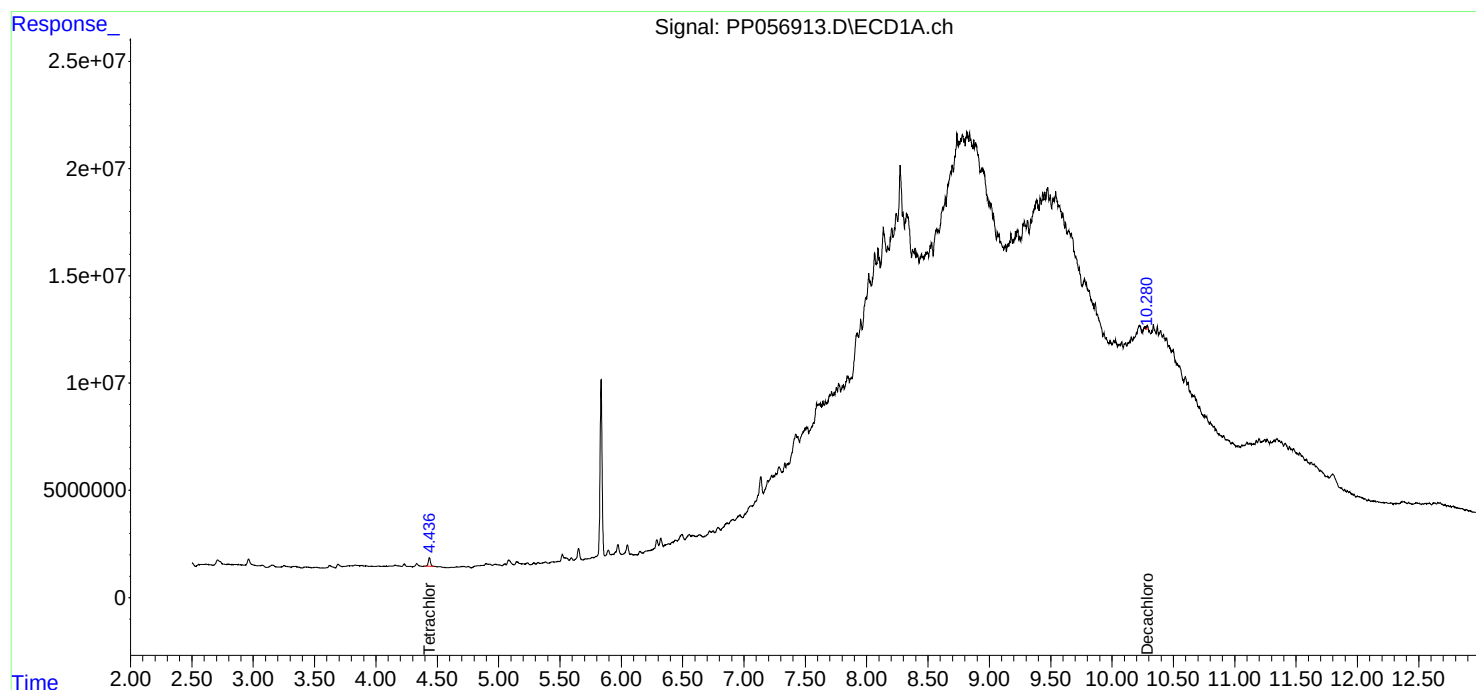

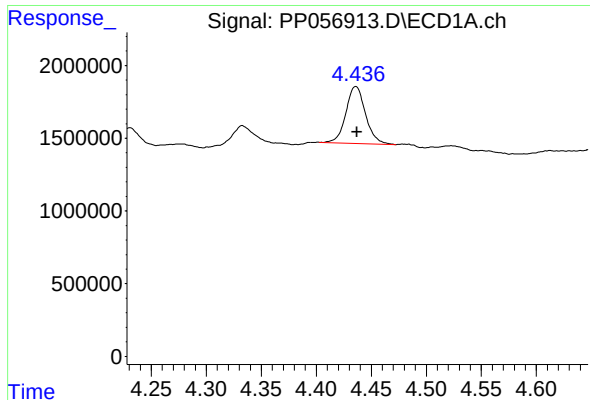


#1 Tetrachloro-m-xylene

R.T.: 4.436 min
Delta R.T.: -0.001 min
Response: 4904926
Conc: 2.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEW-30994RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

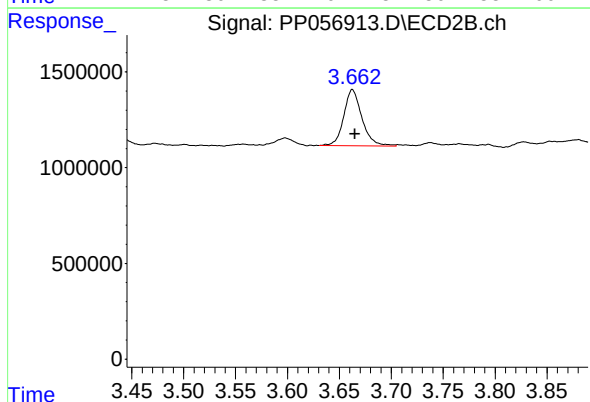


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.002 min
Response: 3552379
Conc: 2.04 ng/ml

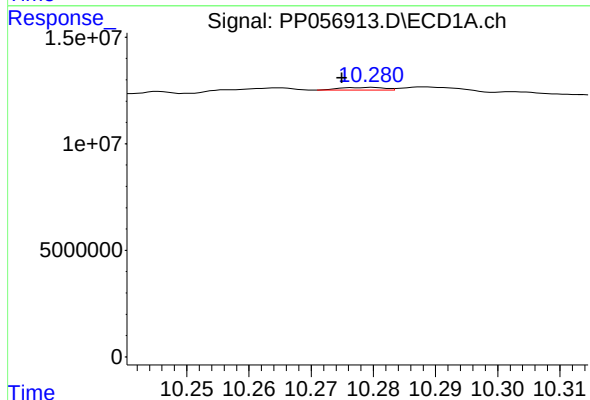

#2 Decachlorobiphenyl

R.T.: 10.280 min
Delta R.T.: 0.005 min
Response: 606876
Conc: 0.46 ng/ml m

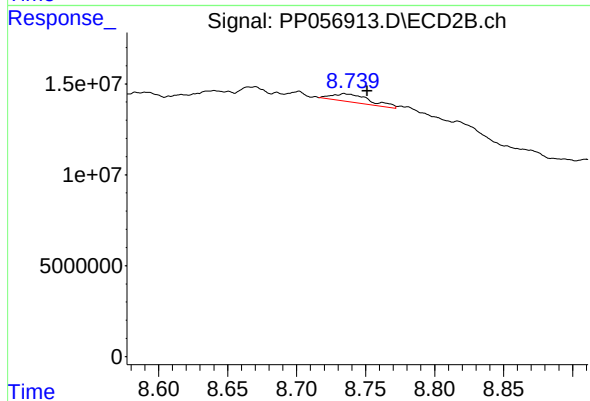

#2 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: -0.013 min
Response: 8222986
Conc: 5.23 ng/ml m