

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041421\
 Data File : PP034864.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Apr 2021 10:25
 Operator : DD\AJ
 Sample : M2016-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 UNLABELED-24OZ-JAR

Manual Integrations
 APPROVED

Ankita
 4/15/2021 2:06:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 11:11:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.843	4.260	1198291	770736	15.708	17.157
2) SA Decachlor...	10.755	9.554	1137222	455417	14.773m	16.129

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041421\
Data File : PP034864.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Apr 2021 10:25
Operator : DD\AJ
Sample : M2016-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
UNLABELED-24OZ-JAR


Manual Integrations
APPROVED

Ankita
4/15/2021 2:06:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 11:11:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

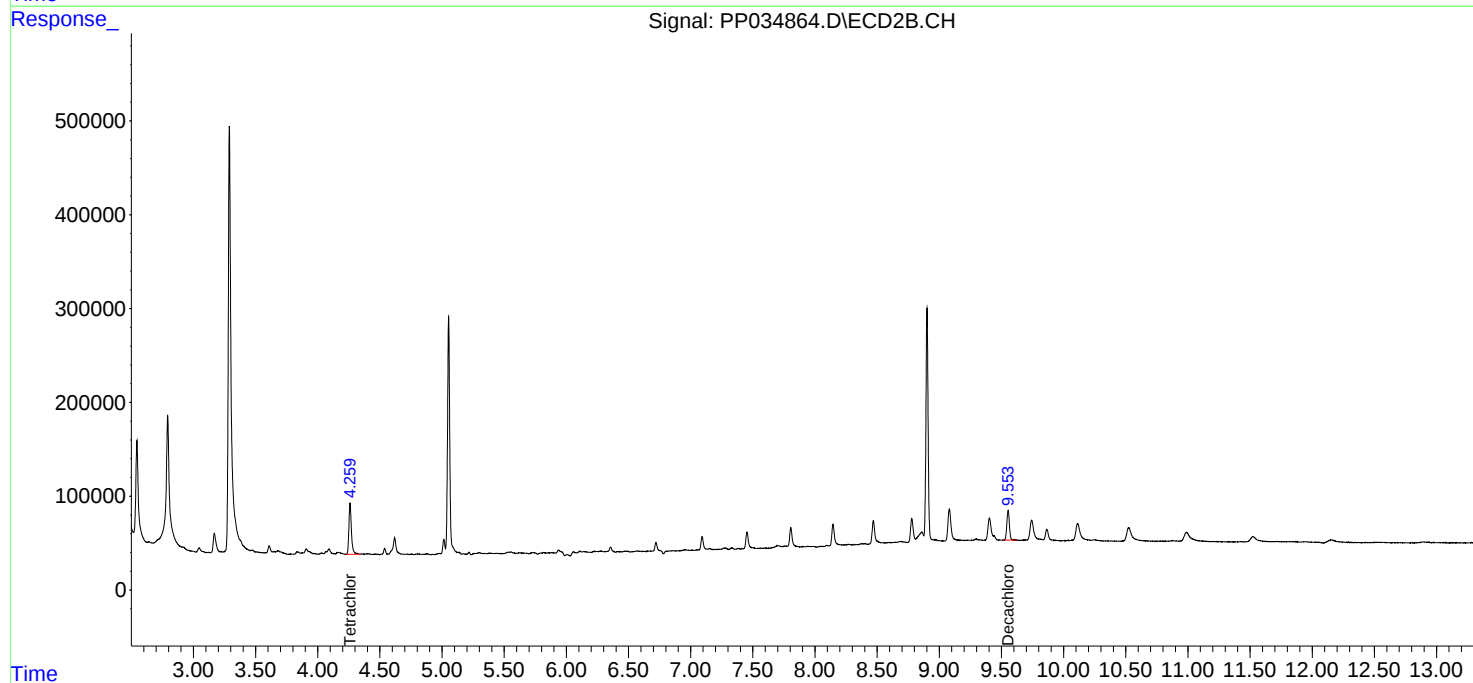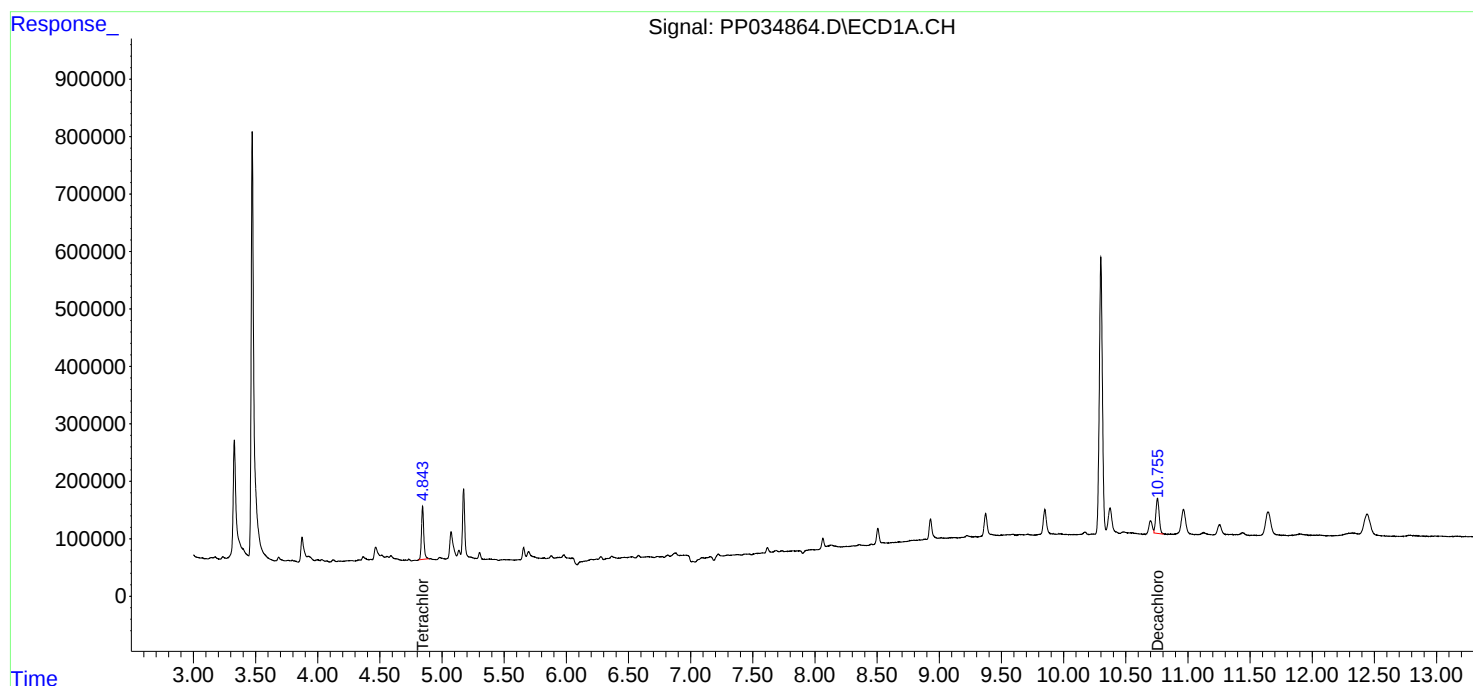

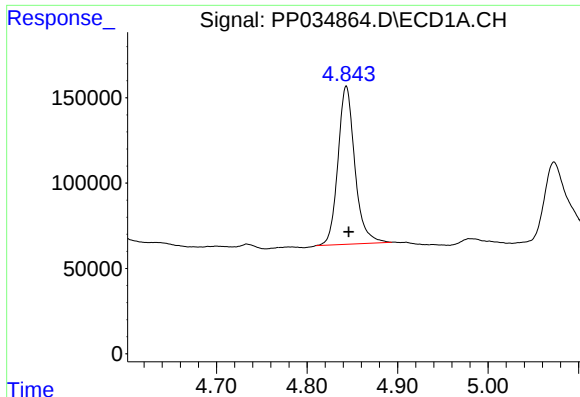


#1 Tetrachloro-m-xylene

R.T.: 4.843 min
Delta R.T.: -0.003 min
Response: 1198291
Conc: 15.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
UNLABELED-24OZ-JAR


Manual Integrations
APPROVED

Ankita
4/15/2021 2:06:47 PM

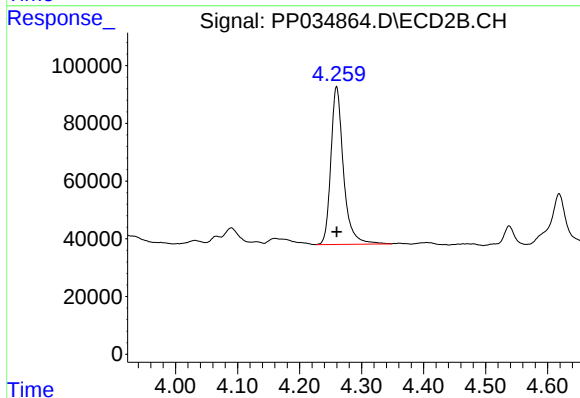


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: 0.000 min
Response: 770736
Conc: 17.16 ng/ml

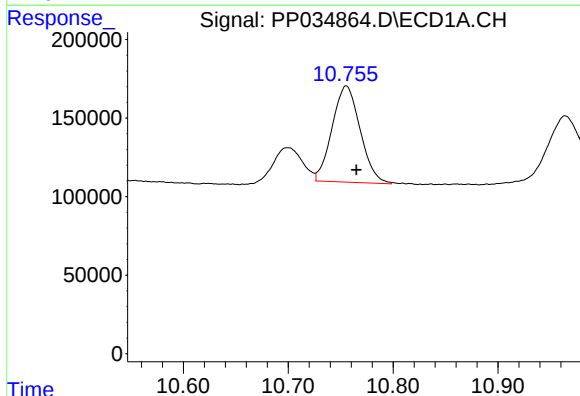

#2 Decachlorobiphenyl

R.T.: 10.755 min
Delta R.T.: -0.010 min
Response: 1137222
Conc: 14.77 ng/ml m

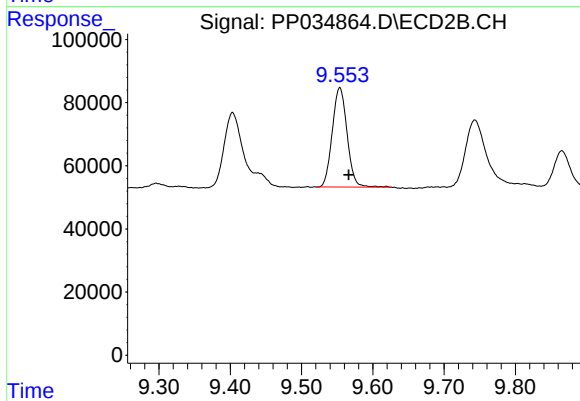

#2 Decachlorobiphenyl

R.T.: 9.554 min
Delta R.T.: -0.012 min
Response: 455417
Conc: 16.13 ng/ml