

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041423\
 Data File : PP056922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 14:33
 Operator : YP\AJ
 Sample : PB152126BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB152126BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/17/2023
 Supervised By :Ankita Jodhani 04/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 18:32:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 04:14:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.433	3.659	46888921	32342781	21.824	18.596
2) SA Decachlor...	10.276	8.741	31843060	33099888	24.328	21.052m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041423\
Data File : PP056922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 14:33
Operator : YP\AJ
Sample : PB152126BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB152126BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/17/2023
Supervised By :Ankita Jodhani 04/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 18:32:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040623.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 04:14:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

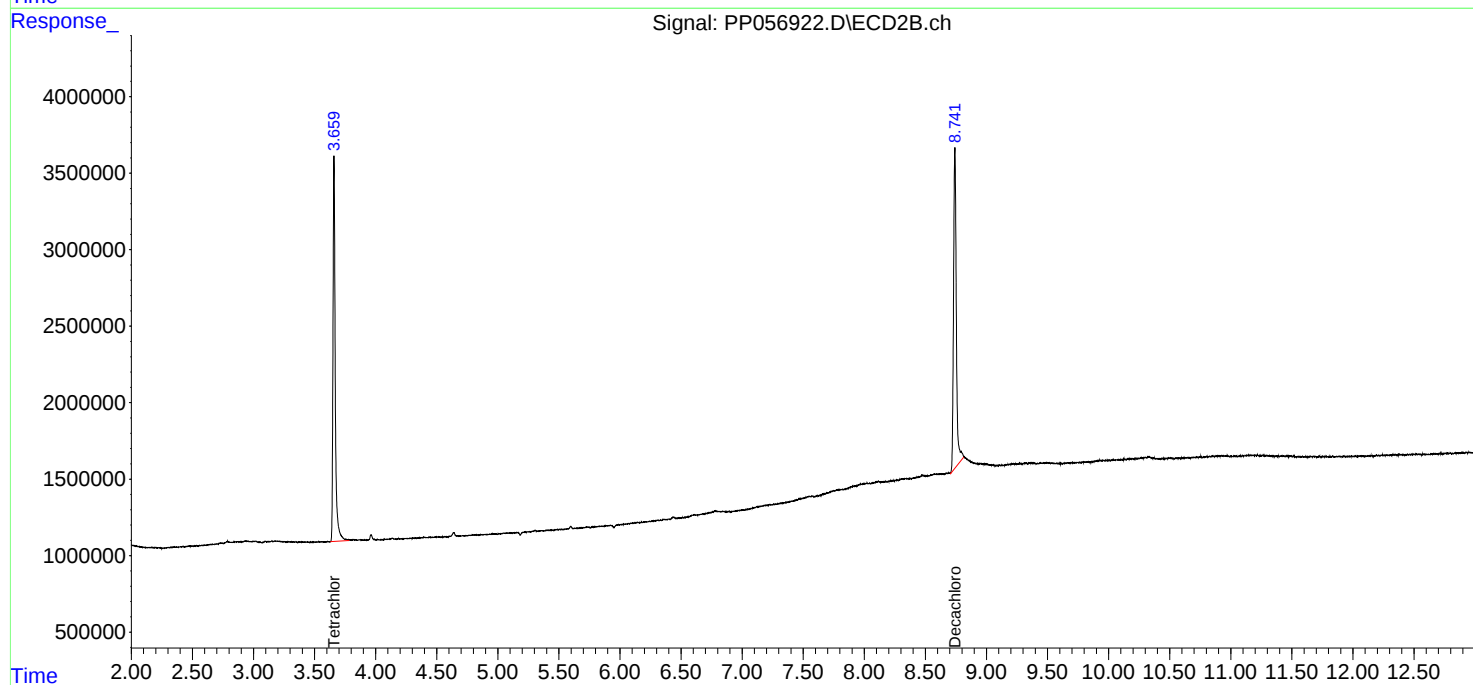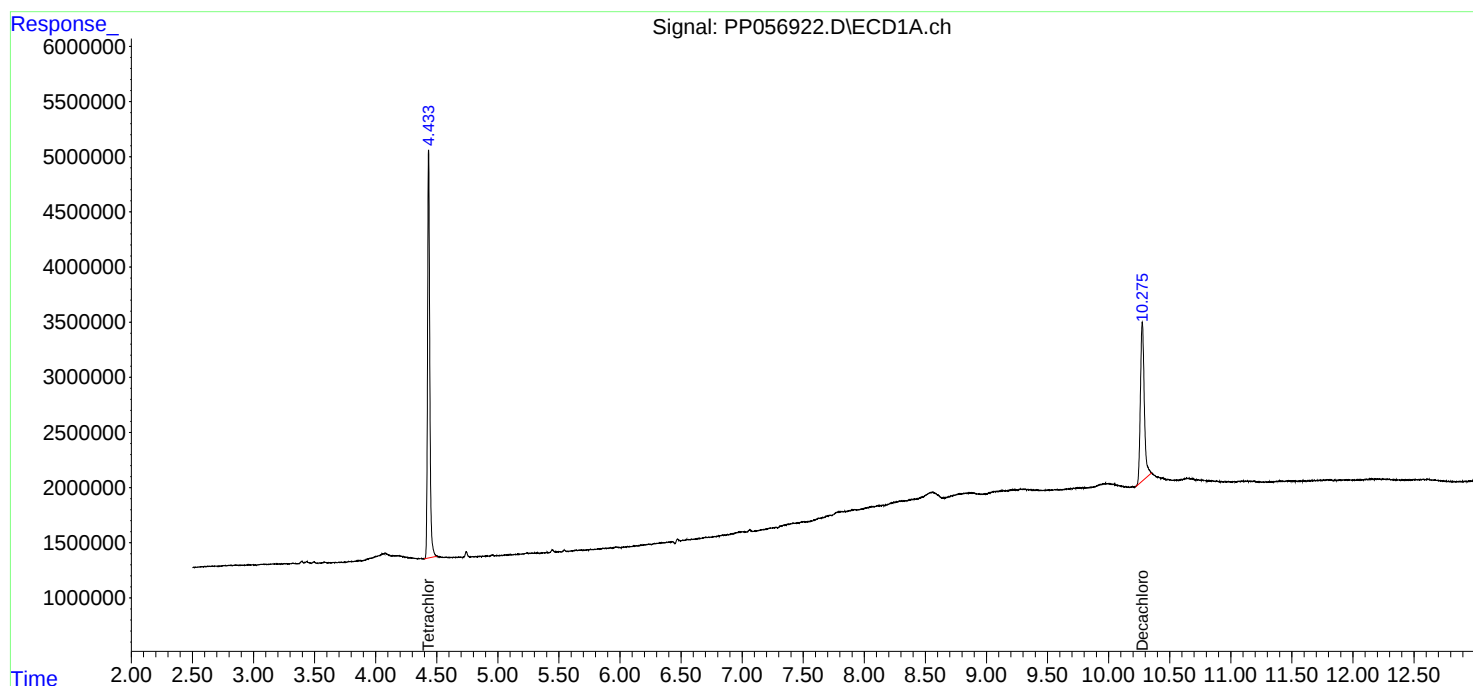

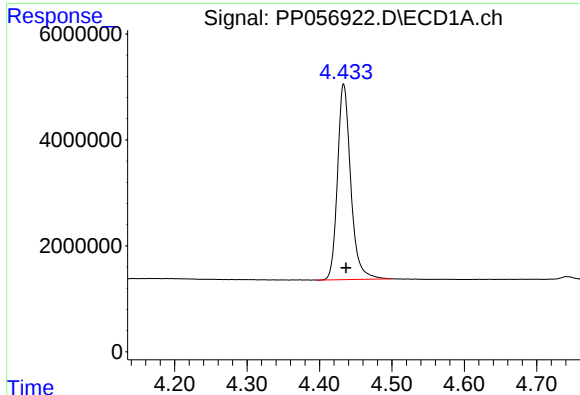

#1 Tetrachloro-m-xylene

R.T.: 4.433 min
Delta R.T.: -0.004 min
Response: 46888921
Conc: 21.82 ng/ml

Instrument :

ECD_P


ClientSampleId :

PB152126BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 04/17/2023
Supervised By :Ankita Jodhani 04/17/2023

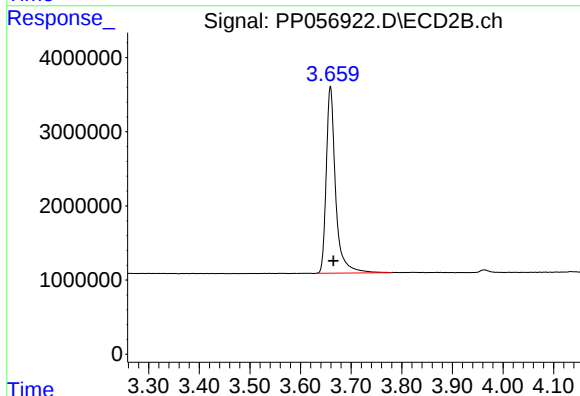


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.006 min
Response: 32342781
Conc: 18.60 ng/ml

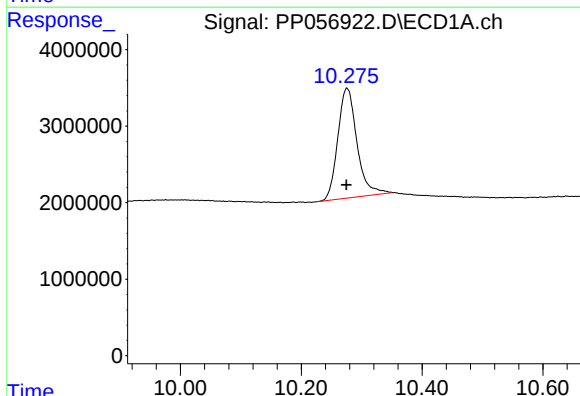

#2 Decachlorobiphenyl

R.T.: 10.276 min
Delta R.T.: 0.000 min
Response: 31843060
Conc: 24.33 ng/ml

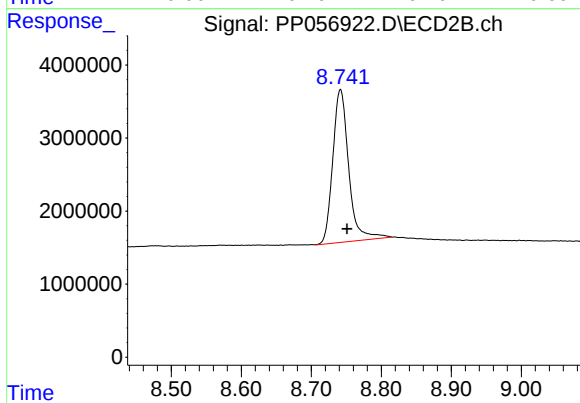

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.010 min
Response: 33099888
Conc: 21.05 ng/ml m