

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041521\
 Data File : PP034906.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2021 13:26
 Operator : DD\AJ
 Sample : M2036-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RT-80-W-ROCKAWAY-A-2

Manual Integrations
 APPROVED

Ankita
 4/16/2021 3:23:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 16:29:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.843	4.258	1815028	1223885	23.793	27.244
2) SA Decachlor...	10.760	9.554	1794094	690547	23.306	24.456

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041521\
Data File : PP034906.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2021 13:26
Operator : DD\AJ
Sample : M2036-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RT-80-W-ROCKAWAY-A-2


Manual Integrations
APPROVED

Ankita
4/16/2021 3:23:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 16:29:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

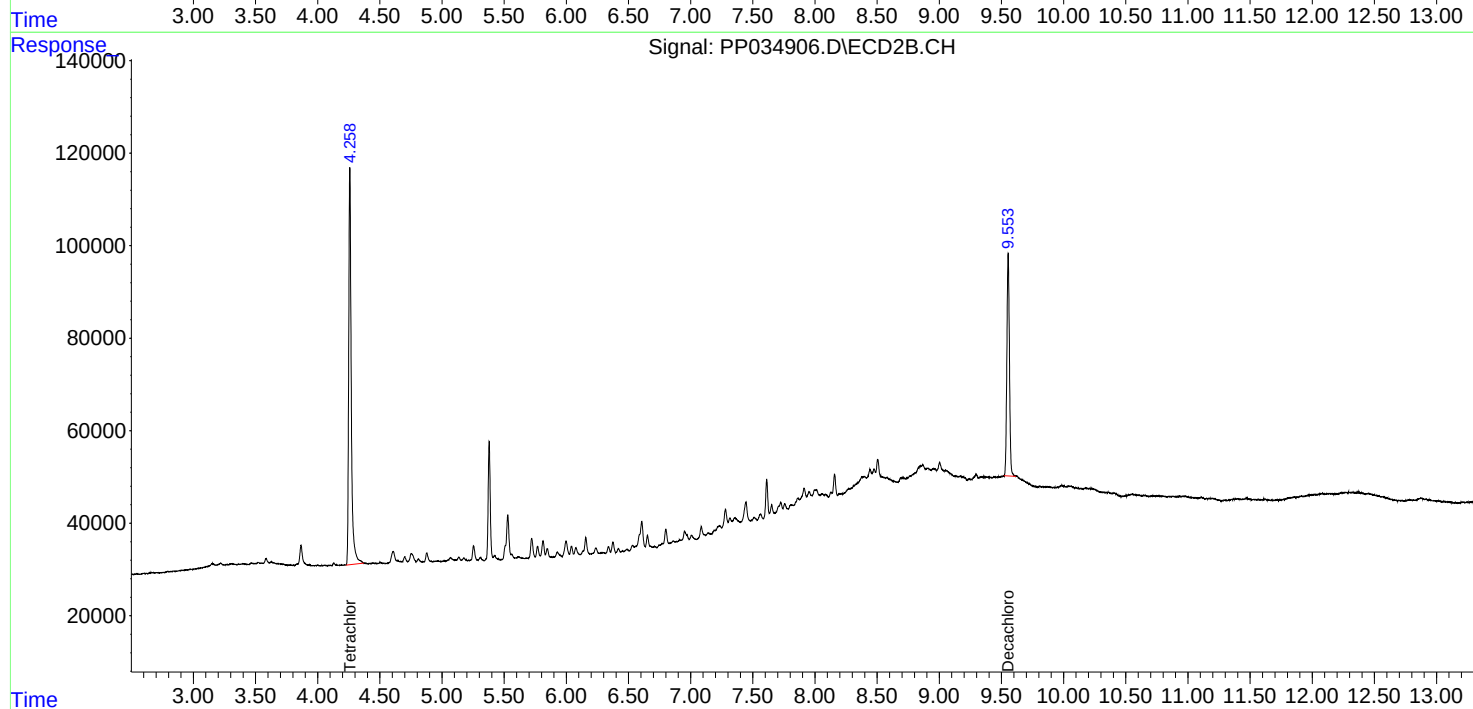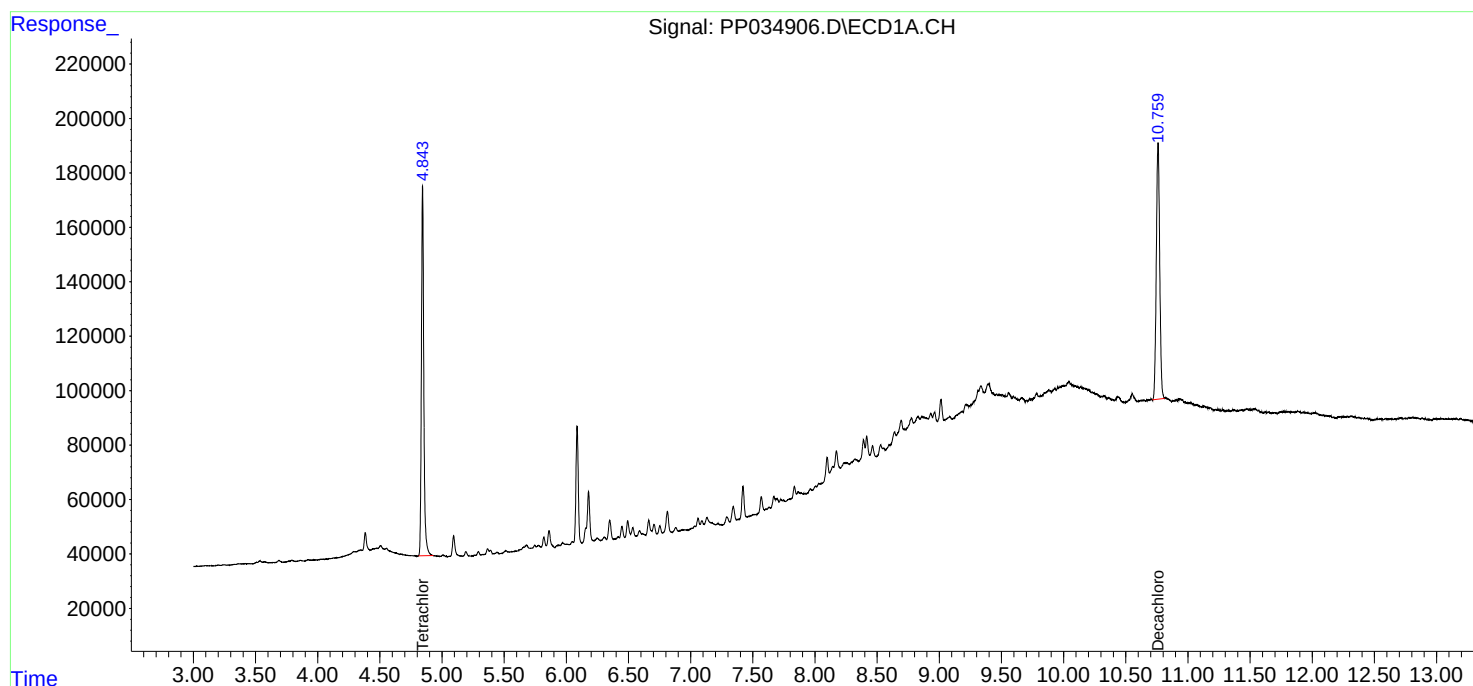

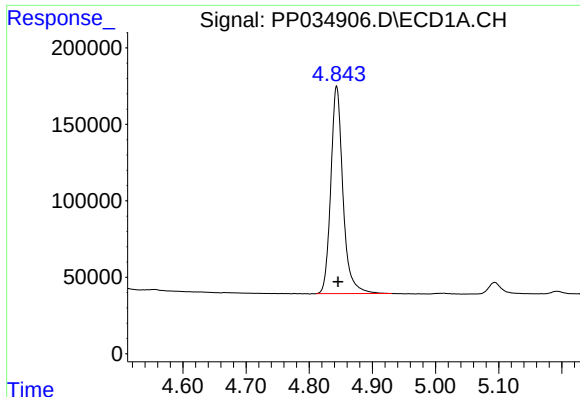


#1 Tetrachloro-m-xylene

R.T.: 4.843 min
Delta R.T.: -0.003 min
Response: 1815028
Conc: 23.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
RT-80-W-ROCKAWAY-A-2


Manual Integrations
APPROVED

Ankita
4/16/2021 3:23:17 PM

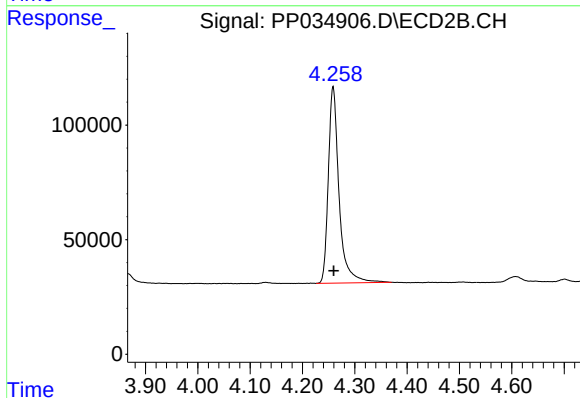


#1 Tetrachloro-m-xylene

R.T.: 4.258 min
Delta R.T.: -0.001 min
Response: 1223885
Conc: 27.24 ng/ml

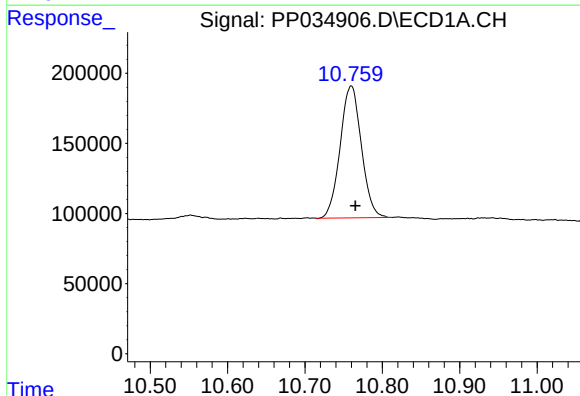

#2 Decachlorobiphenyl

R.T.: 10.760 min
Delta R.T.: -0.005 min
Response: 1794094
Conc: 23.31 ng/ml

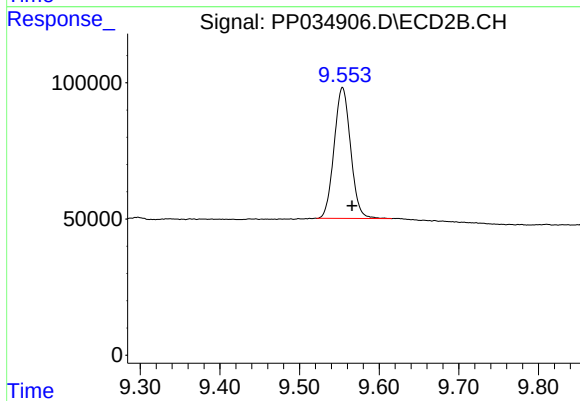

#2 Decachlorobiphenyl

R.T.: 9.554 min
Delta R.T.: -0.012 min
Response: 690547
Conc: 24.46 ng/ml