

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
 Data File : PP046036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2022 12:49
 Operator : YP\AJ
 Sample : N2380-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-02-041222

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/15/2022
 Supervised By :mohammad ahmed 04/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 17:06:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 12 05:31:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.874	3.137	34635835	36620323	14.081m	23.047 #
2) SA Decachlor...	9.972	8.472	33740908	29313223	20.554	20.566

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
Data File : PP046036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2022 12:49
Operator : YP\AJ
Sample : N2380-01
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
OK-02-041222


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
Supervised By :mohammad ahmed 04/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 17:06:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 12 05:31:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

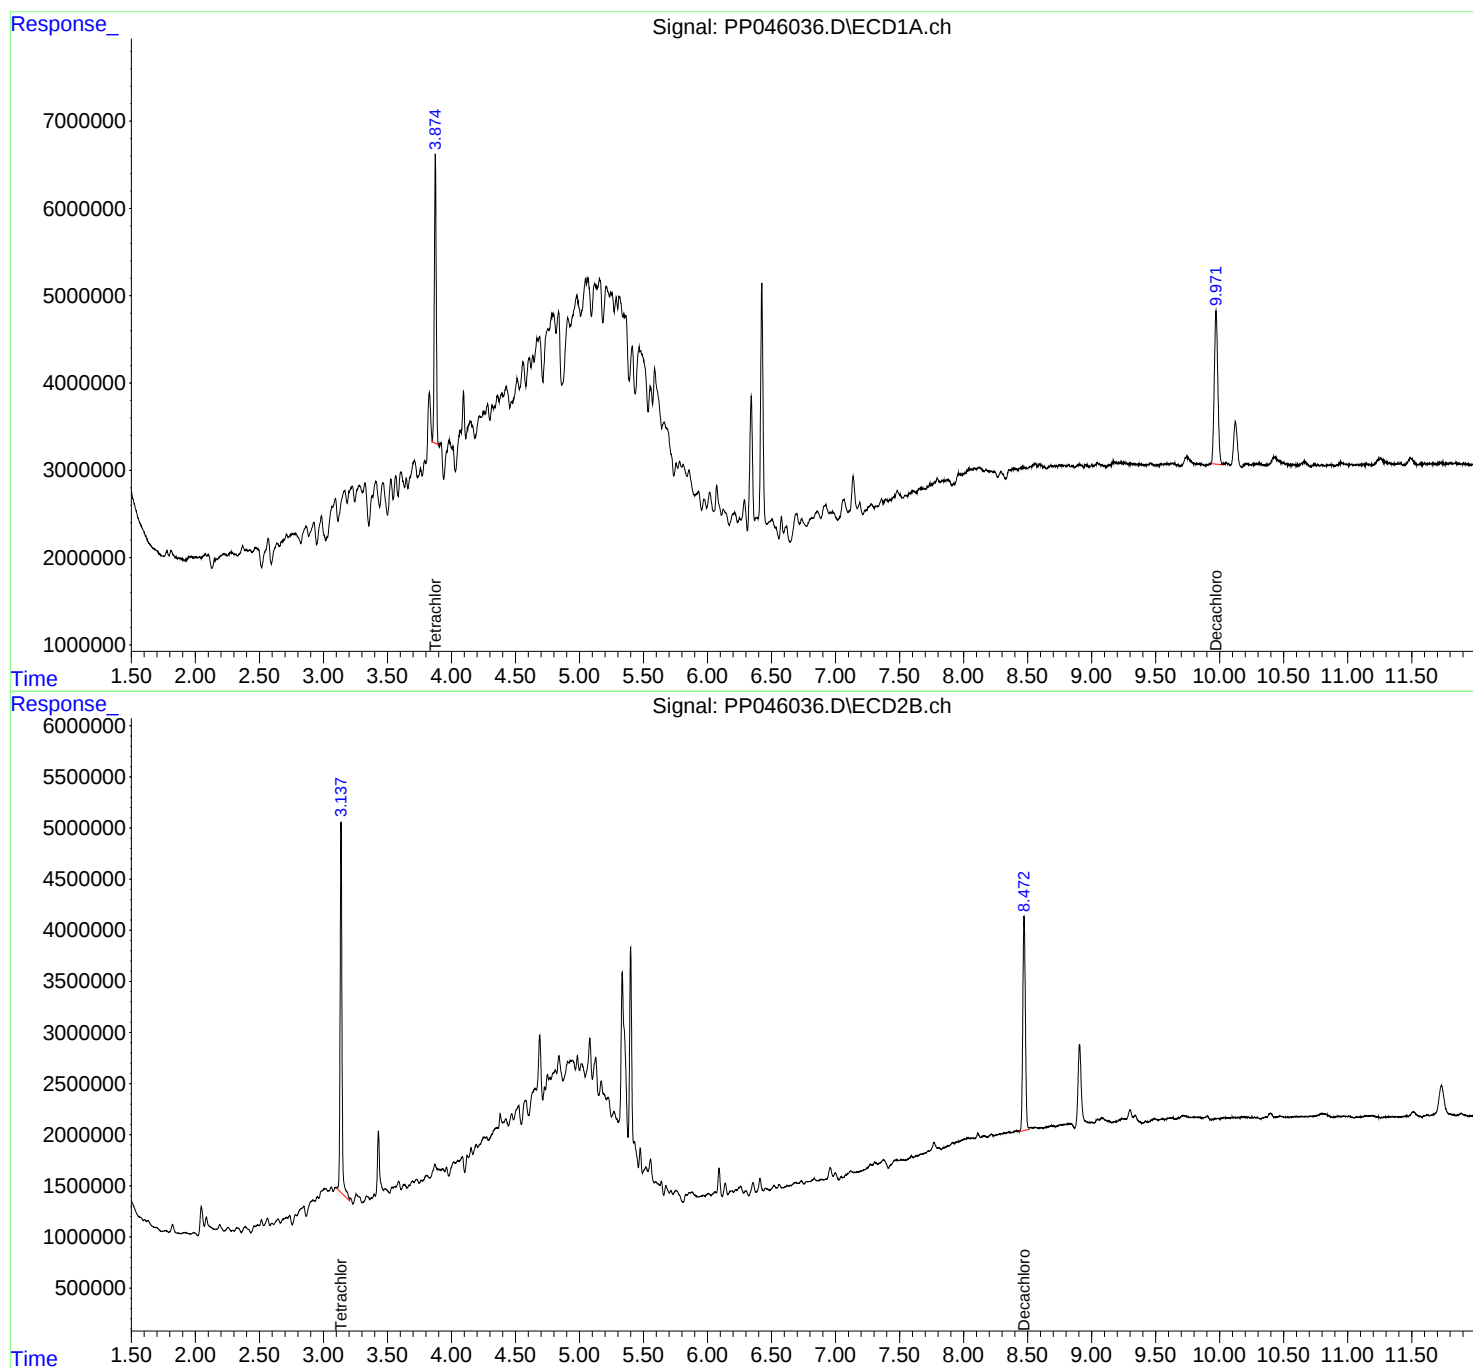

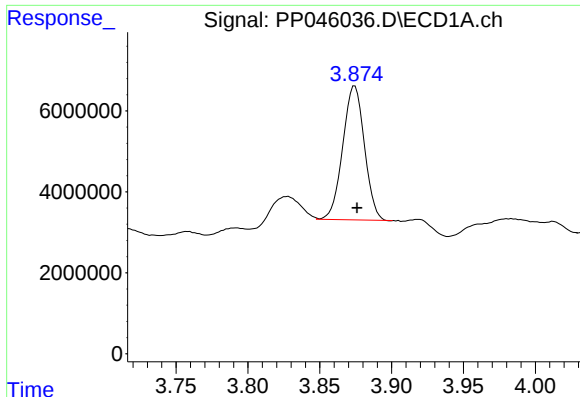


#1 Tetrachloro-m-xylene

R.T.: 3.874 min
Delta R.T.: -0.002 min
Response: 34635835
Conc: 14.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-02-041222


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
Supervised By :mohammad ahmed 04/15/2022

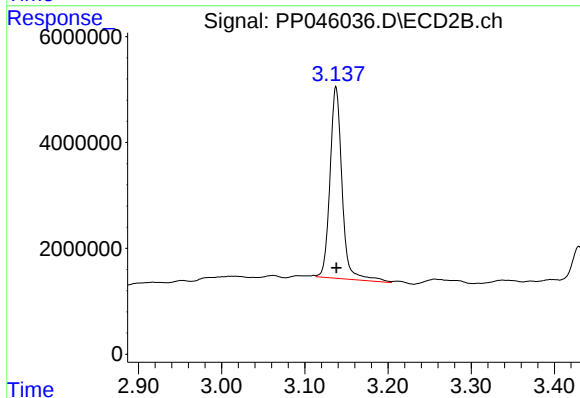


#1 Tetrachloro-m-xylene

R.T.: 3.137 min
Delta R.T.: 0.000 min
Response: 36620323
Conc: 23.05 ng/ml

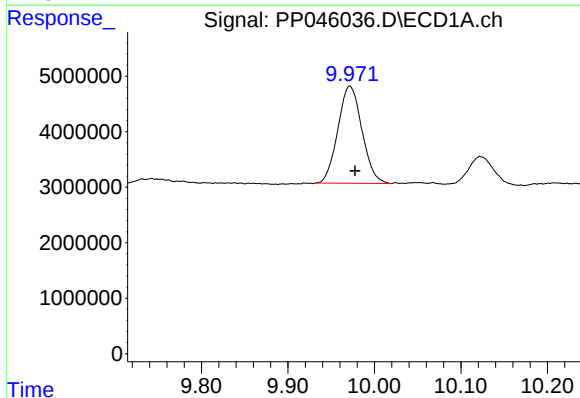

#2 Decachlorobiphenyl

R.T.: 9.972 min
Delta R.T.: -0.006 min
Response: 33740908
Conc: 20.55 ng/ml

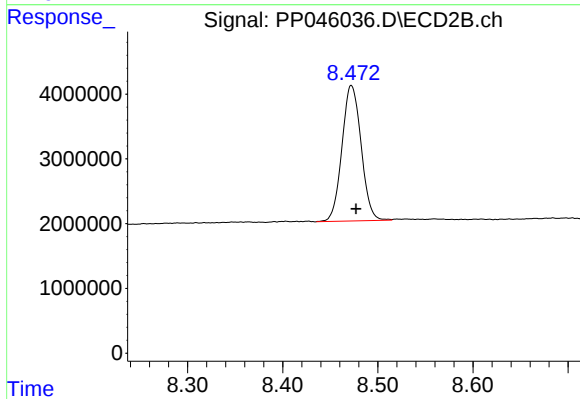

#2 Decachlorobiphenyl

R.T.: 8.472 min
Delta R.T.: -0.005 min
Response: 29313223
Conc: 20.57 ng/ml