

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
 Data File : PP046087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 04:02
 Operator : YP\AJ
 Sample : N2389-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20564

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/15/2022
 Supervised By :mohammad ahmed 04/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 05:51:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 12 05:31:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.874	3.138	30257382	20883700	12.301m	13.143m
2) SA Decachlor...	9.970	8.472	22739326	22559641	13.852	15.828

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
Data File : PP046087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 04:02
Operator : YP\AJ
Sample : N2389-01
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
20564


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
Supervised By :mohammad ahmed 04/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 05:51:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 12 05:31:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

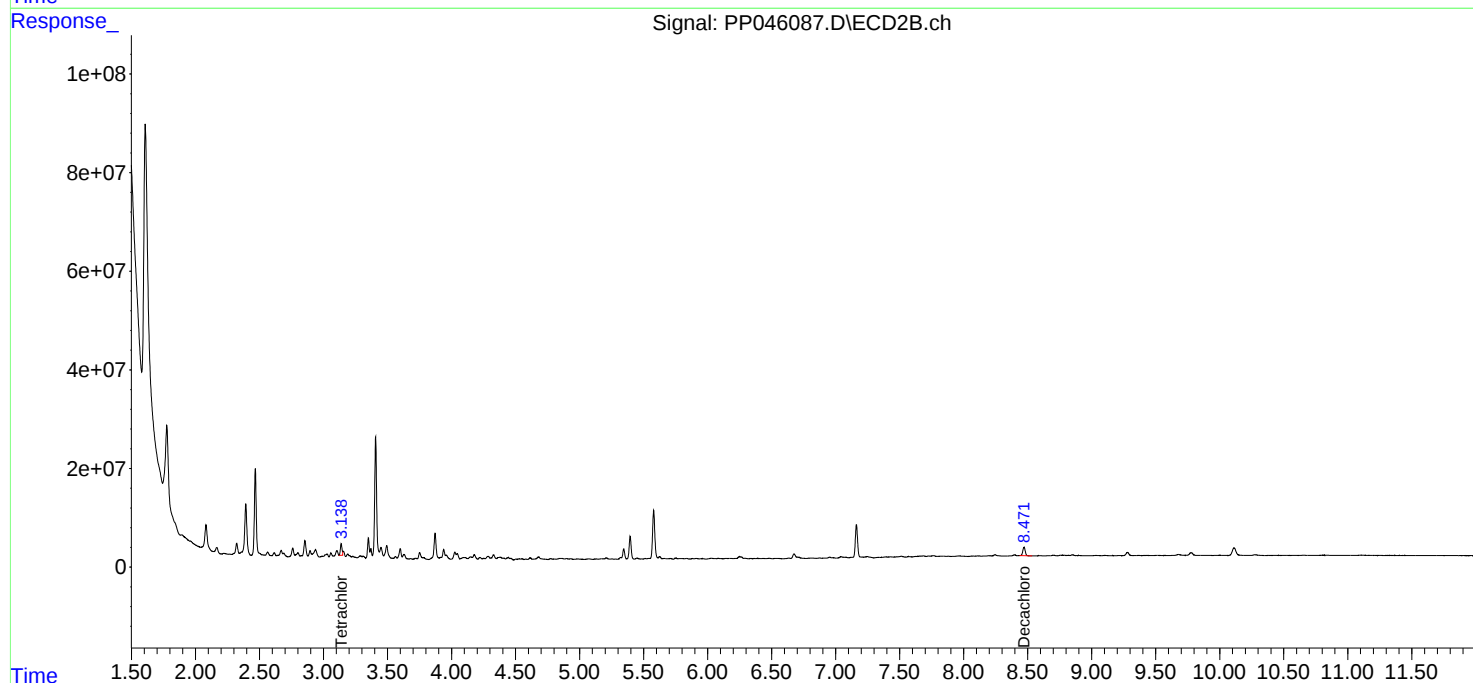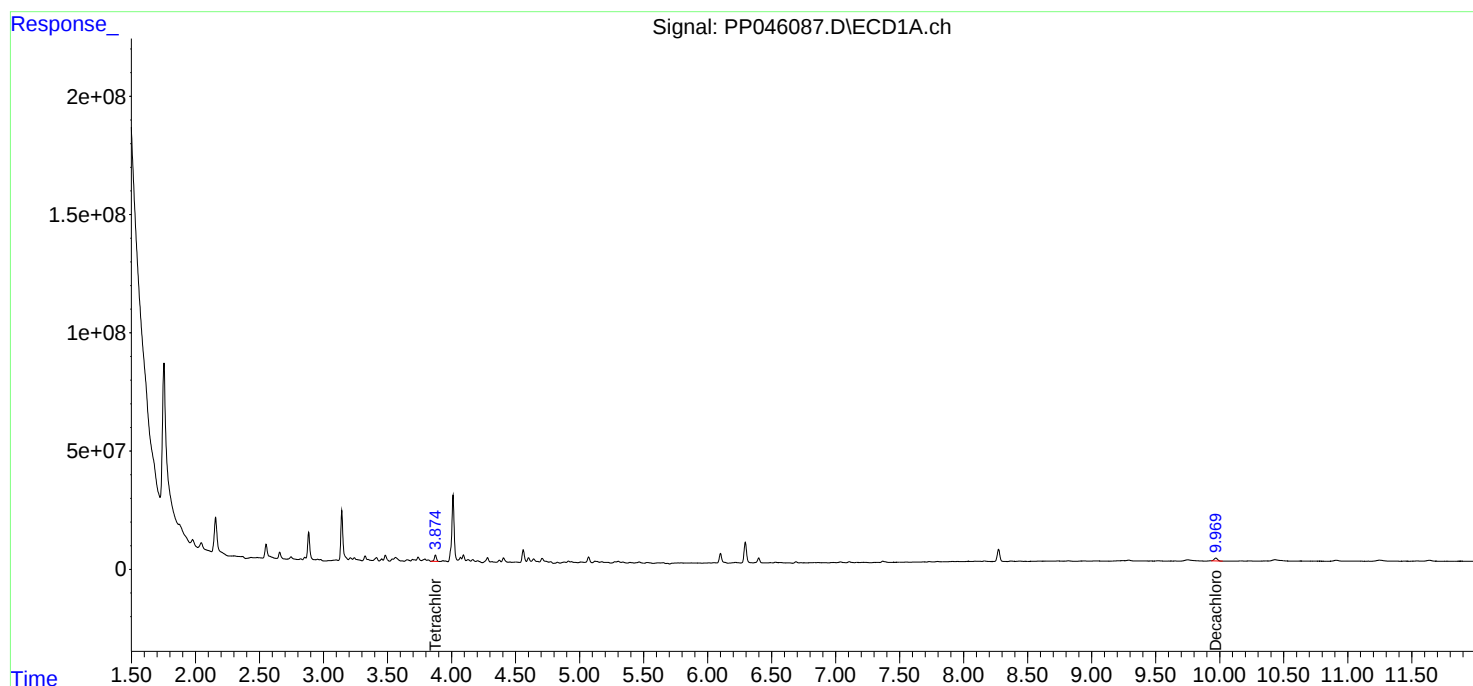

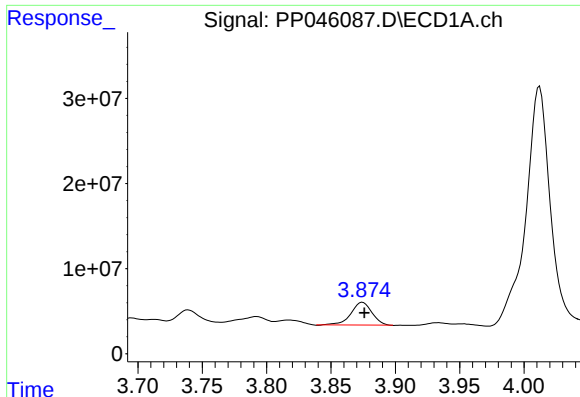


#1 Tetrachloro-m-xylene

R.T.: 3.874 min
Delta R.T.: -0.002 min
Response: 30257382
Conc: 12.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
20564


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
Supervised By :mohammad ahmed 04/15/2022

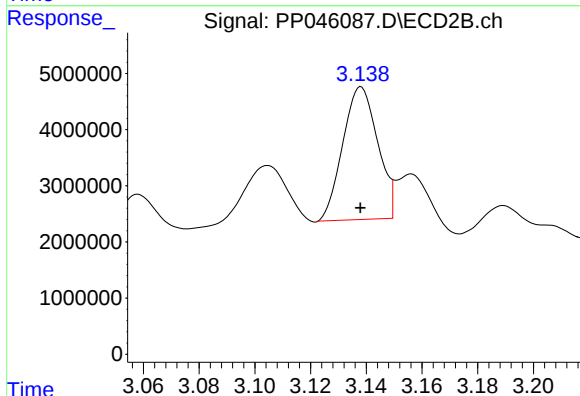


#1 Tetrachloro-m-xylene

R.T.: 3.138 min
Delta R.T.: 0.000 min
Response: 20883700
Conc: 13.14 ng/ml m

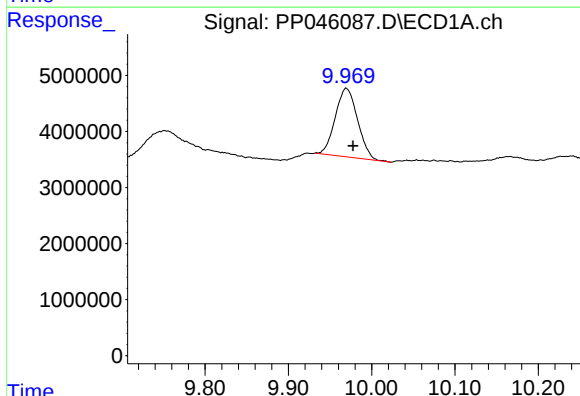

#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.008 min
Response: 22739326
Conc: 13.85 ng/ml

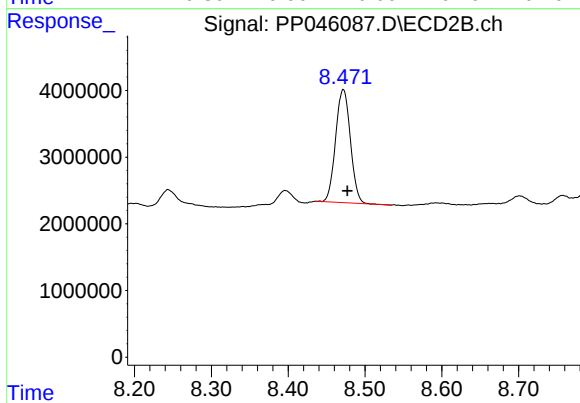

#2 Decachlorobiphenyl

R.T.: 8.472 min
Delta R.T.: -0.005 min
Response: 22559641
Conc: 15.83 ng/ml