

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
 Data File : PP046097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 07:21
 Operator : YP\AJ
 Sample : N2396-02
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 5576

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/15/2022
 Supervised By :mohammad ahmed 04/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 08:41:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 12 05:31:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.877	3.140	22844045	22116052	9.287m	13.918 #
2) SA Decachlor...	9.988	8.487	13603855	11688370	8.287	8.201

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
Data File : PP046097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 07:21
Operator : YP\AJ
Sample : N2396-02
Misc :
ALS Vial : 64 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
5576


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
Supervised By :mohammad ahmed 04/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 08:41:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 12 05:31:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

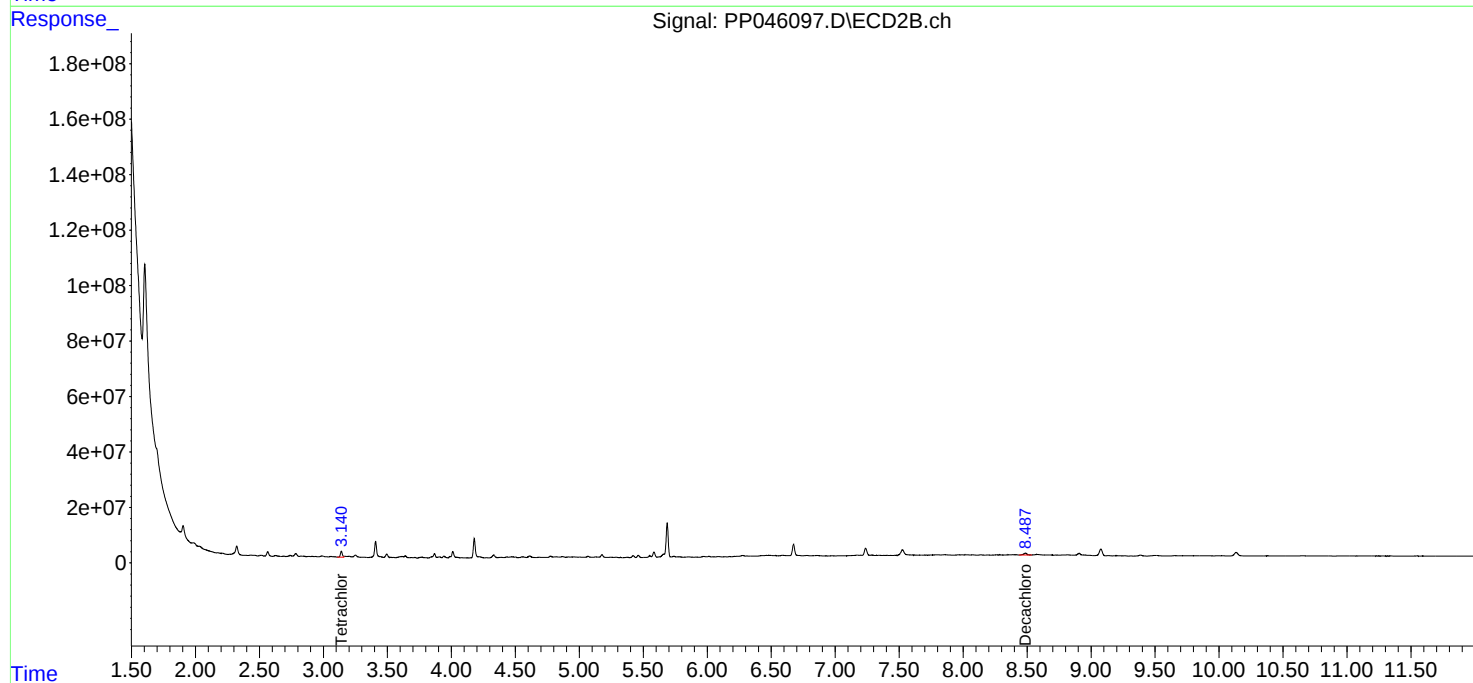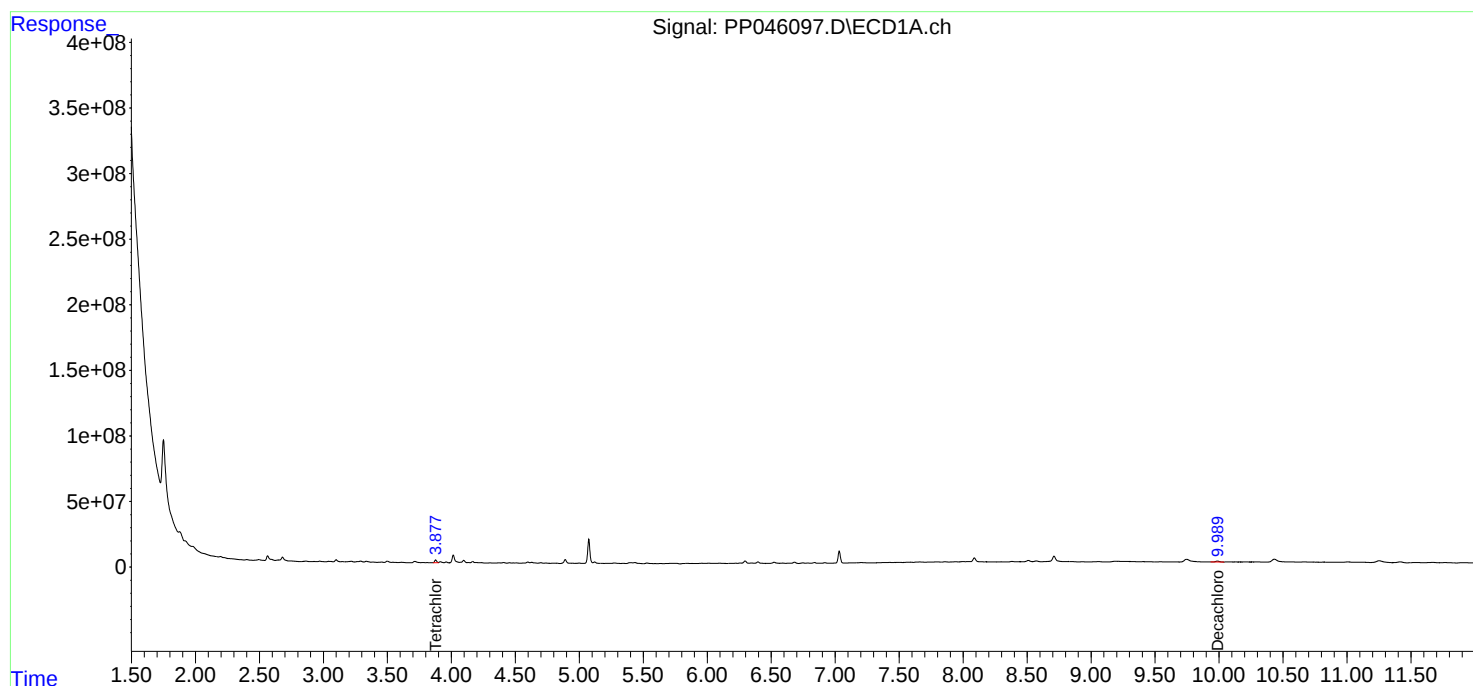

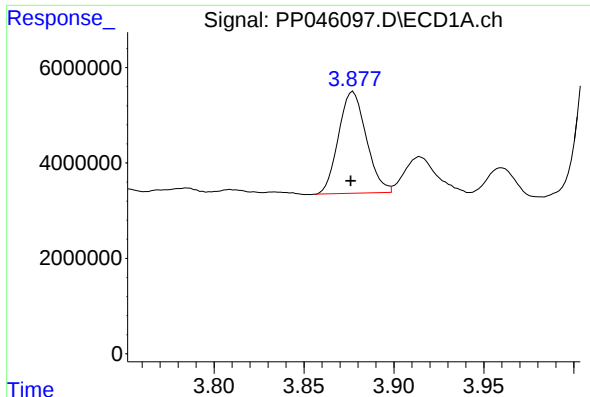


#1 Tetrachloro-m-xylene

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 22844045
Conc: 9.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
5576


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
Supervised By :mohammad ahmed 04/15/2022

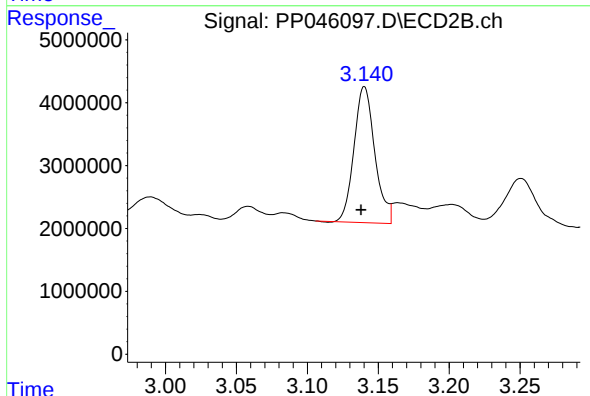


#1 Tetrachloro-m-xylene

R.T.: 3.140 min
Delta R.T.: 0.002 min
Response: 22116052
Conc: 13.92 ng/ml

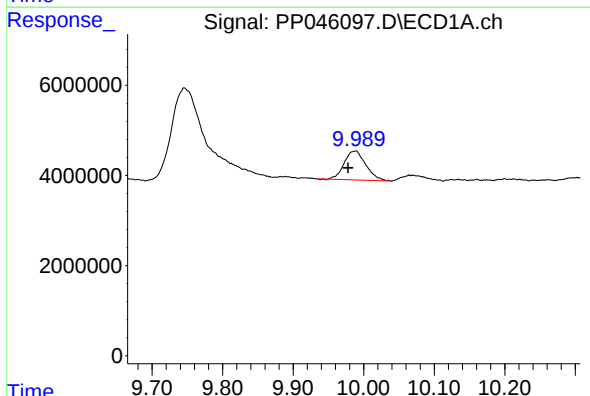

#2 Decachlorobiphenyl

R.T.: 9.988 min
Delta R.T.: 0.010 min
Response: 13603855
Conc: 8.29 ng/ml

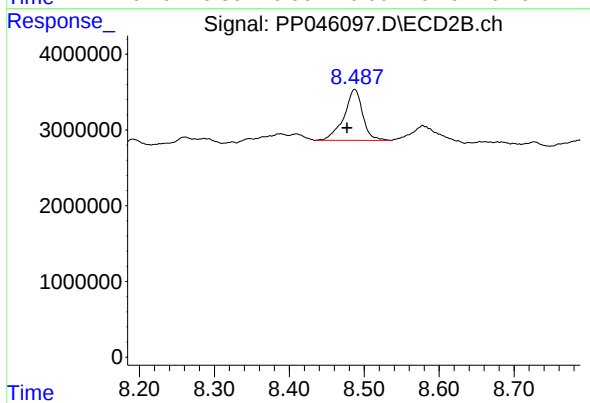

#2 Decachlorobiphenyl

R.T.: 8.487 min
Delta R.T.: 0.010 min
Response: 11688370
Conc: 8.20 ng/ml