

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
 Data File : PP046104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 09:12
 Operator : YP\AJ
 Sample : N2395-05 10X
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2022-13A


Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 16:48:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 12 05:31:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.875	3.138	4694428	3501415	1.909	2.204
2) SA Decachlor...	9.974	8.473	6636474	2535564	4.043	1.779m#
Target Compounds						
31) L7 AR-1260-1	6.863	5.852	8876906	8223471	100.560	103.901
32) L7 AR-1260-2	7.147	6.059	13594748	13715236	132.702	146.516
33) L7 AR-1260-3	7.540	6.221	9014401	8952078	109.418	101.058
34) L7 AR-1260-4	7.787	6.731	8147334	7781757	96.145	108.372
35) L7 AR-1260-5	8.129	7.000	23375406	24140998	142.331	142.119


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

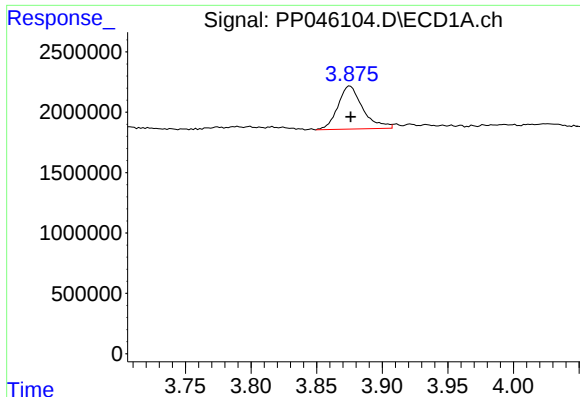

#1 Tetrachloro-m-xylene


R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 4694428
Conc: 1.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13A

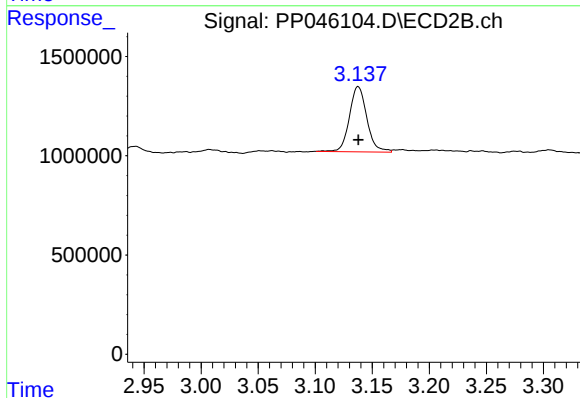


#1 Tetrachloro-m-xylene

R.T.: 3.138 min
Delta R.T.: 0.000 min
Response: 3501415
Conc: 2.20 ng/ml

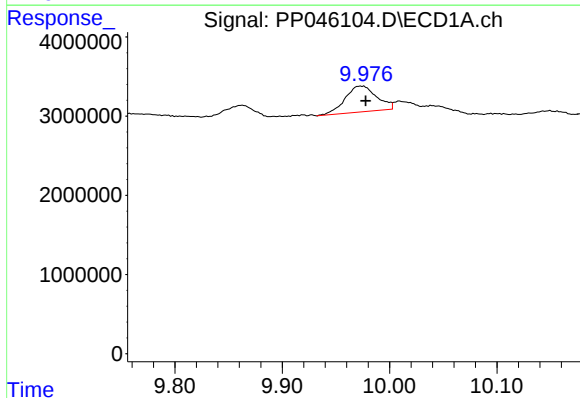


#2 Decachlorobiphenyl

R.T.: 9.974 min
Delta R.T.: -0.004 min
Response: 6636474
Conc: 4.04 ng/ml

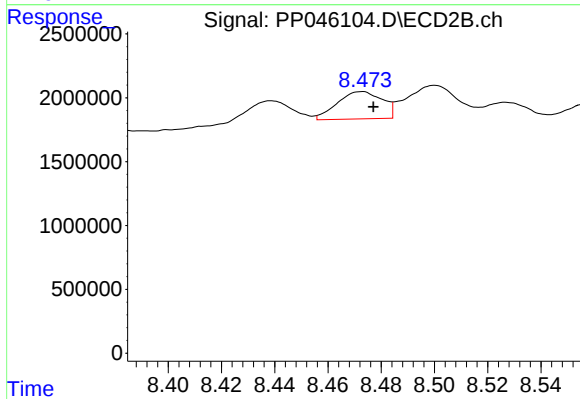

#2 Decachlorobiphenyl


R.T.: 8.473 min
Delta R.T.: -0.004 min
Response: 2535564
Conc: 1.78 ng/ml m

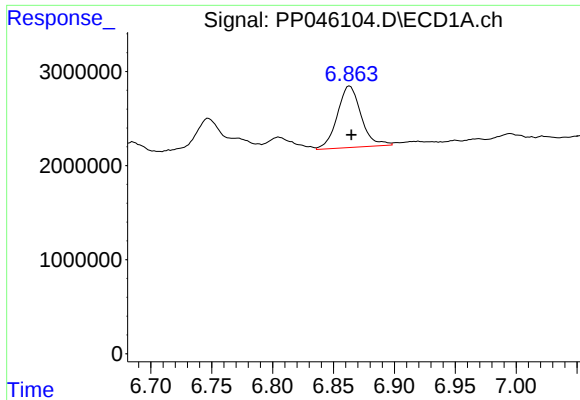

#31 AR-1260-1


R.T.: 6.863 min
Delta R.T.: -0.001 min
Response: 8876906
Conc: 100.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13A

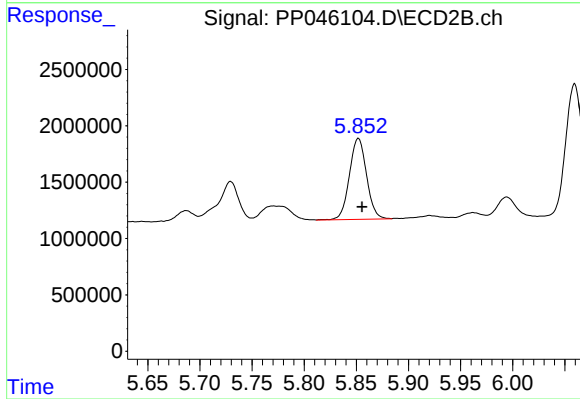


#31 AR-1260-1

R.T.: 5.852 min
Delta R.T.: -0.003 min
Response: 8223471
Conc: 103.90 ng/ml

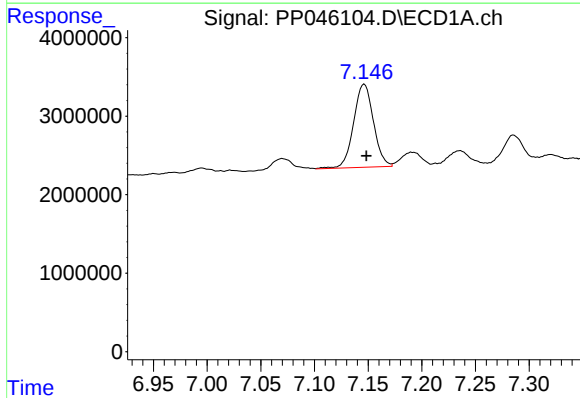


#32 AR-1260-2

R.T.: 7.147 min
Delta R.T.: -0.002 min
Response: 13594748
Conc: 132.70 ng/ml

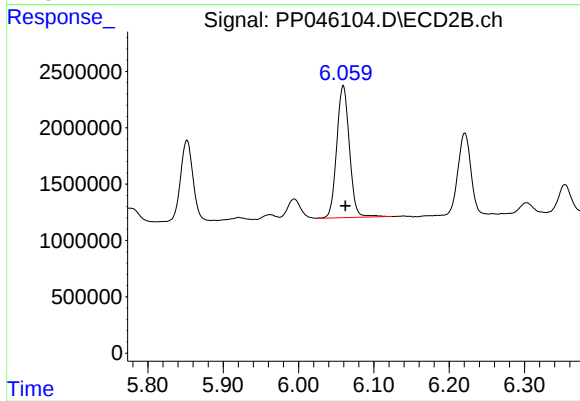

#32 AR-1260-2


R.T.: 6.059 min
Delta R.T.: -0.003 min
Response: 13715236
Conc: 146.52 ng/ml

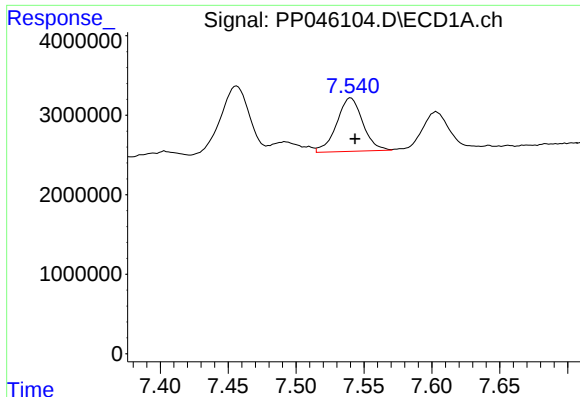

#33 AR-1260-3


R.T.: 7.540 min
Delta R.T.: -0.003 min
Response: 9014401
Conc: 109.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13A

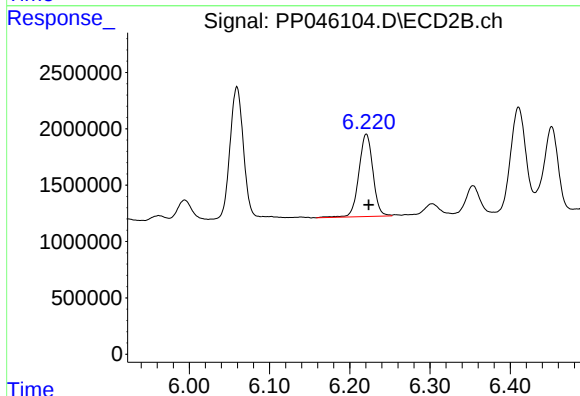


#33 AR-1260-3

R.T.: 6.221 min
Delta R.T.: -0.003 min
Response: 8952078
Conc: 101.06 ng/ml

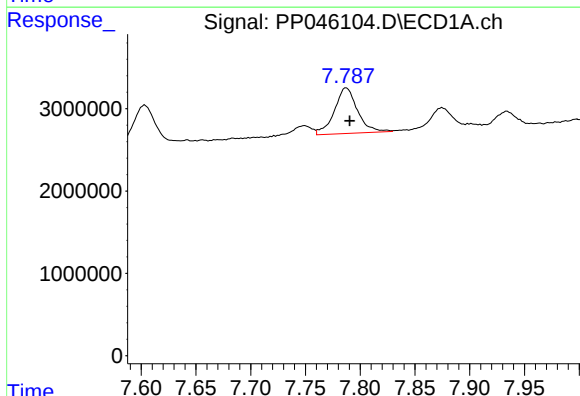


#34 AR-1260-4

R.T.: 7.787 min
Delta R.T.: -0.003 min
Response: 8147334
Conc: 96.15 ng/ml

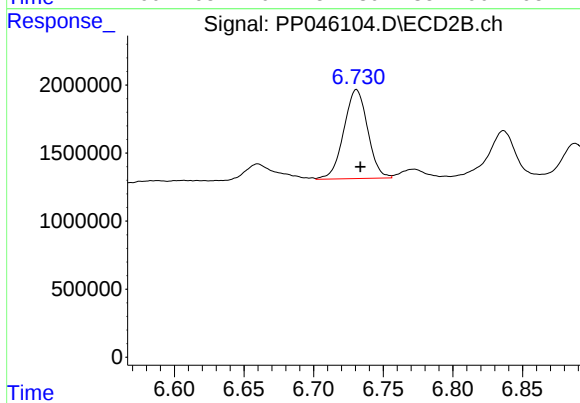

#34 AR-1260-4


R.T.: 6.731 min
Delta R.T.: -0.003 min
Response: 7781757
Conc: 108.37 ng/ml

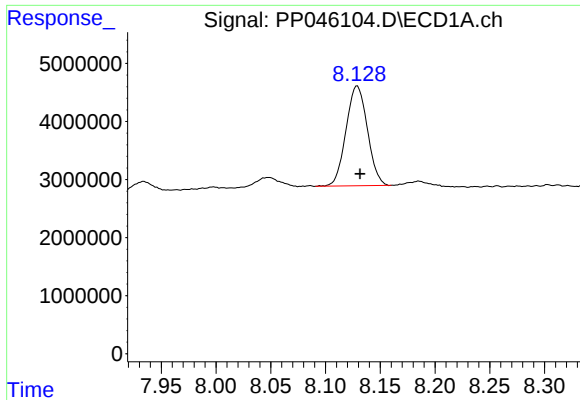

#35 AR-1260-5

R.T.: 8.129 min
Delta R.T.: -0.003 min
Response: 23375406
Conc: 142.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13A

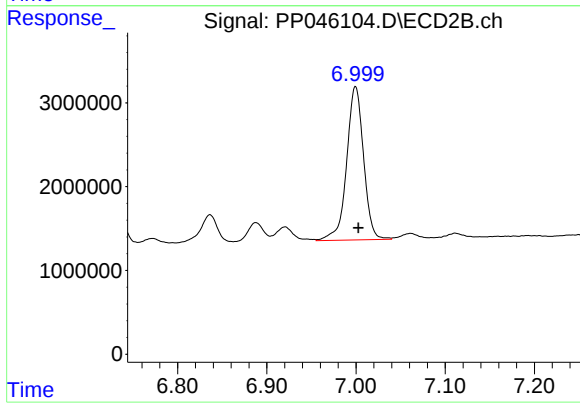

#35 AR-1260-5

R.T.: 7.000 min
Delta R.T.: -0.003 min
Response: 24140998
Conc: 142.12 ng/ml