

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
 Data File : PP046110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 11:31
 Operator : YP\AJ
 Sample : N2395-06 10X
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2022-13B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 16:50:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 12 05:31:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.874	3.137	4284919	3679415	1.742	2.316 #
2) SA Decachlor...	9.978	8.471	6365592	2364250	3.878	1.659m#
Target Compounds						
31) L7 AR-1260-1	6.864	5.851	6907026	5333613	78.245	67.388
32) L7 AR-1260-2	7.147	6.058	9966929	8535632	97.290	91.184
33) L7 AR-1260-3	7.541	6.218	6453738	6267427	78.336	70.752
34) L7 AR-1260-4	7.789	6.730	5614128	5661829	66.251	78.849
35) L7 AR-1260-5	8.130	6.998	15940779	15537176	97.062	91.468



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041522\
Data File : PP046110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 11:31
Operator : YP\AJ
Sample : N2395-06 10X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 16:50:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 12 05:31:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

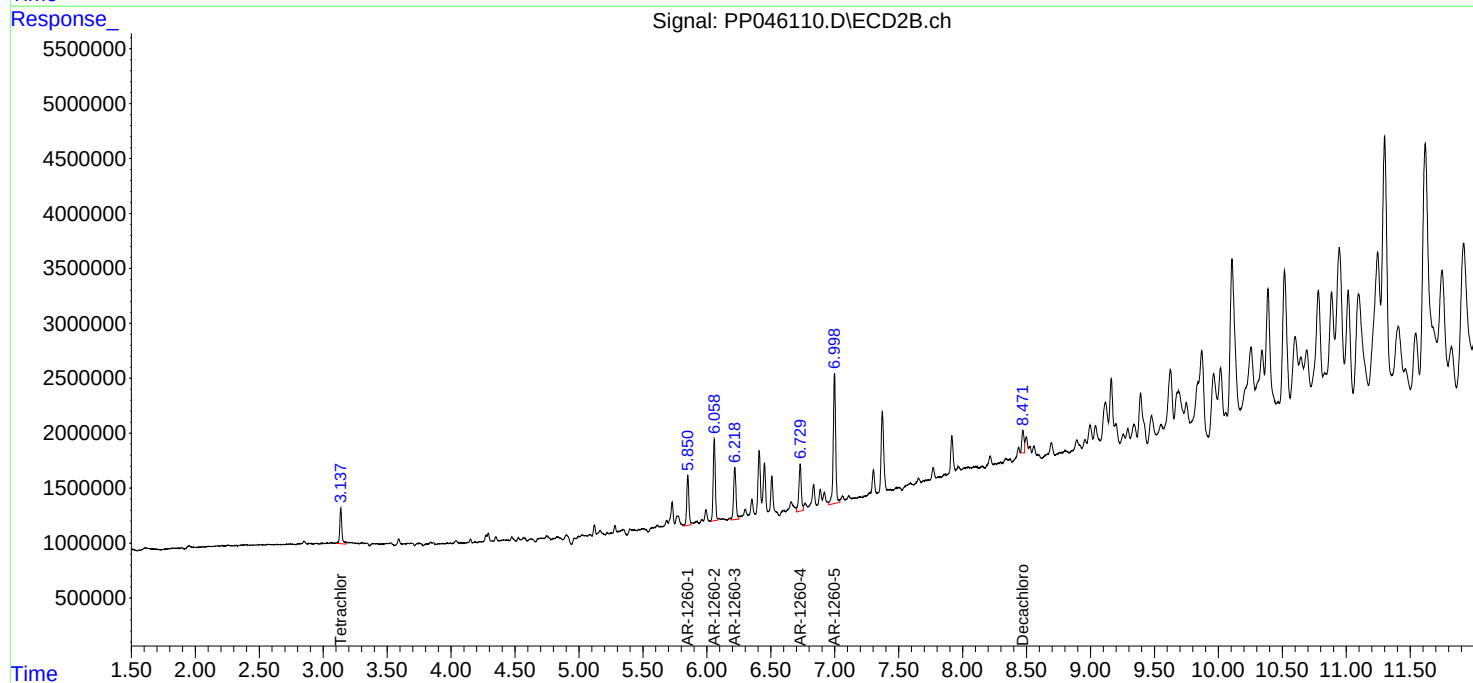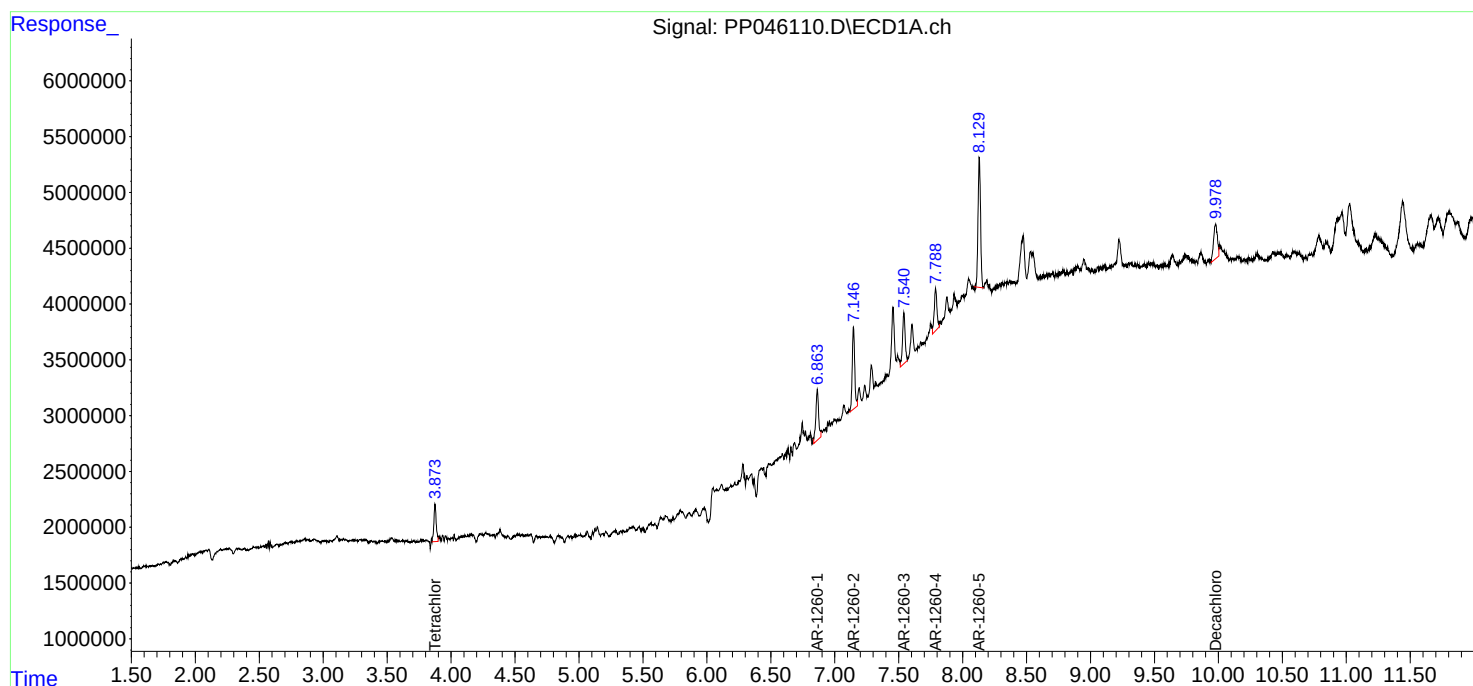


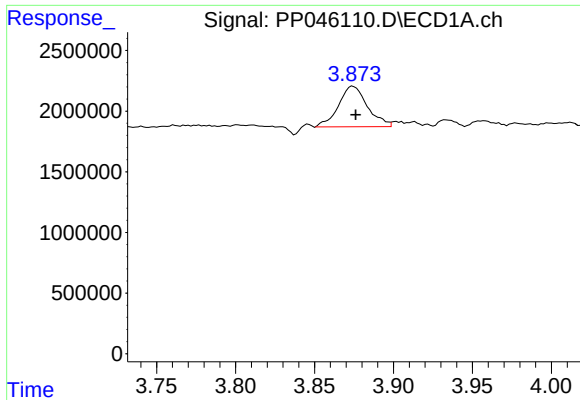

#1 Tetrachloro-m-xylene


R.T.: 3.874 min
Delta R.T.: -0.002 min
Response: 4284919
Conc: 1.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13B

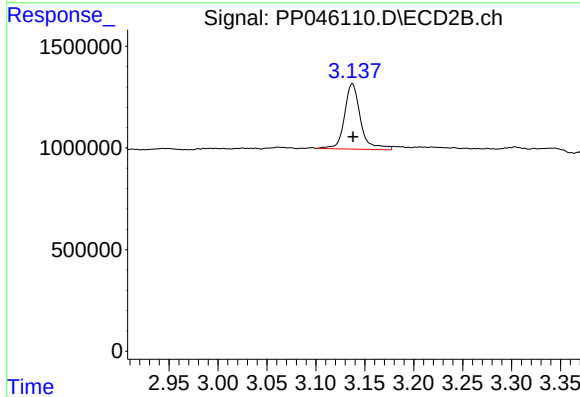


#1 Tetrachloro-m-xylene

R.T.: 3.137 min
Delta R.T.: 0.000 min
Response: 3679415
Conc: 2.32 ng/ml

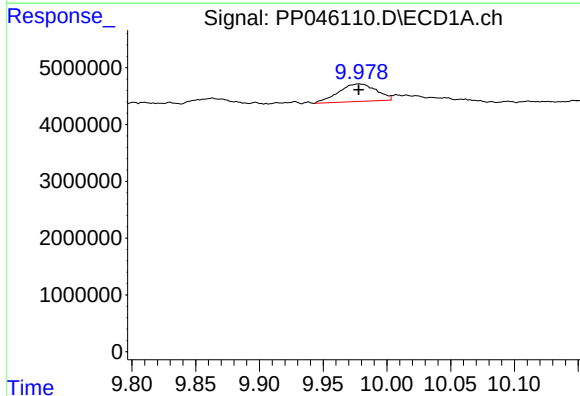


#2 Decachlorobiphenyl

R.T.: 9.978 min
Delta R.T.: 0.000 min
Response: 6365592
Conc: 3.88 ng/ml

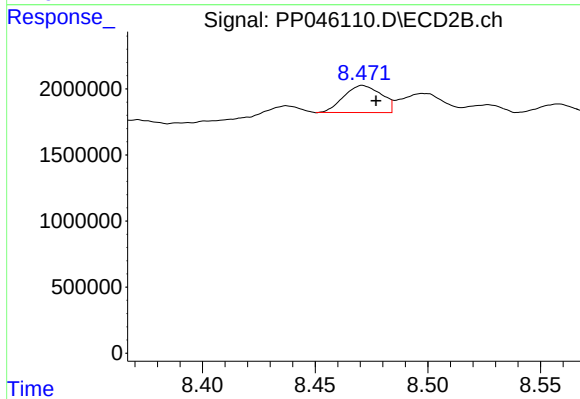

#2 Decachlorobiphenyl


R.T.: 8.471 min
Delta R.T.: -0.006 min
Response: 2364250
Conc: 1.66 ng/ml m

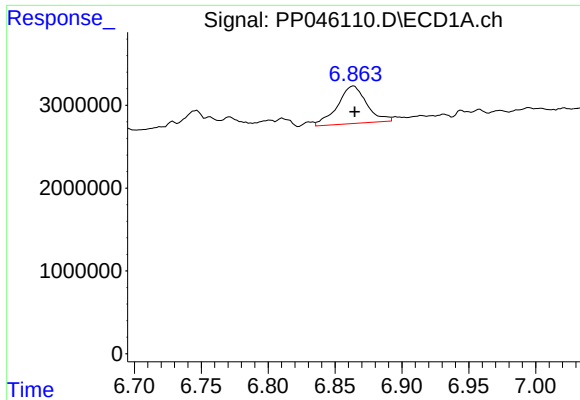

#31 AR-1260-1


R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 6907026
Conc: 78.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13B

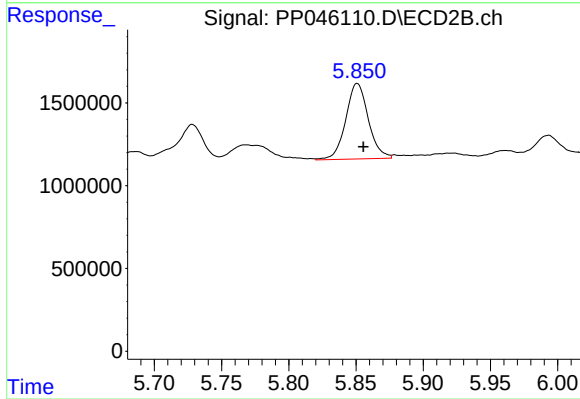


#31 AR-1260-1

R.T.: 5.851 min
Delta R.T.: -0.005 min
Response: 5333613
Conc: 67.39 ng/ml

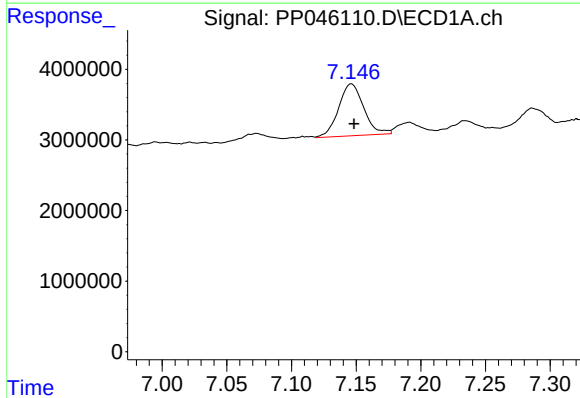


#32 AR-1260-2

R.T.: 7.147 min
Delta R.T.: -0.002 min
Response: 9966929
Conc: 97.29 ng/ml

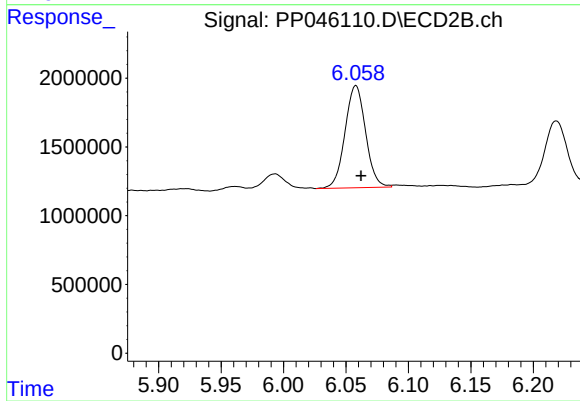

#32 AR-1260-2


R.T.: 6.058 min
Delta R.T.: -0.004 min
Response: 8535632
Conc: 91.18 ng/ml

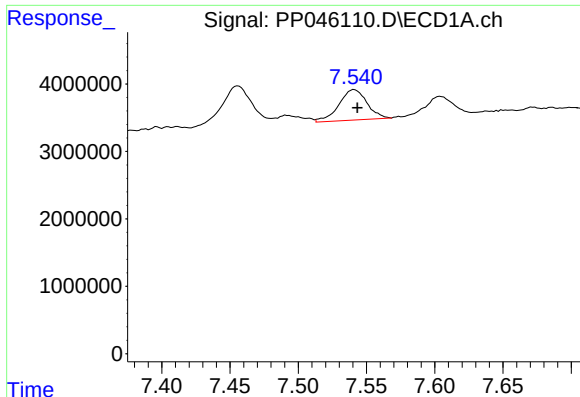

#33 AR-1260-3


R.T.: 7.541 min
Delta R.T.: -0.002 min
Response: 6453738
Conc: 78.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13B

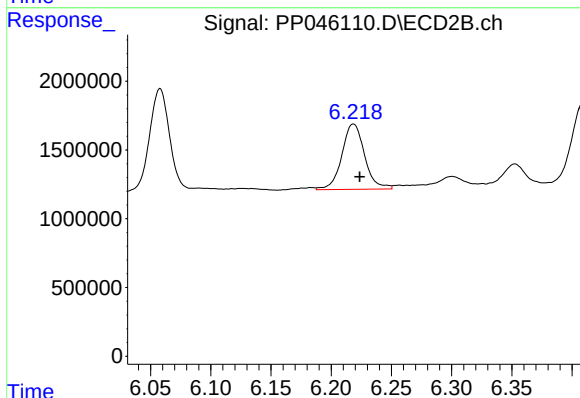


#33 AR-1260-3

R.T.: 6.218 min
Delta R.T.: -0.005 min
Response: 6267427
Conc: 70.75 ng/ml

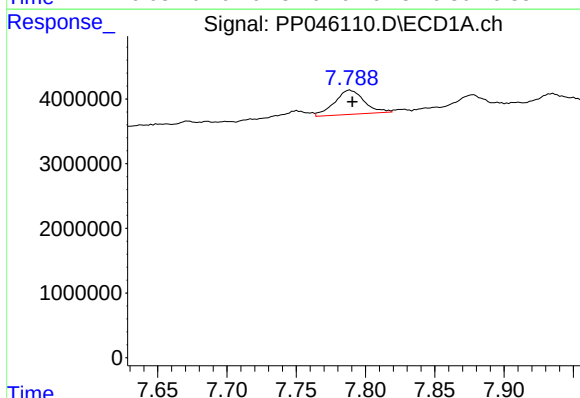


#34 AR-1260-4

R.T.: 7.789 min
Delta R.T.: -0.002 min
Response: 5614128
Conc: 66.25 ng/ml

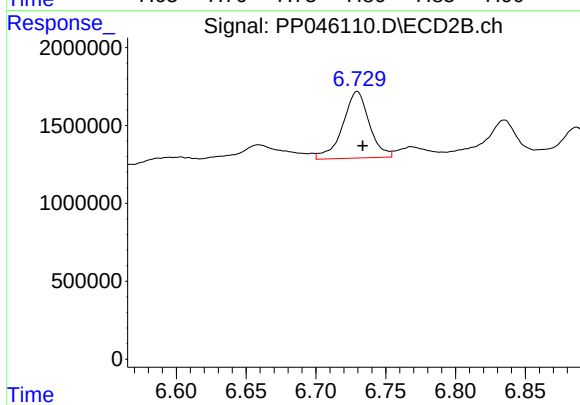

#34 AR-1260-4


R.T.: 6.730 min
Delta R.T.: -0.004 min
Response: 5661829
Conc: 78.85 ng/ml

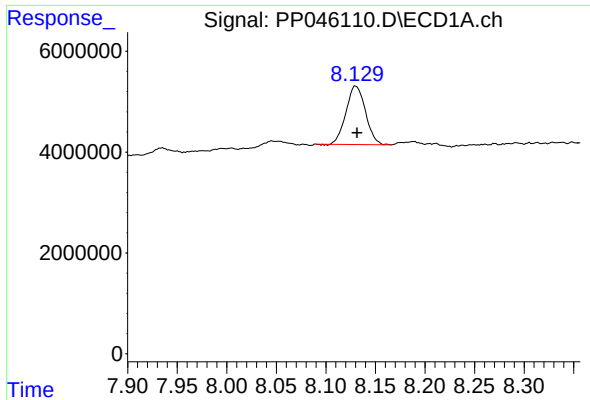

#35 AR-1260-5

R.T.: 8.130 min
Delta R.T.: -0.001 min
Response: 15940779
Conc: 97.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-2022-13B

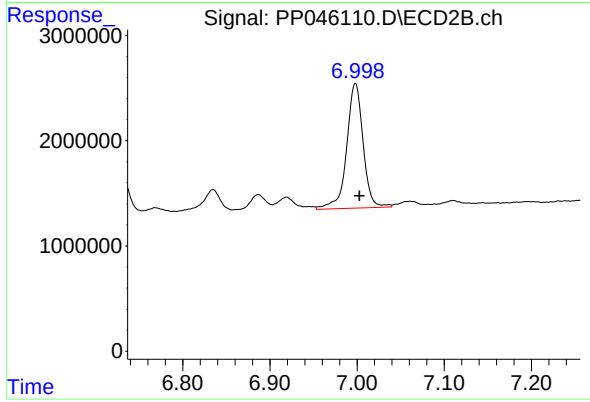

#35 AR-1260-5

R.T.: 6.998 min
Delta R.T.: -0.005 min
Response: 15537176
Conc: 91.47 ng/ml