

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041524\
 Data File : PP064336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2024 19:52
 Operator : YP\AJ
 Sample : P2112-06 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC288026-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :Ankita Jodhani 04/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:28:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.484	3.636	3705204	2966384	1.553m	1.242
2) SA Decachlor...	10.350	8.667	5622575	3677408	2.214	1.361 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041524\
Data File : PP064336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2024 19:52
Operator : YP\AJ
Sample : P2112-06 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC288026-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :Ankita Jodhani 04/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:28:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

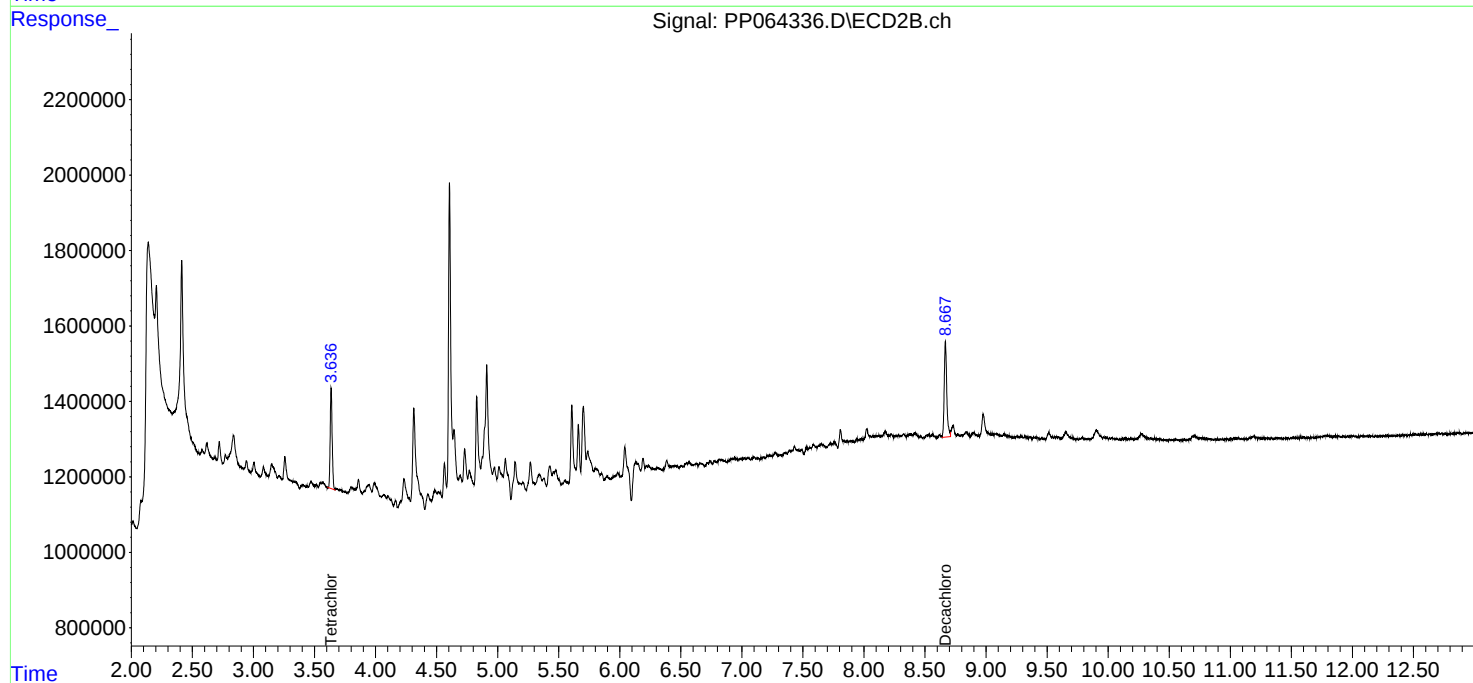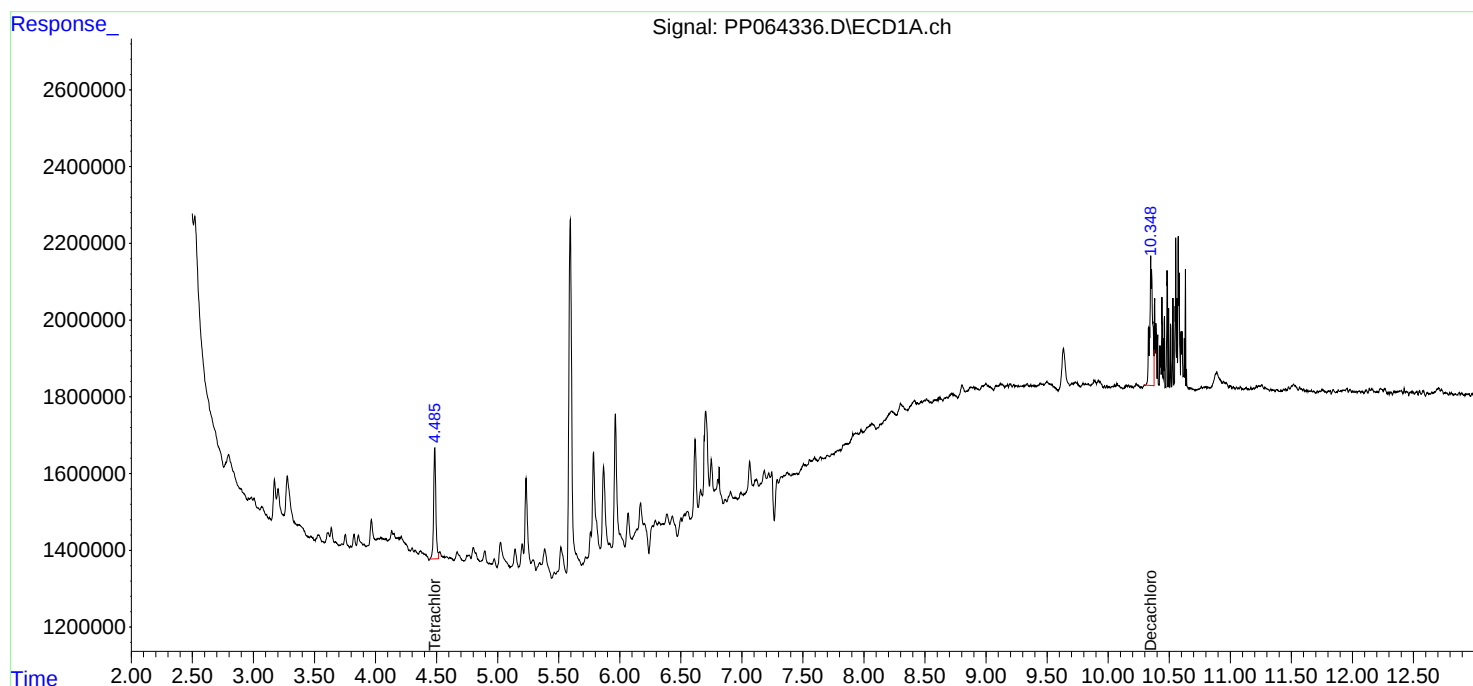

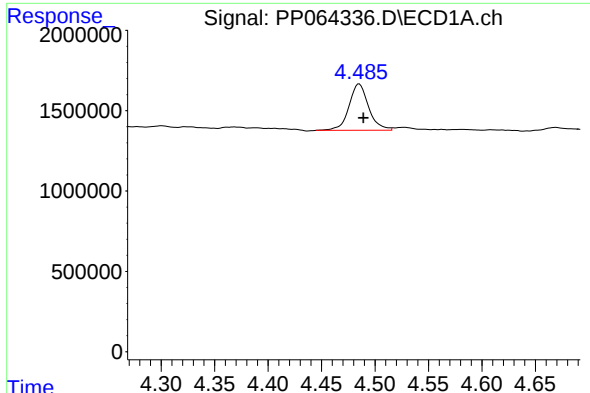


#1 Tetrachloro-m-xylene

R.T.: 4.484 min
Delta R.T.: -0.005 min
Response: 3705204
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC288026-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :Ankita Jodhani 04/16/2024

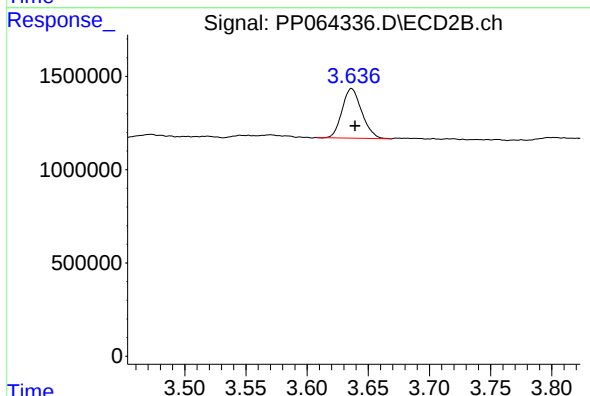


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.003 min
Response: 2966384
Conc: 1.24 ng/ml

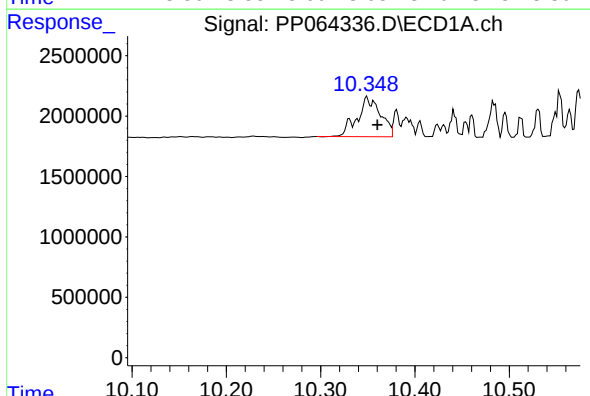

#2 Decachlorobiphenyl

R.T.: 10.350 min
Delta R.T.: -0.010 min
Response: 5622575
Conc: 2.21 ng/ml

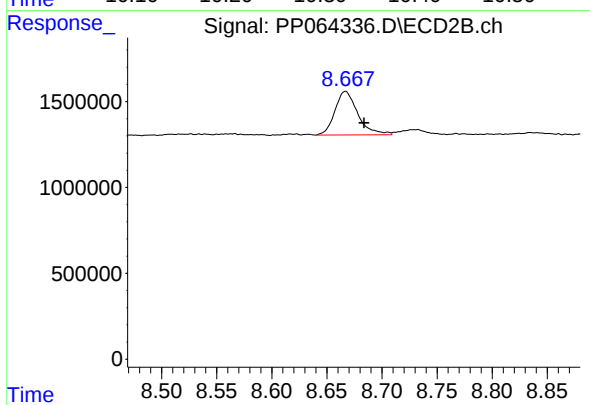

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.017 min
Response: 3677408
Conc: 1.36 ng/ml