

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041524\
 Data File : PP064340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2024 20:57
 Operator : YP\AJ
 Sample : P2112-03 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC274767-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :Ankita Jodhani 04/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 01:29:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.486	3.638	3538691	3643092	1.483	1.526
2) SA Decachlor...	10.353	8.666	4533061	3753188	1.785m	1.389

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041524\
Data File : PP064340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2024 20:57
Operator : YP\AJ
Sample : P2112-03 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC274767-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :Ankita Jodhani 04/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 01:29:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

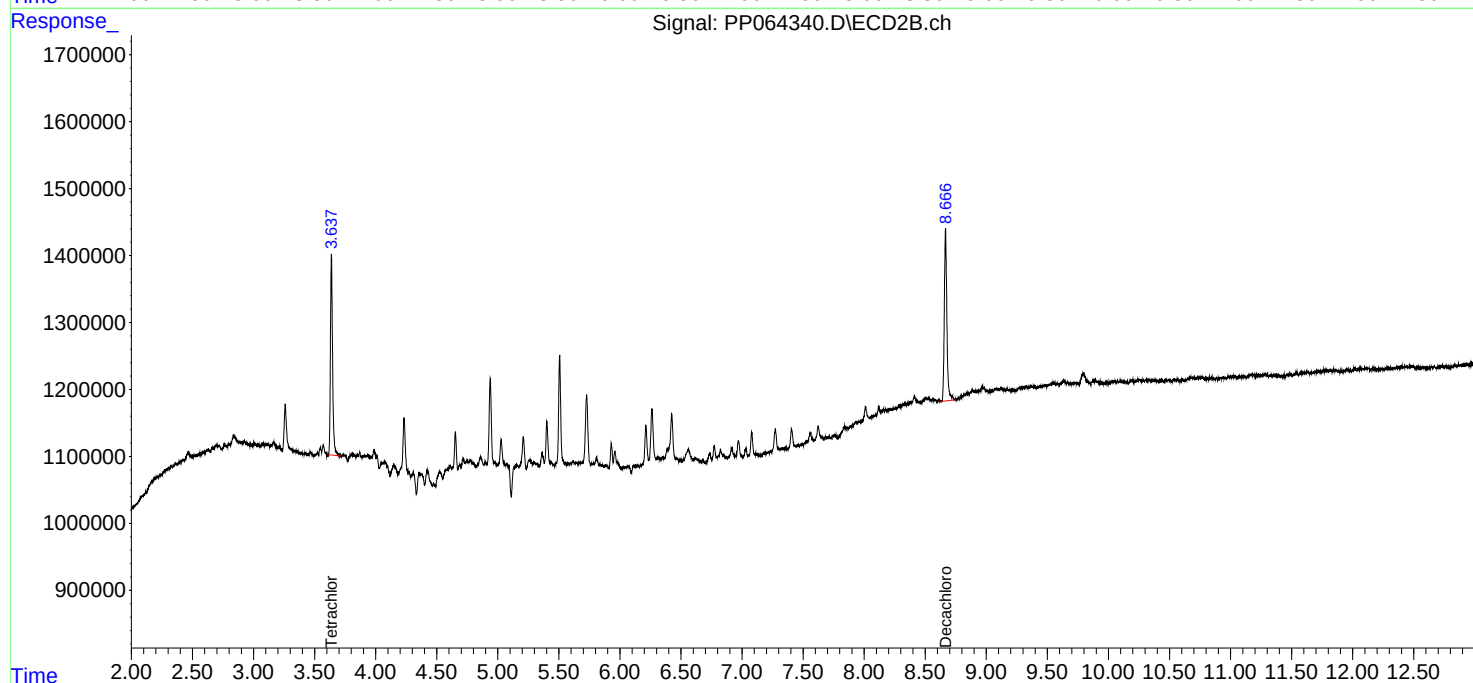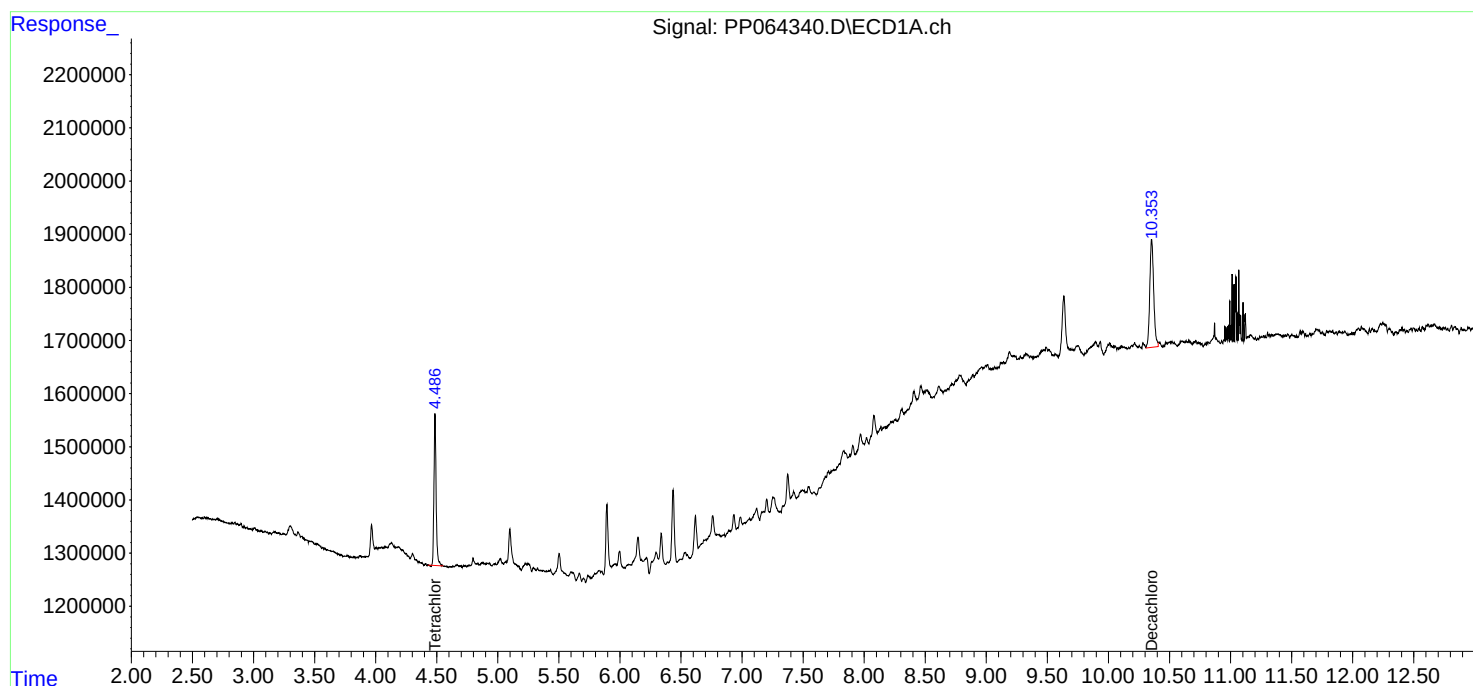

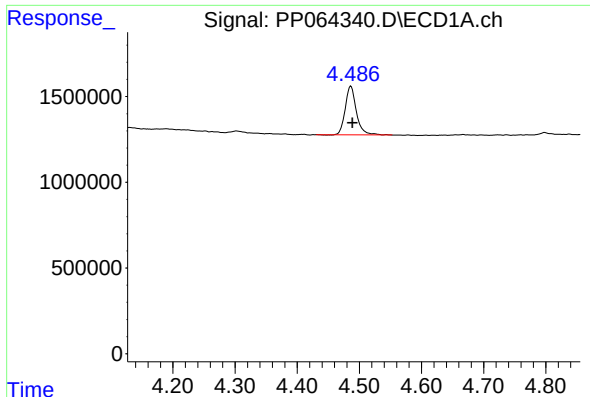


#1 Tetrachloro-m-xylene

R.T.: 4.486 min
Delta R.T.: -0.003 min
Response: 3538691
Conc: 1.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC274767-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :Ankita Jodhani 04/16/2024

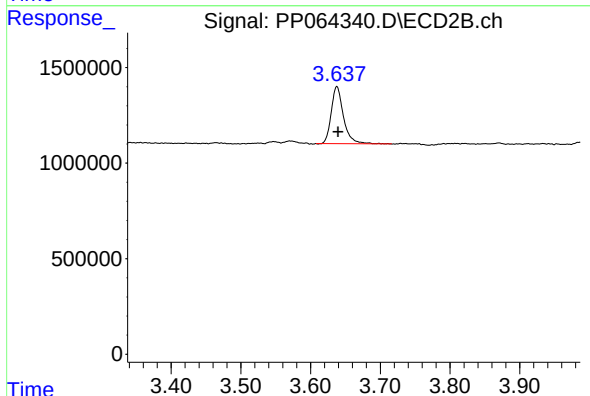


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.002 min
Response: 3643092
Conc: 1.53 ng/ml

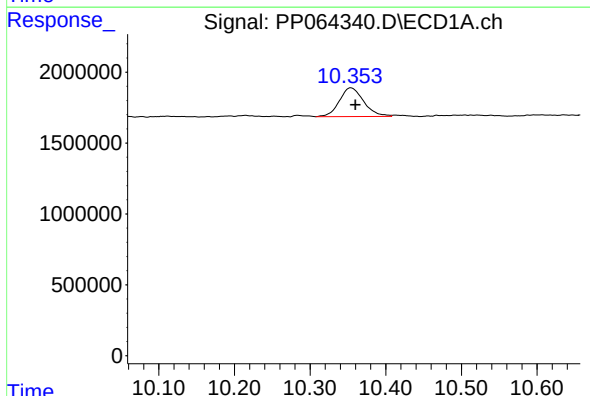

#2 Decachlorobiphenyl

R.T.: 10.353 min
Delta R.T.: -0.007 min
Response: 4533061
Conc: 1.79 ng/ml m

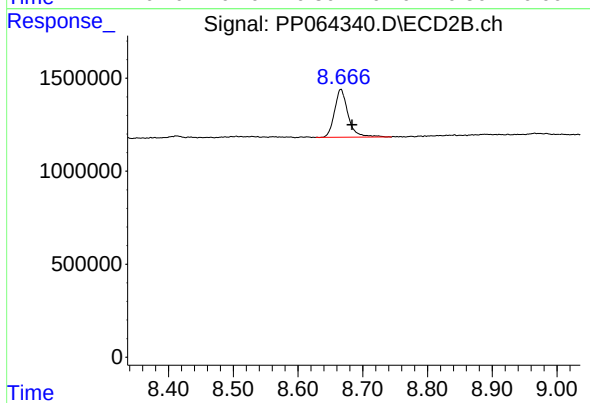

#2 Decachlorobiphenyl

R.T.: 8.666 min
Delta R.T.: -0.018 min
Response: 3753188
Conc: 1.39 ng/ml