

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041621\
 Data File : PP034943.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2021 9:30
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 4/20/2021 11:12:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 17:27:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.844	4.259	4404523	2685634	57.738	59.784
2) SA Decachlor...	10.760	9.555	4155566	1637084	53.982	57.979
Target Compounds						
26) L6 AR-1254-1	7.059	6.376	1484134	1039835	539.777	563.624
27) L6 AR-1254-2	7.288	6.532	2335147	908895	549.171	568.099
28) L6 AR-1254-3	7.669	6.952	2483252	1422036	544.074	569.781
29) L6 AR-1254-4	7.965	7.189	1608017	762056	520.081	579.712
30) L6 AR-1254-5	8.392	7.614	1905887	1058999	536.290	521.051m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041621\
Data File : PP034943.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2021 9:30
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/20/2021 11:12:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 17:27:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

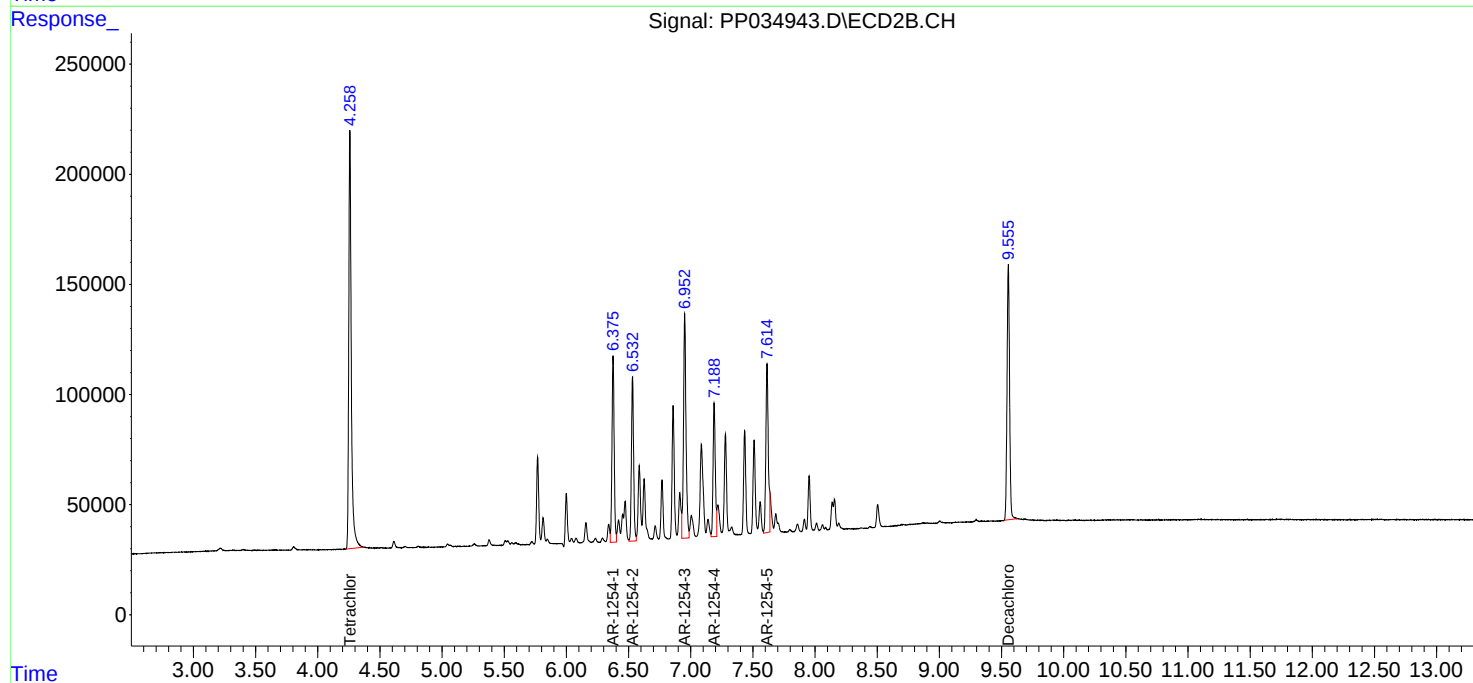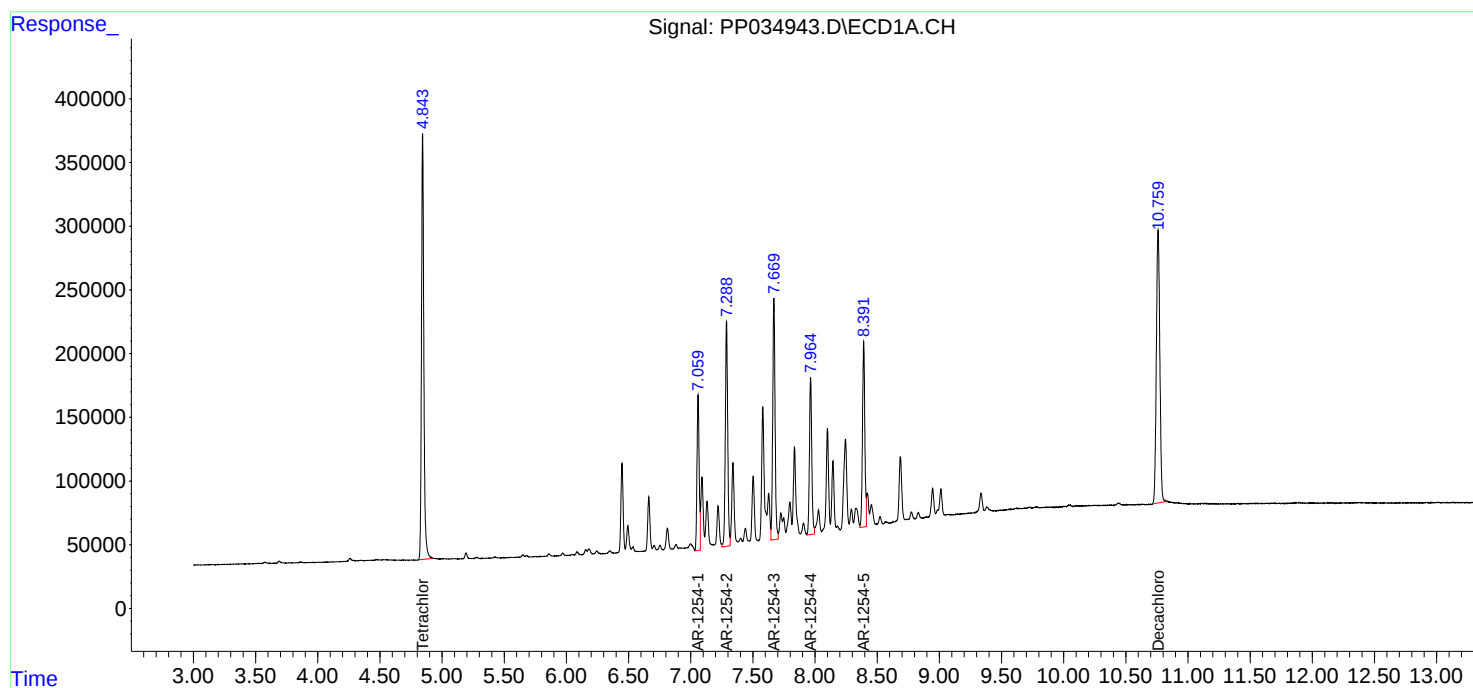

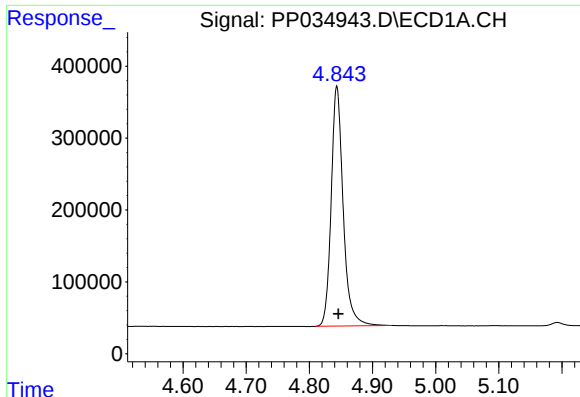


#1 Tetrachloro-m-xylene

R.T.: 4.844 min
Delta R.T.: -0.002 min
Response: 4404523
Conc: 57.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/20/2021 11:12:40 AM

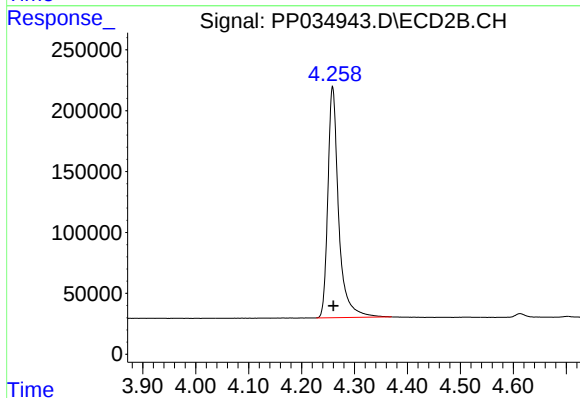


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: -0.001 min
Response: 2685634
Conc: 59.78 ng/ml

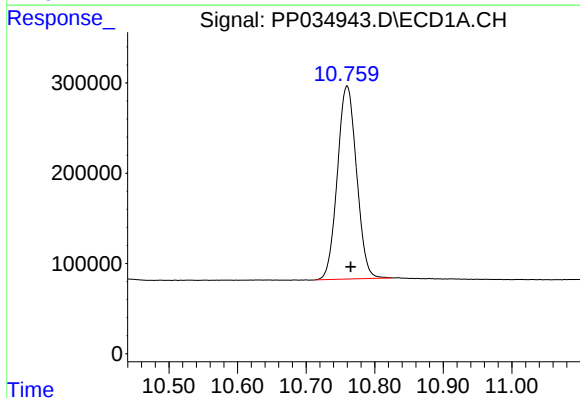


#2 Decachlorobiphenyl

R.T.: 10.760 min
Delta R.T.: -0.005 min
Response: 4155566
Conc: 53.98 ng/ml

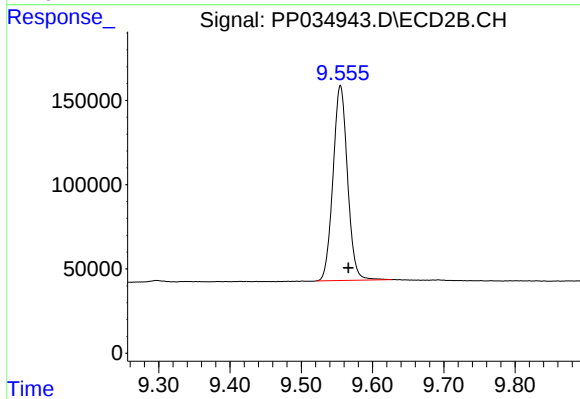

#2 Decachlorobiphenyl

R.T.: 9.555 min
Delta R.T.: -0.011 min
Response: 1637084
Conc: 57.98 ng/ml

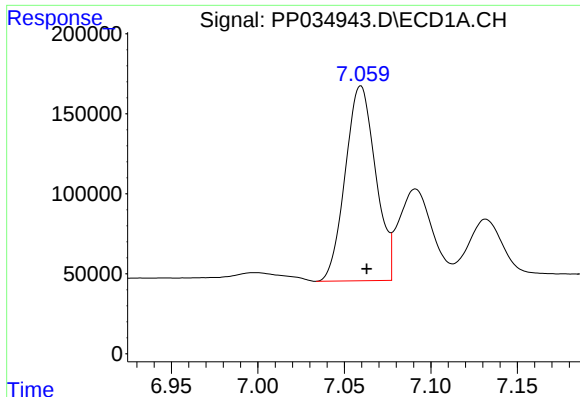


#26 AR-1254-1

R.T.: 7.059 min
Delta R.T.: -0.004 min
Response: 1484134
Conc: 539.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/20/2021 11:12:40 AM

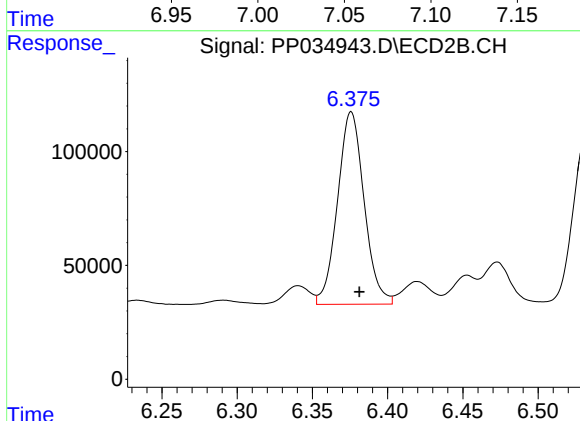


#26 AR-1254-1

R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 1039835
Conc: 563.62 ng/ml

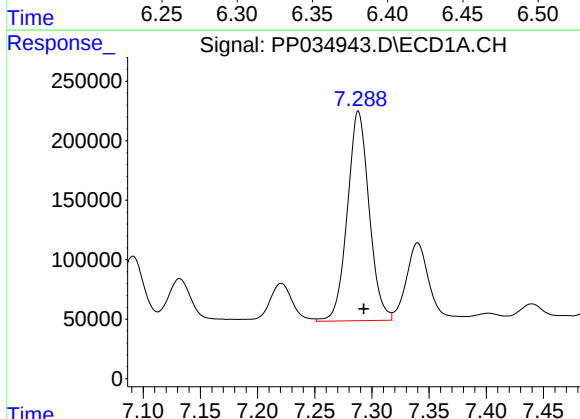


#27 AR-1254-2

R.T.: 7.288 min
Delta R.T.: -0.005 min
Response: 2335147
Conc: 549.17 ng/ml

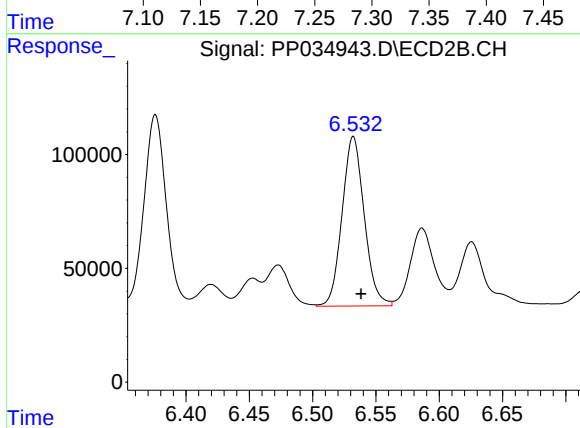

#27 AR-1254-2

R.T.: 6.532 min
Delta R.T.: -0.006 min
Response: 908895
Conc: 568.10 ng/ml

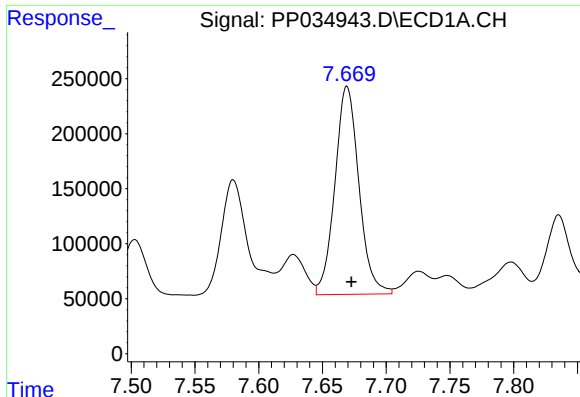


#28 AR-1254-3

R.T.: 7.669 min
Delta R.T.: -0.003 min
Response: 2483252
Conc: 544.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/20/2021 11:12:40 AM

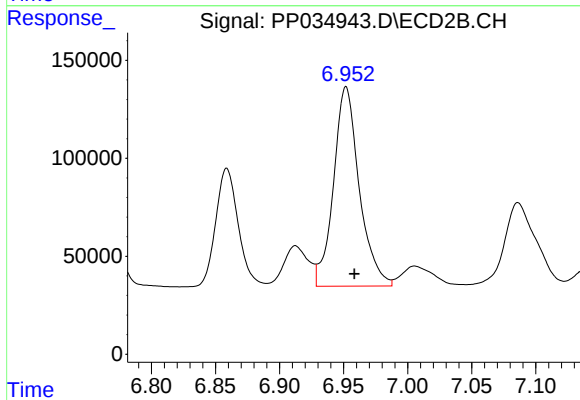


#28 AR-1254-3

R.T.: 6.952 min
Delta R.T.: -0.007 min
Response: 1422036
Conc: 569.78 ng/ml

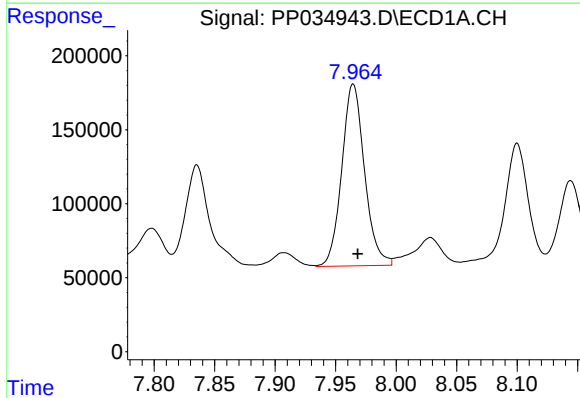


#29 AR-1254-4

R.T.: 7.965 min
Delta R.T.: -0.004 min
Response: 1608017
Conc: 520.08 ng/ml

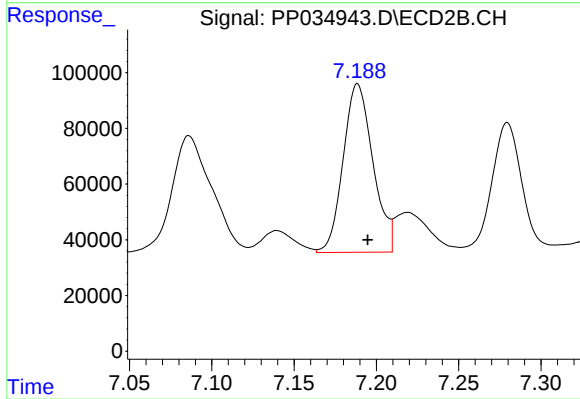

#29 AR-1254-4

R.T.: 7.189 min
Delta R.T.: -0.006 min
Response: 762056
Conc: 579.71 ng/ml

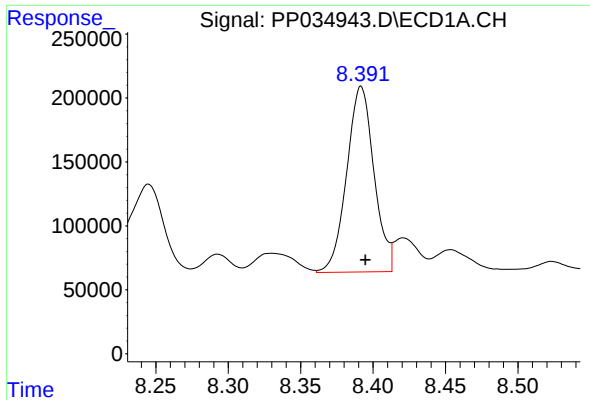


#30 AR-1254-5

R.T.: 8.392 min
Delta R.T.: -0.003 min
Response: 1905887
Conc: 536.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
4/20/2021 11:12:40 AM

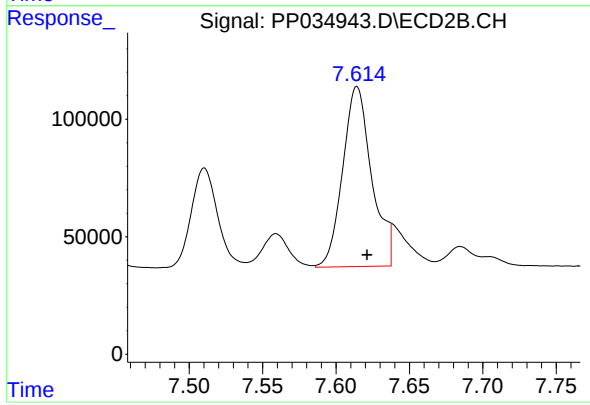

#30 AR-1254-5

R.T.: 7.614 min
Delta R.T.: -0.007 min
Response: 1058999
Conc: 521.05 ng/ml m