

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041621\
 Data File : PP034947.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Apr 2021 10:57
 Operator : DD\AJ
 Sample : M2046-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-4

Manual Integrations
 APPROVED

Ankita
 4/20/2021 11:12:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 17:29:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.258	1858131	1163018	24.358	25.890
2) SA Decachlor...	10.765	9.556	2030040	726393	26.371m	25.726m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041621\
Data File : PP034947.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Apr 2021 10:57
Operator : DD\AJ
Sample : M2046-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-4


Manual Integrations
APPROVED

Ankita
4/20/2021 11:12:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 17:29:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

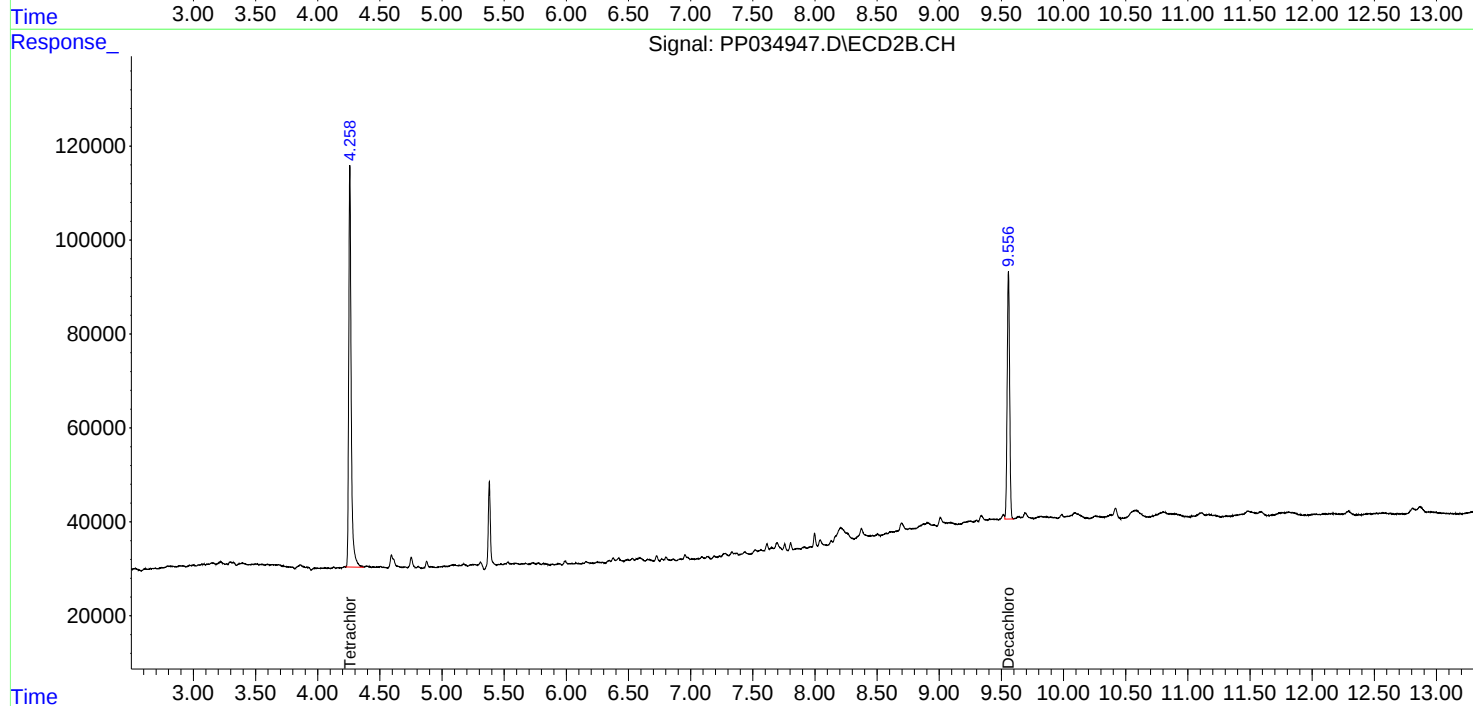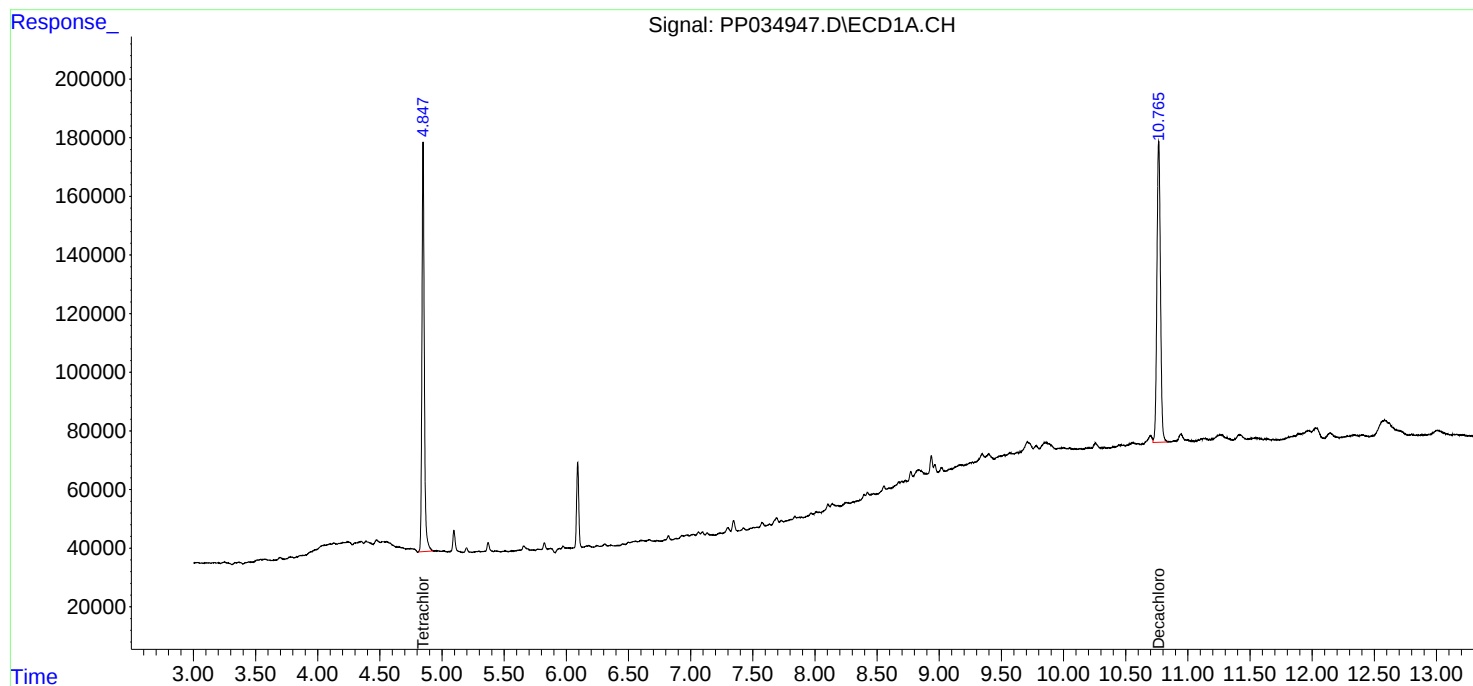

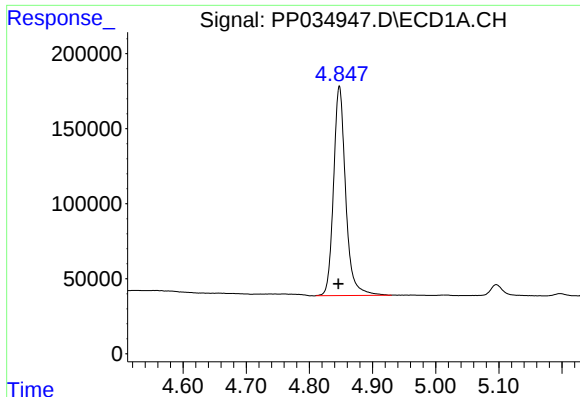


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: 0.002 min
Response: 1858131
Conc: 24.36 ng/ml

Instrument :
ECD_P
ClientSampled :
WC-4


Manual Integrations
APPROVED

Ankita
4/20/2021 11:12:42 AM

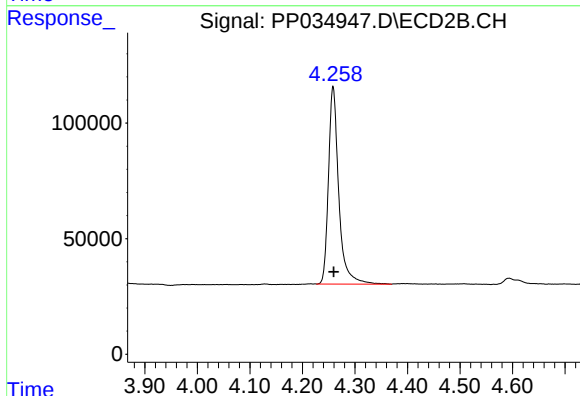


#1 Tetrachloro-m-xylene

R.T.: 4.258 min
Delta R.T.: -0.001 min
Response: 1163018
Conc: 25.89 ng/ml

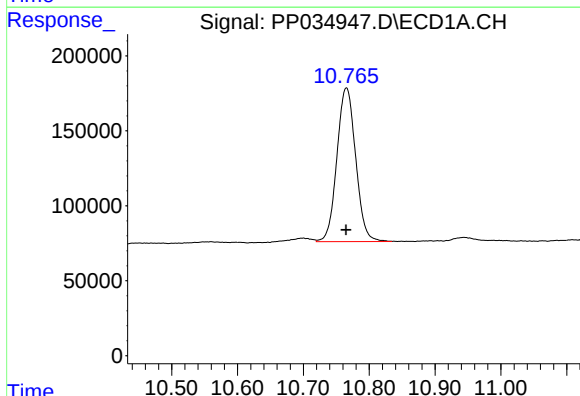

#2 Decachlorobiphenyl

R.T.: 10.765 min
Delta R.T.: 0.000 min
Response: 2030040
Conc: 26.37 ng/ml m

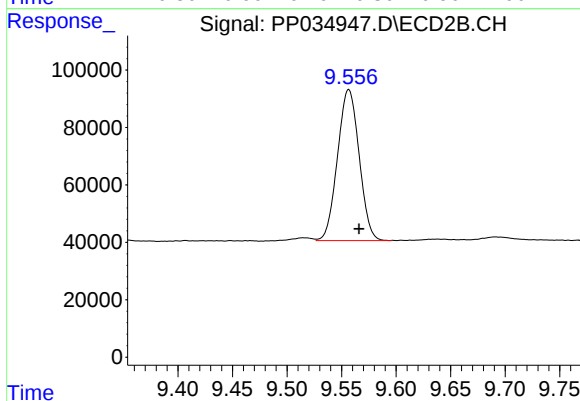

#2 Decachlorobiphenyl

R.T.: 9.556 min
Delta R.T.: -0.010 min
Response: 726393
Conc: 25.73 ng/ml m