

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041622\
 Data File : PP046133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 19:27
 Operator : YP\AJ
 Sample : N2395-19 10X
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-2022-21B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/18/2022
 Supervised By :mohammad ahmed 04/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 00:58:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 12 05:31:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.875	3.138	3007734	2586783	1.223	1.628 #
2) SA Decachlor...	9.980	8.471	5606125	3230936	3.415m	2.267 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041622\
Data File : PP046133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 19:27
Operator : YP\AJ
Sample : N2395-19 10X
Misc :
ALS Vial : 85 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LAW-2022-21B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/18/2022
Supervised By :mohammad ahmed 04/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 00:58:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 12 05:31:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

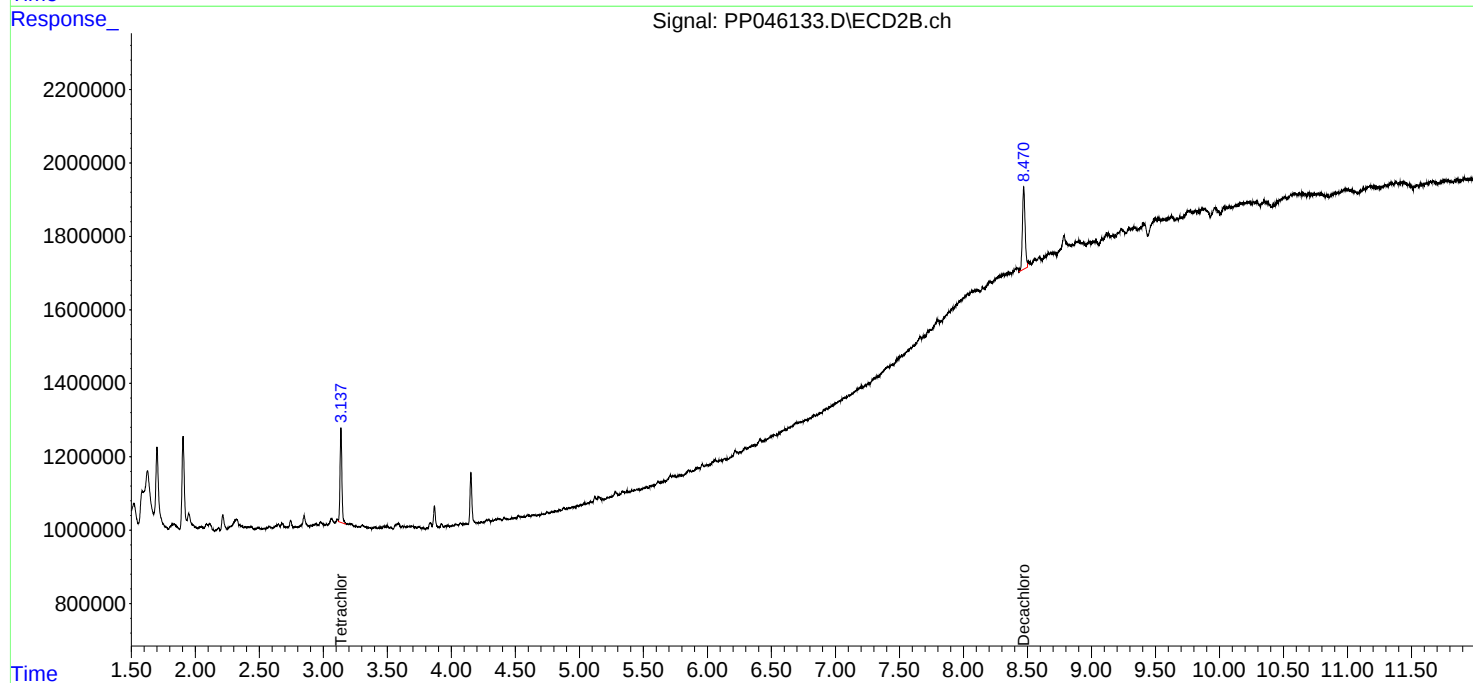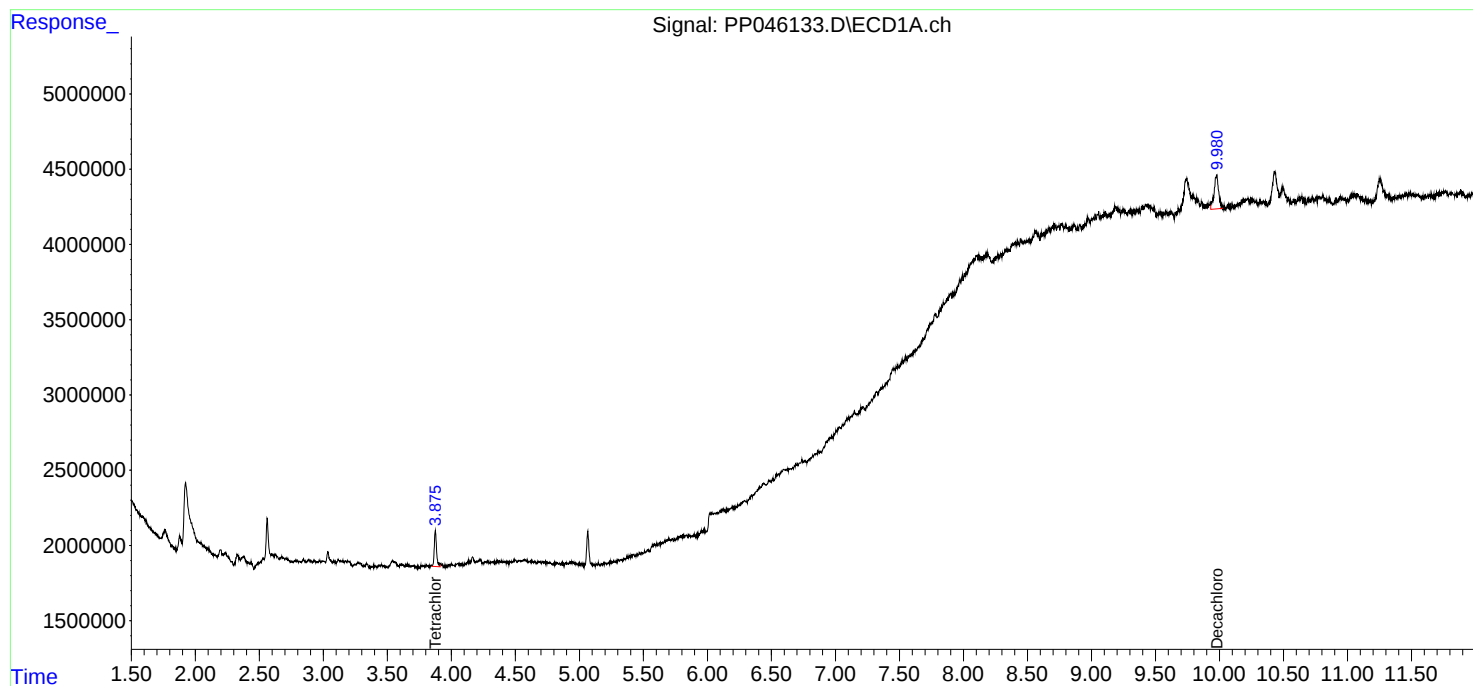

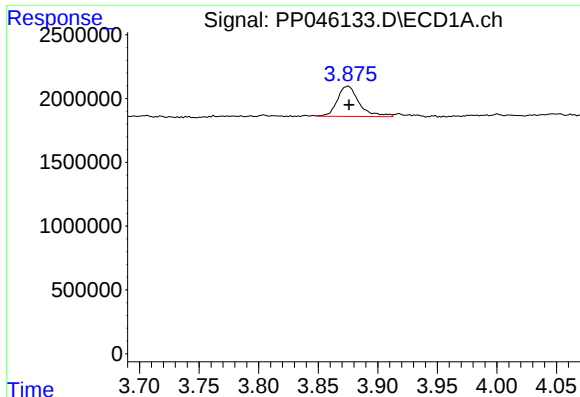

#1 Tetrachloro-m-xylene

R.T.: 3.875 min
Delta R.T.: 0.000 min
Response: 3007734
Conc: 1.22 ng/ml

Instrument :

ECD_P

ClientSampleId :


LAW-2022-21B

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 04/18/2022

Supervised By :mohammad ahmed 04/18/2022

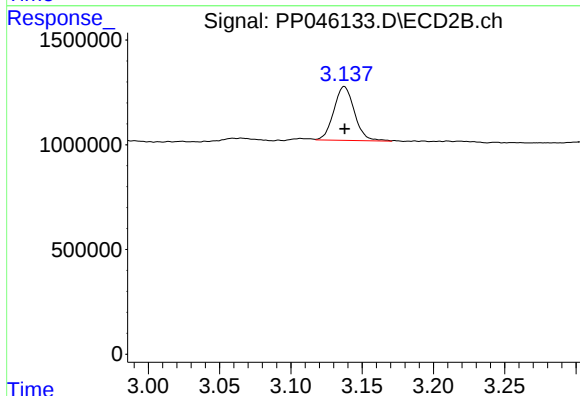


#1 Tetrachloro-m-xylene

R.T.: 3.138 min
Delta R.T.: 0.000 min
Response: 2586783
Conc: 1.63 ng/ml

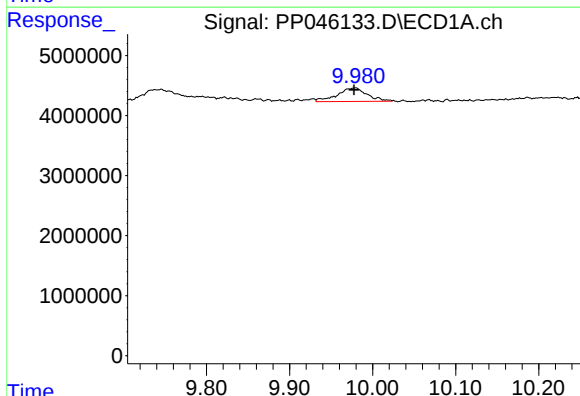

#2 Decachlorobiphenyl

R.T.: 9.980 min
Delta R.T.: 0.002 min
Response: 5606125
Conc: 3.42 ng/ml m

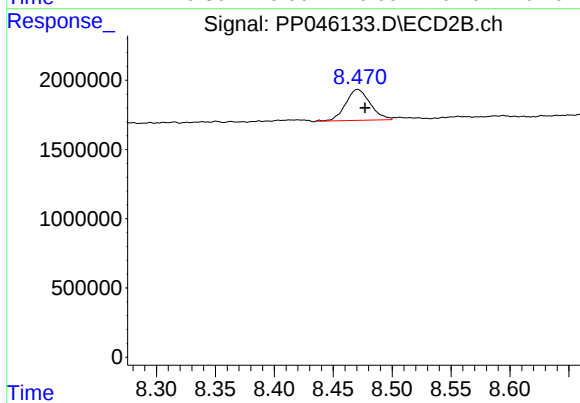

#2 Decachlorobiphenyl

R.T.: 8.471 min
Delta R.T.: -0.006 min
Response: 3230936
Conc: 2.27 ng/ml