

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041719\
 Data File : PP029924.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Apr 2019 16:10
 Operator : EI/SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 03:14:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041319.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 12 14:33:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
15) T	Picloram	17.524	0.000	1893015	0	7.411 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041719\
Data File : PP029924.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Apr 2019 16:10
Operator : EI/SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 03:14:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041319.M
Quant Title : 8080.M
QLast Update : Fri Apr 12 14:33:50 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

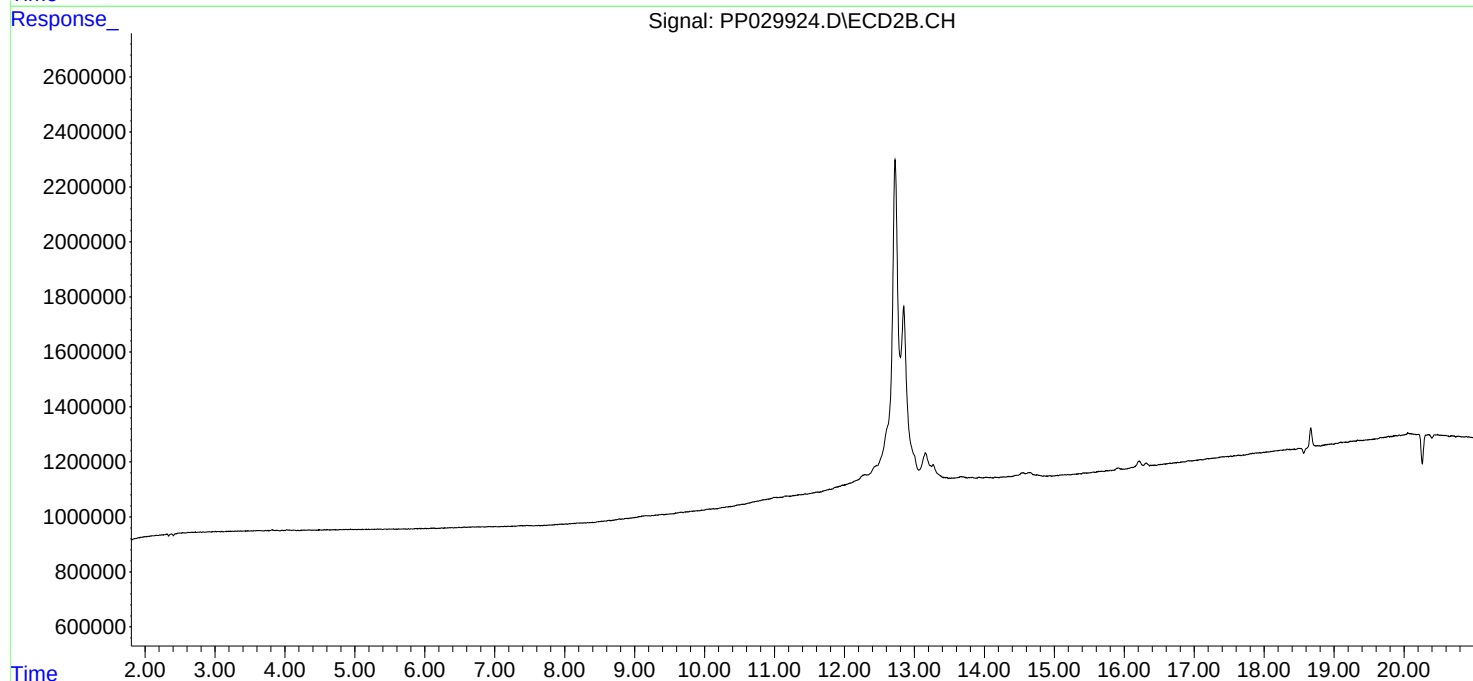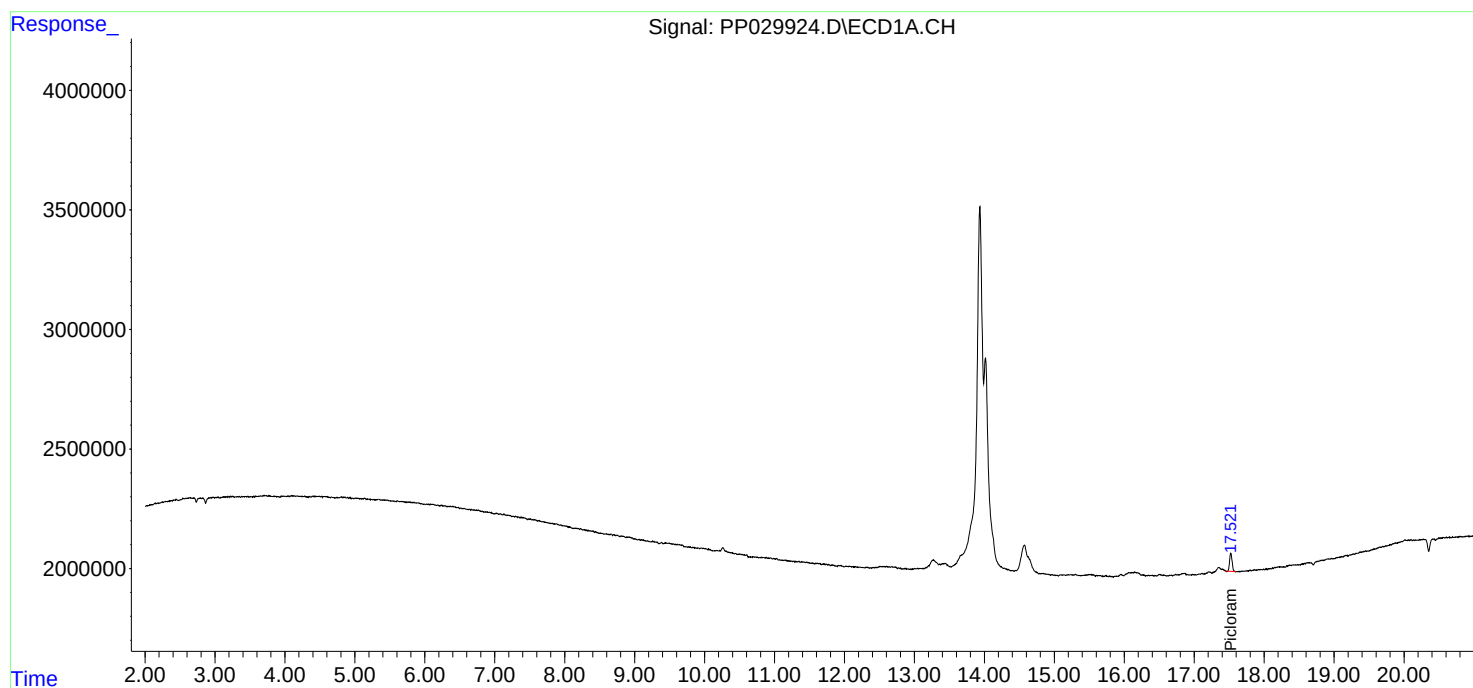


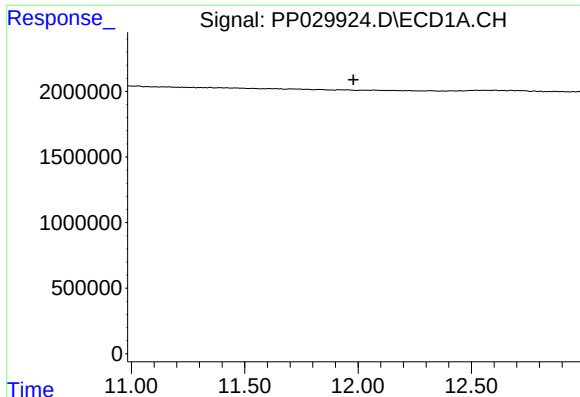

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.980 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

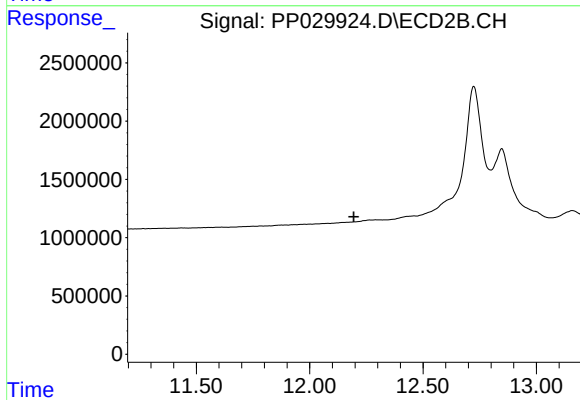


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 12.195 min
Response: 0
Conc: N.D.

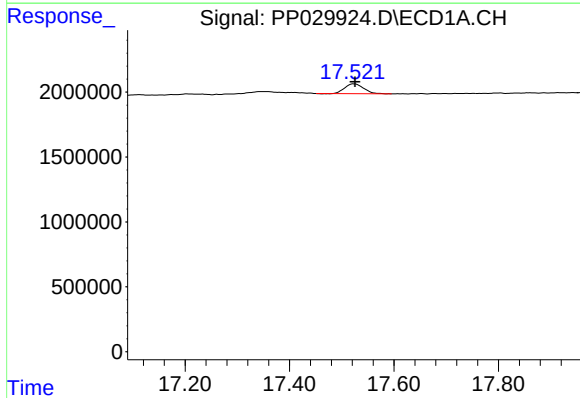

#15 Picloram

R.T.: 17.524 min
Delta R.T.: -0.002 min
Response: 1893015
Conc: 7.41 ng/ml

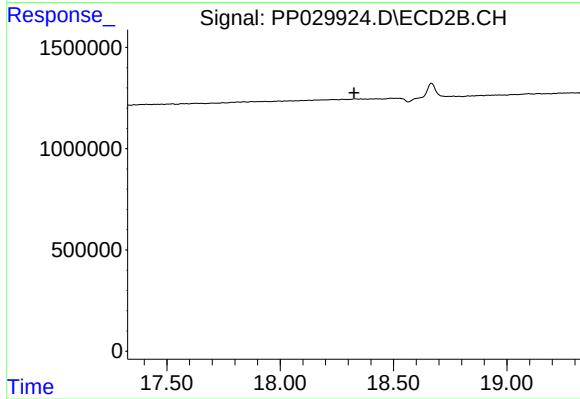

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.326 min
Response: 0
Conc: N.D.