

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041724\
 Data File : PP064398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2024 16:26
 Operator : YP\AJ
 Sample : P2148-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SOM-24-37

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/18/2024
 Supervised By :Ankita Jodhani 04/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 03:36:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 18 03:05:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.639	50876271	45735612	11.160m	14.334m#
2) SA Decachlor...	10.340	8.661	54892222	42754728	17.745	14.814

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041724\
Data File : PP064398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2024 16:26
Operator : YP\AJ
Sample : P2148-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SOM-24-37


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/18/2024
Supervised By :Ankita Jodhani 04/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 03:36:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041624.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 18 03:05:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

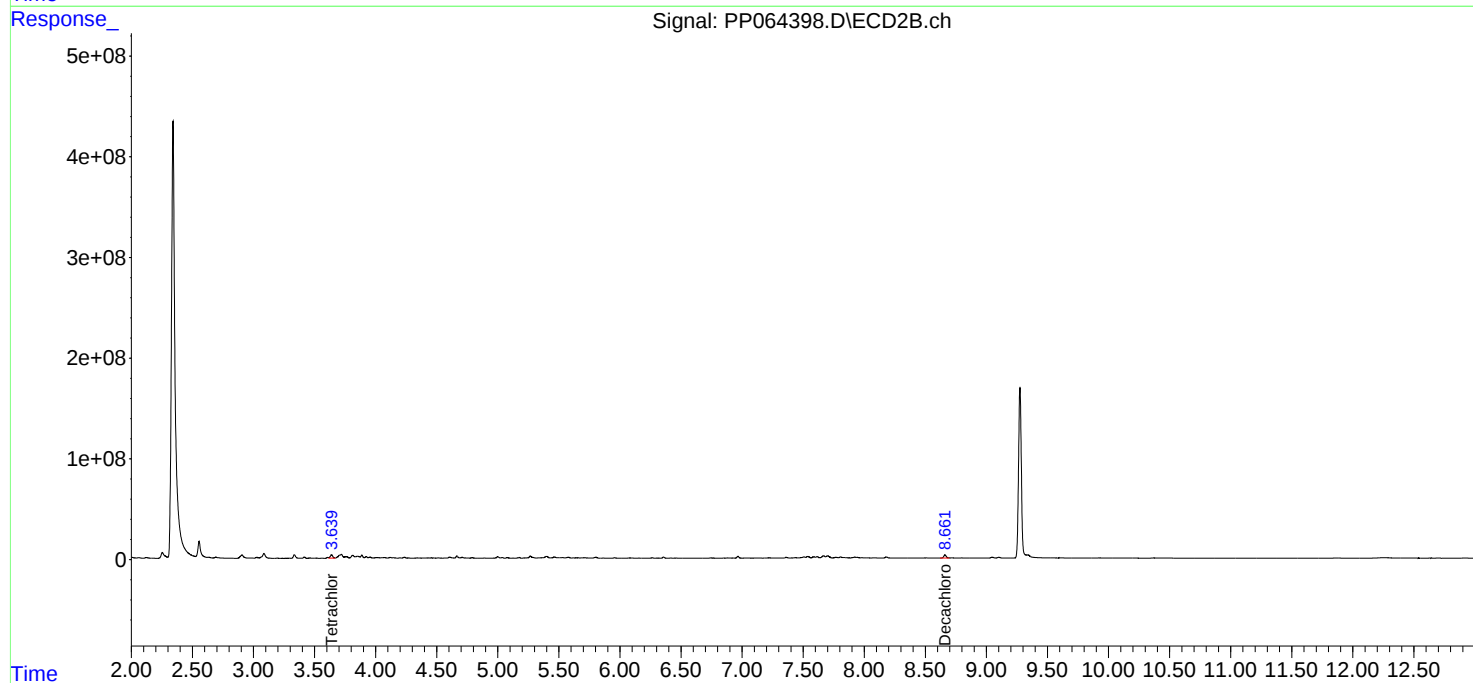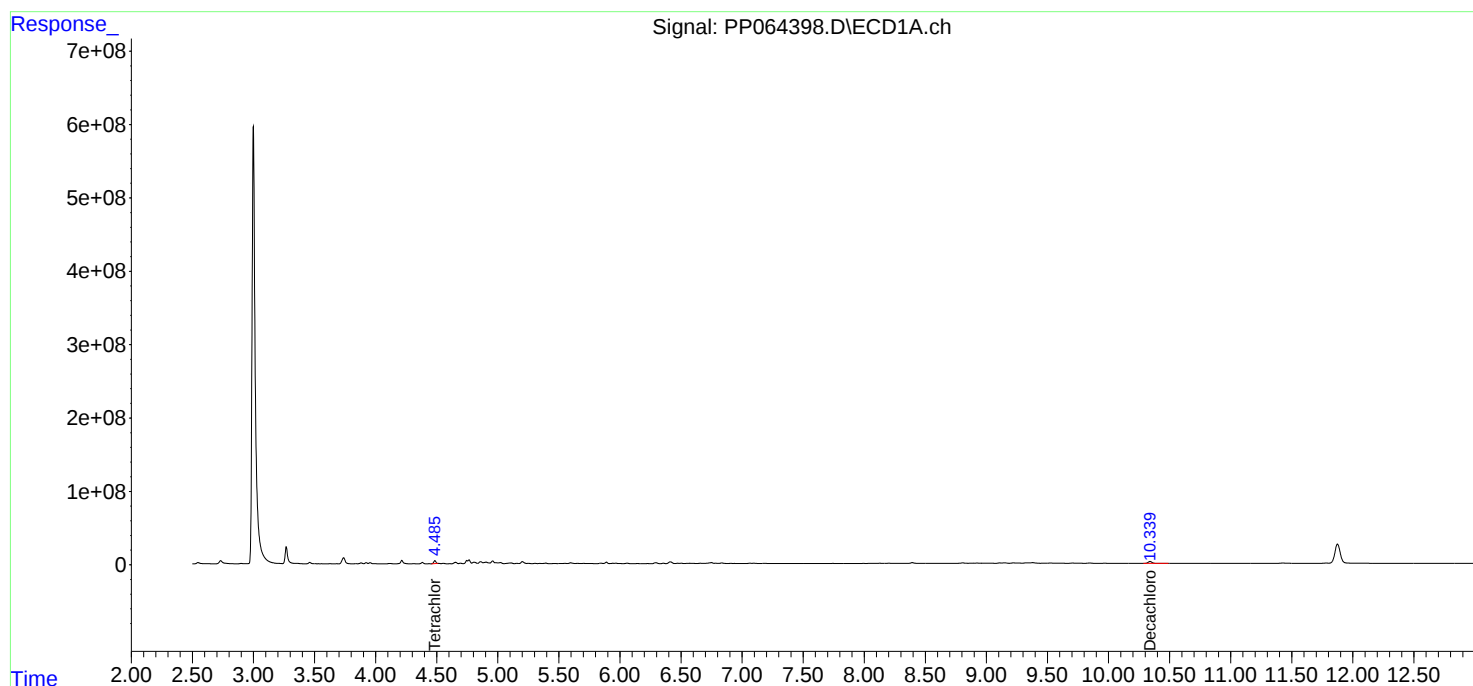

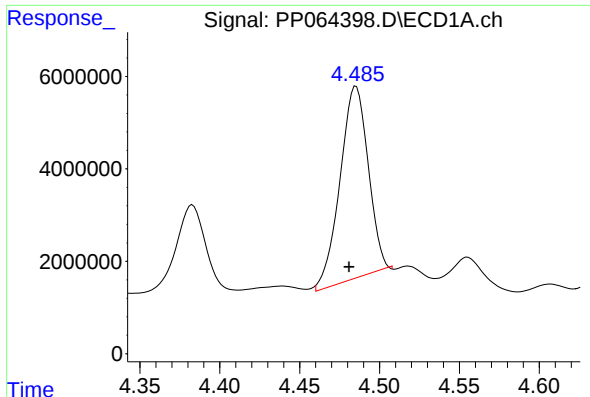


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: 0.004 min
Response: 50876271
Conc: 11.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
SOM-24-37


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/18/2024
Supervised By :Ankita Jodhani 04/18/2024

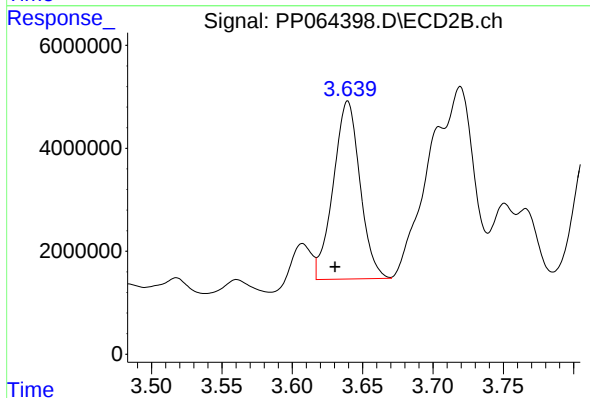


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: 0.009 min
Response: 45735612
Conc: 14.33 ng/ml m

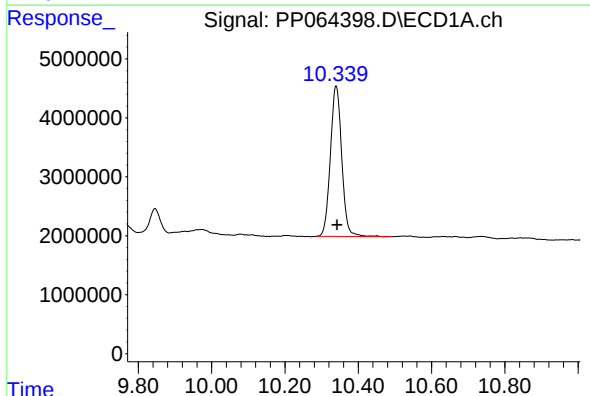

#2 Decachlorobiphenyl

R.T.: 10.340 min
Delta R.T.: -0.002 min
Response: 54892222
Conc: 17.74 ng/ml

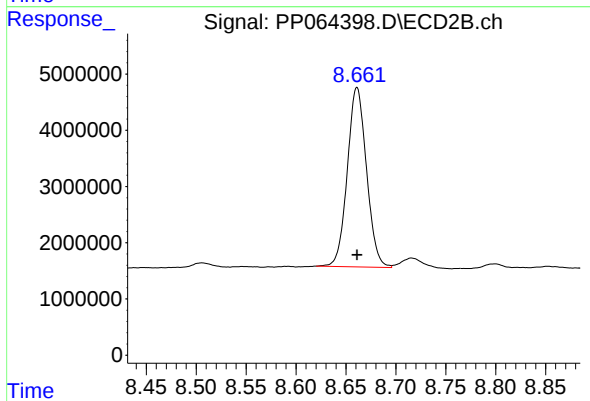

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: 0.000 min
Response: 42754728
Conc: 14.81 ng/ml