

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041725\
 Data File : PP071319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2025 19:04
 Operator : YP\AJ
 Sample : Q1819-06 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC136902-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/18/2025
 Supervised By :mohammad ahmed 04/22/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 02:27:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.507	3.813	2783839	1959680	1.905m	1.890
2) SA Decachlor...	10.234	8.851	2903509	1738813	2.758m	2.206

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041725\
Data File : PP071319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2025 19:04
Operator : YP\AJ
Sample : Q1819-06 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC136902-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/18/2025
Supervised By :mohammad ahmed 04/22/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 02:27:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

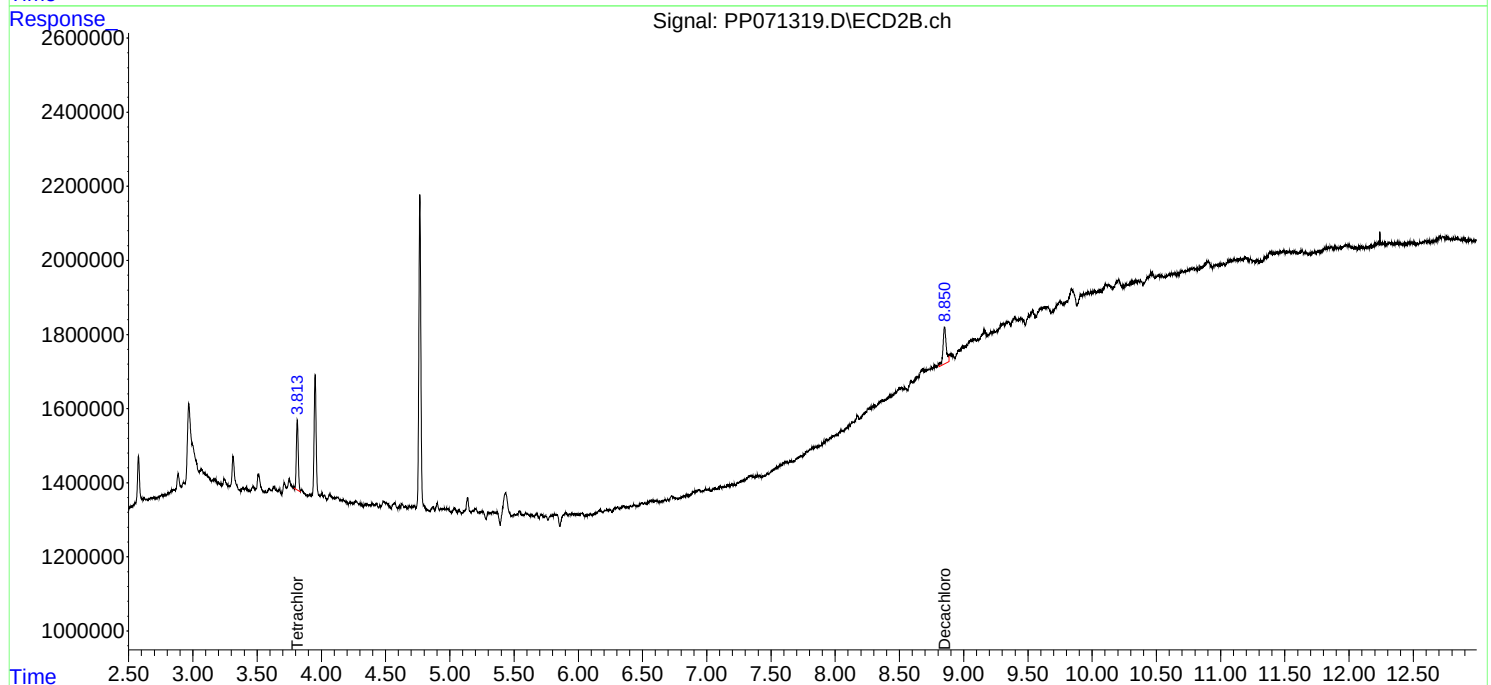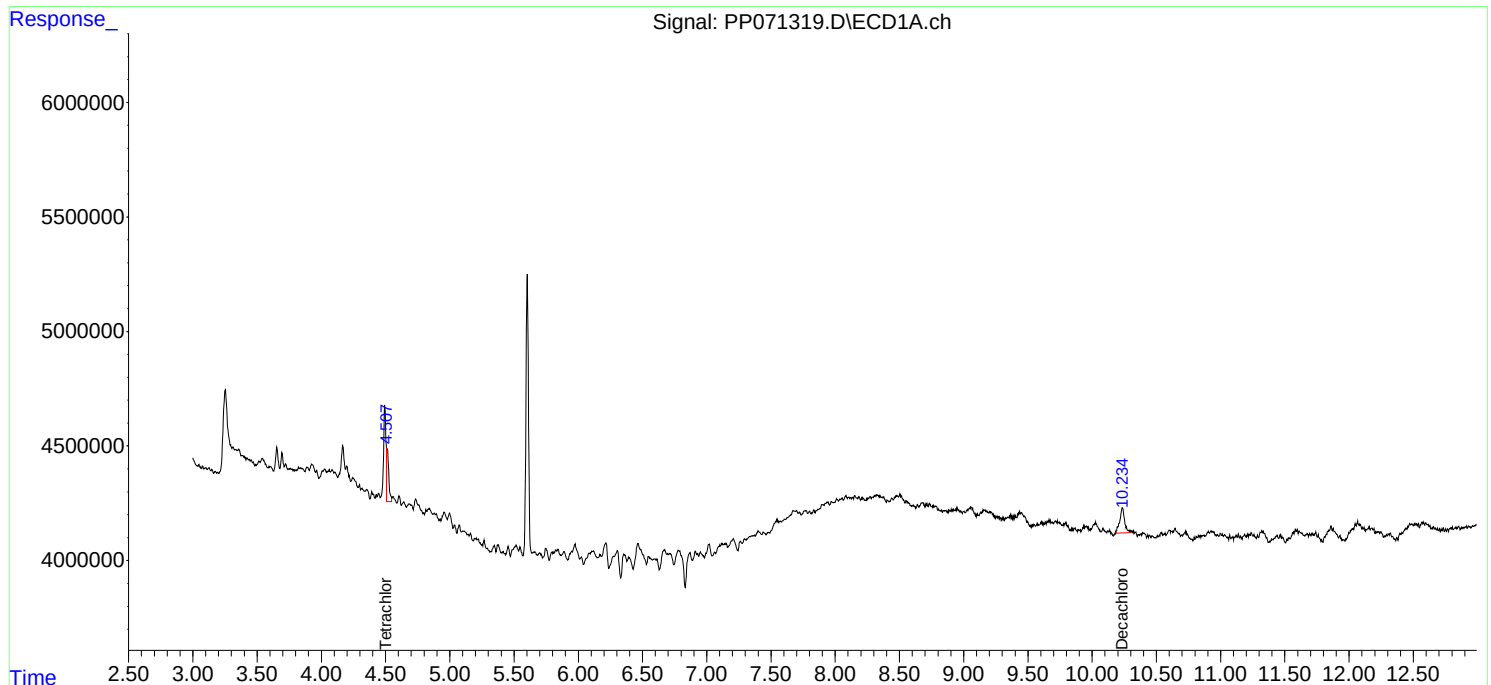

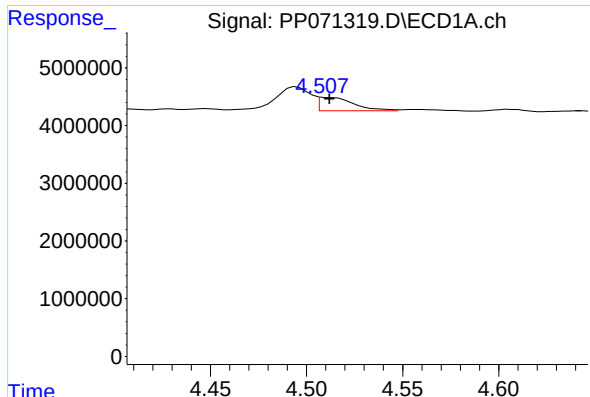

#1 Tetrachloro-m-xylene

R.T.: 4.507 min
Delta R.T.: -0.005 min
Response: 2783839
Conc: 1.90 ng/ml

Instrument :

ECD_P

ClientSampleId :


BC136902-1-2

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 04/18/2025

Supervised By :mohammad ahmed 04/22/2025

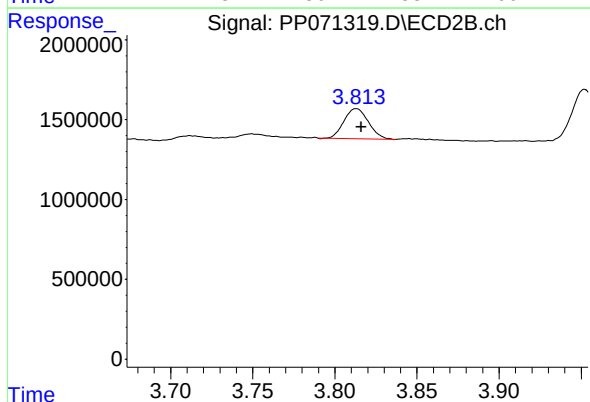


#1 Tetrachloro-m-xylene

R.T.: 3.813 min
Delta R.T.: -0.003 min
Response: 1959680
Conc: 1.89 ng/ml

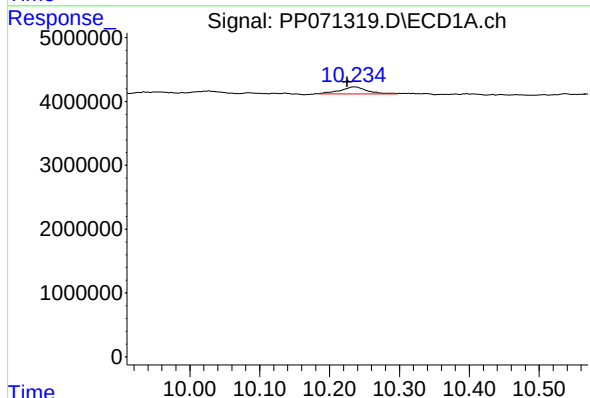

#2 Decachlorobiphenyl

R.T.: 10.234 min
Delta R.T.: 0.009 min
Response: 2903509
Conc: 2.76 ng/ml m

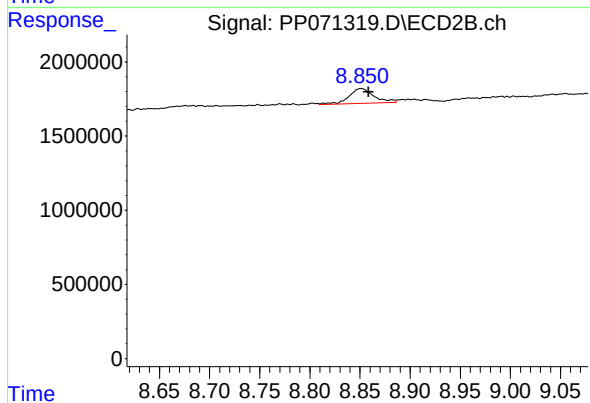

#2 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: -0.008 min
Response: 1738813
Conc: 2.21 ng/ml